


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG022118\
 Data File : BG032754.D
 Acq On : 21 Feb 2018 10:17
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 21 15:45:53 2018

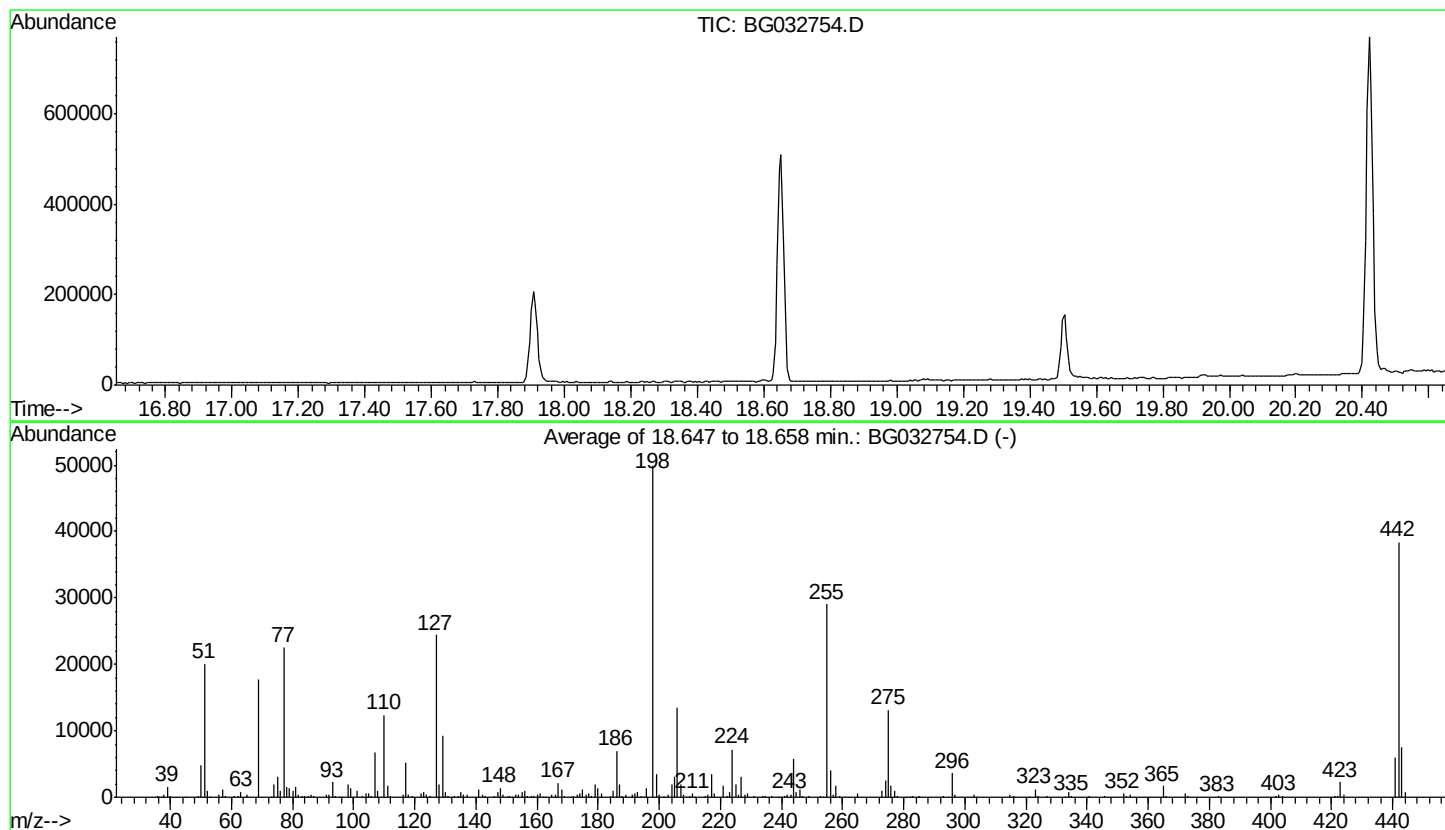

AutoFind: Scans 2614, 2615, 2616; Background Corrected with Scan 2607

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	20139	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.5	17713	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	24434	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49922	PASS
199	198	5	9	6.8	3383	PASS
275	198	10	60	26.3	13114	PASS
365	198	1	100	3.3	1663	PASS
441	442	0.01	24	15.7	6028	PASS
442	198	50	100	76.8	38352	PASS
443	442	15	24	19.8	7611	PASS