
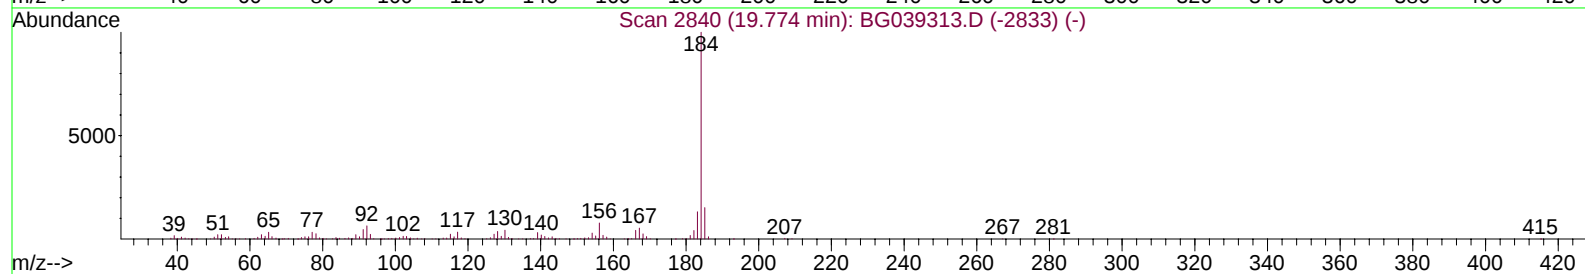
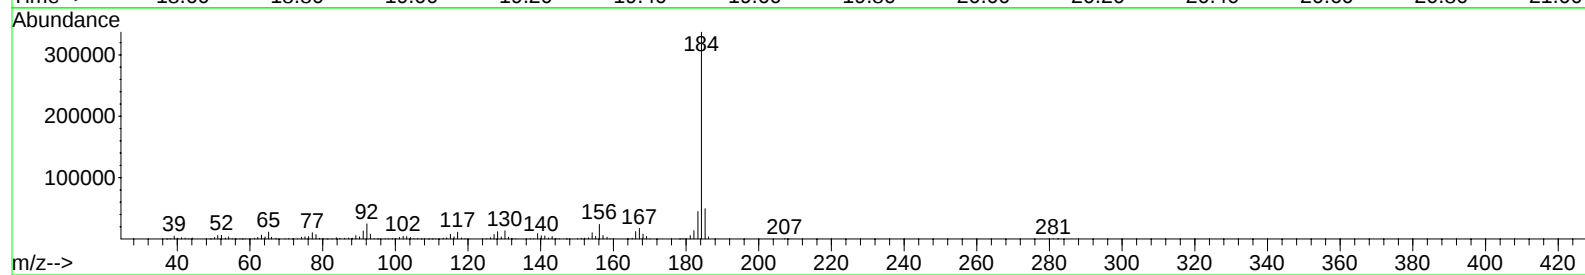


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022119\
 Data File : BG039571.D
 Acq On : 21 Feb 2019 12:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:57:16 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

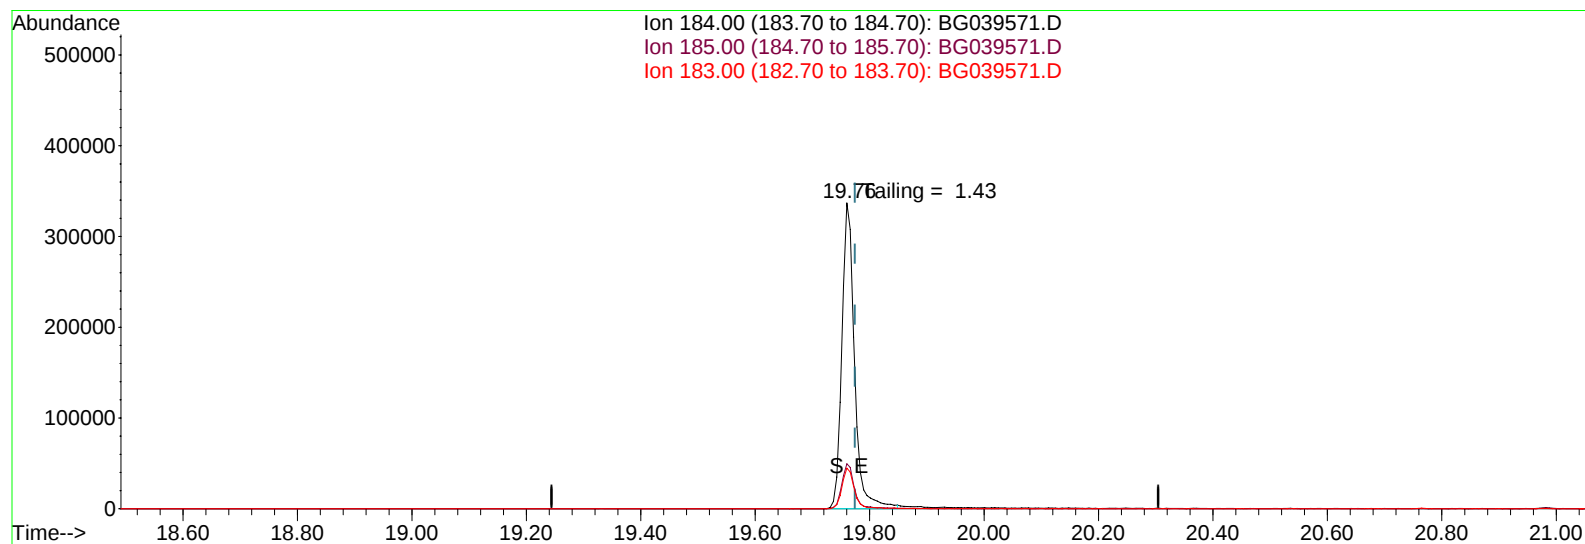

TIC: BG039571.D

(77) Benzidine




19.760min (-0.014) 281170.81ng

response 525446

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.71
183.00	13.20	13.31
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022119\
Data File : BG039571.D
Acq On : 21 Feb 2019 12:32
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 17:57:16 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

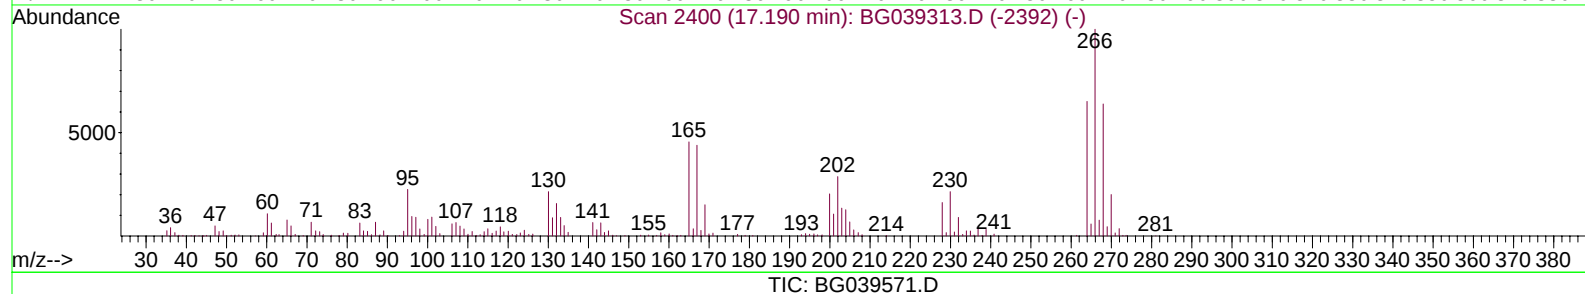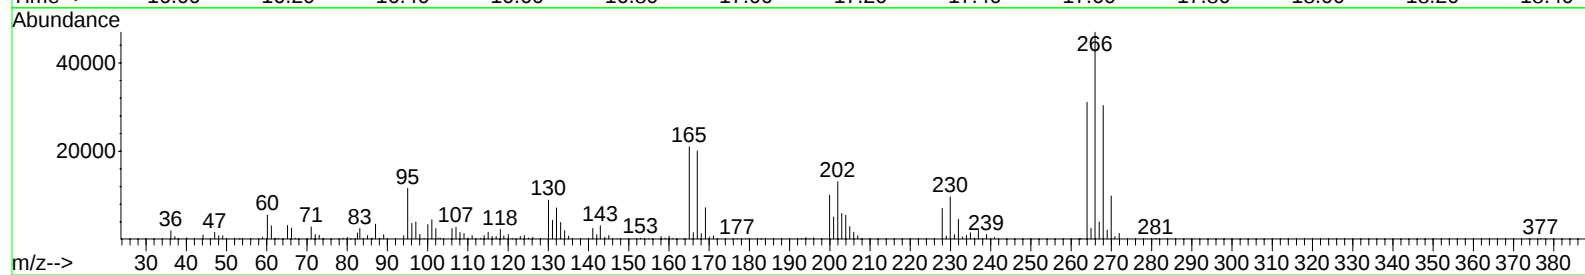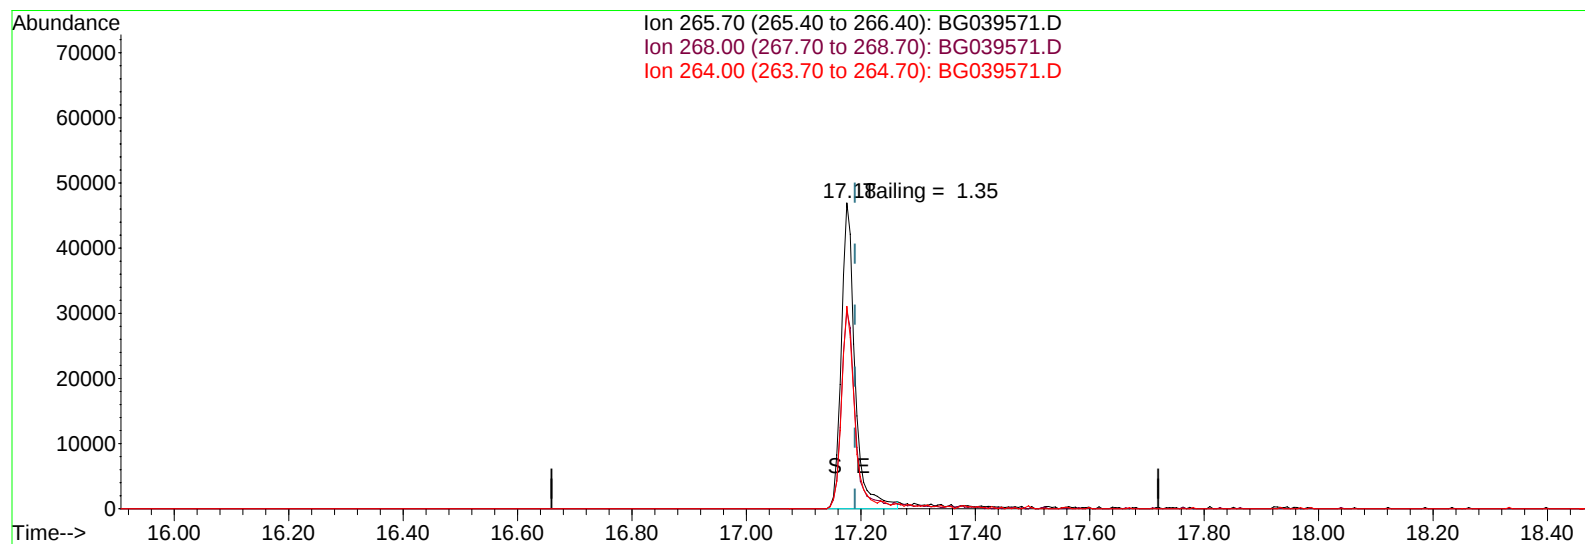

(70) Pentachlorophenol (C)

17.176min (-0.014) 29392.76ng

response 79128

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.68
264.00	65.10	66.18
0.00	0.00	0.00