


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022119\
 Data File : BG039571.D
 Acq On : 21 Feb 2019 12:32
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

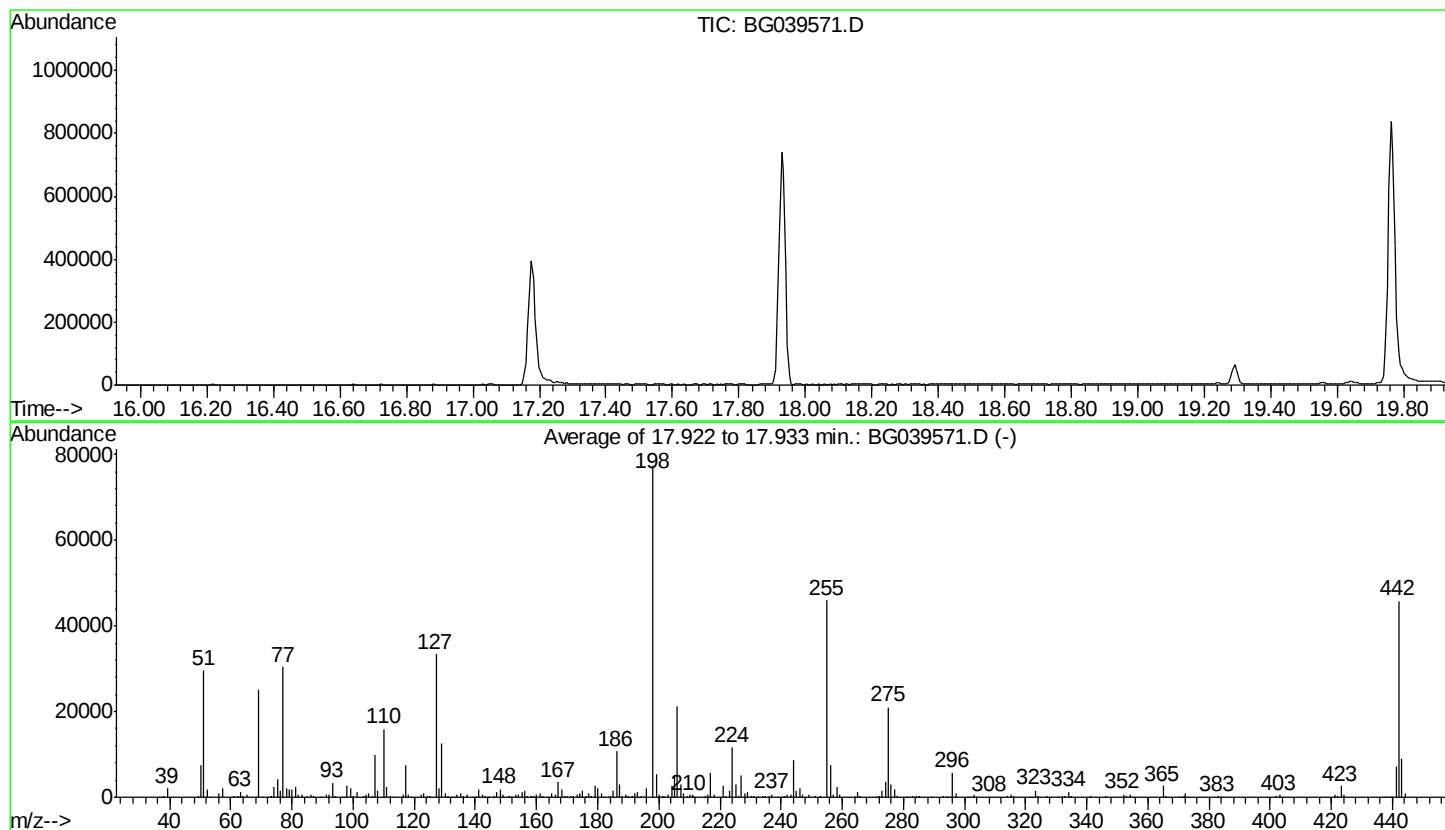

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2519

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.1	29474	PASS
68	69	0.00	2	0.6	139	PASS
69	198	0.00	100	32.5	25177	PASS
70	69	0.00	2	0.5	124	PASS
127	198	10	80	43.1	33365	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77418	PASS
199	198	5	9	7.1	5508	PASS
275	198	10	60	27.0	20920	PASS
365	198	1	100	3.4	2621	PASS
441	198	0.01	100	9.3	7217	PASS
442	198	50	100	59.1	45738	PASS
443	442	15	24	19.9	9084	PASS