
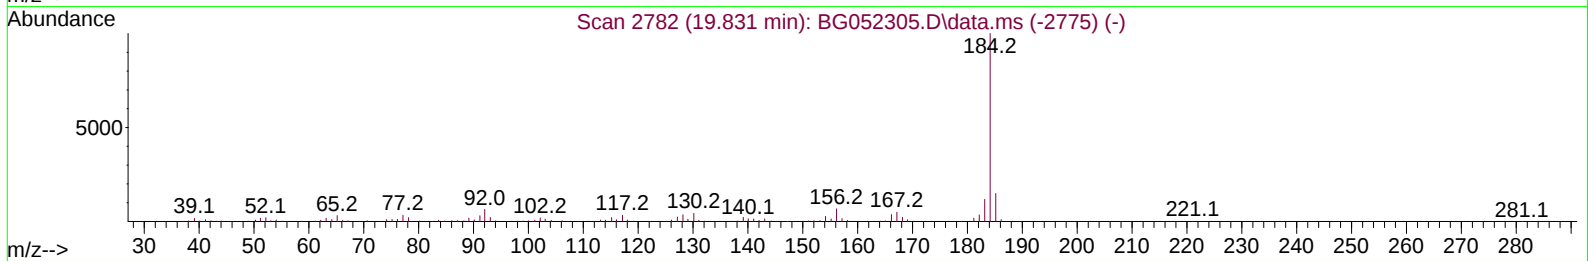
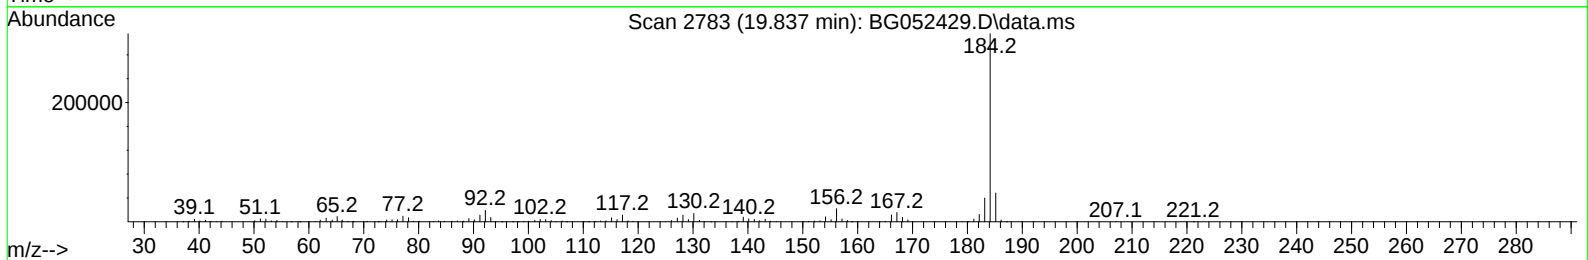


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG022122\  
Data File : BG052429.D  
Acq On : 21 Feb 2022 9:28  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 13:53:04 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG020722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Feb 08 01:21:20 2022  
Response via : Initial Calibration

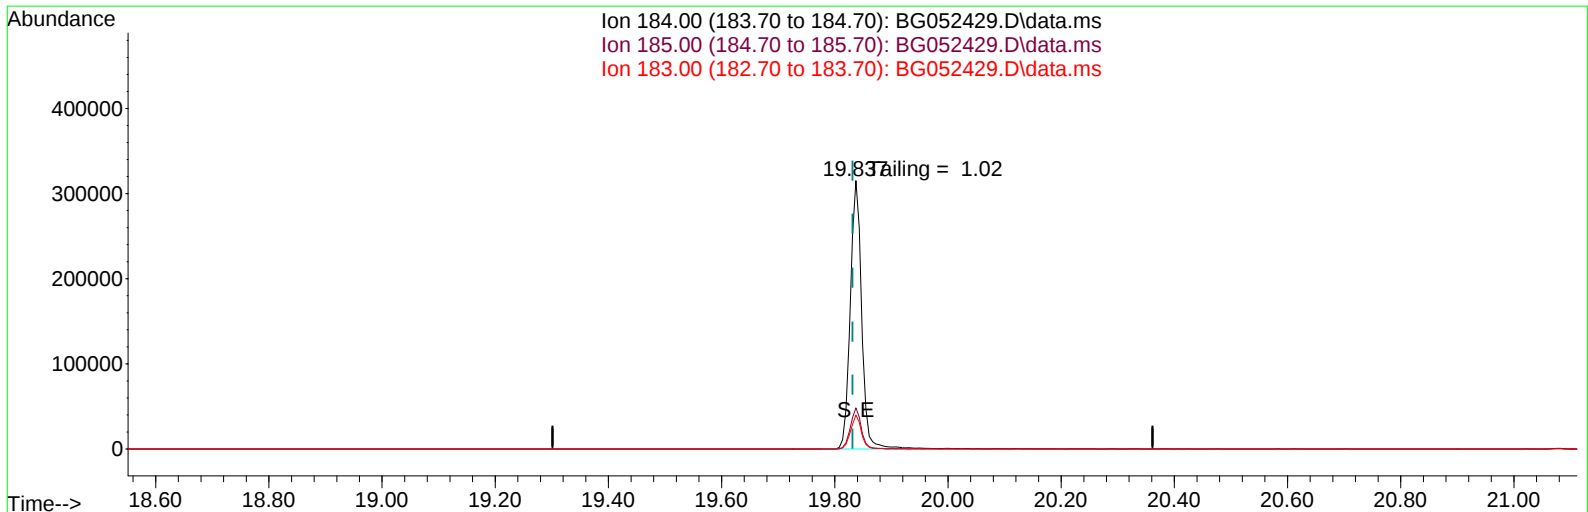

TIC: BG052429.D\data.ms

**(77) Benzidine****19.837min (+ 0.006) 44004.87 ng****response 441934**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 15.35  |
| 183.00 | 12.20  | 12.68  |
| 0.00   | 0.00   | 0.00   |