
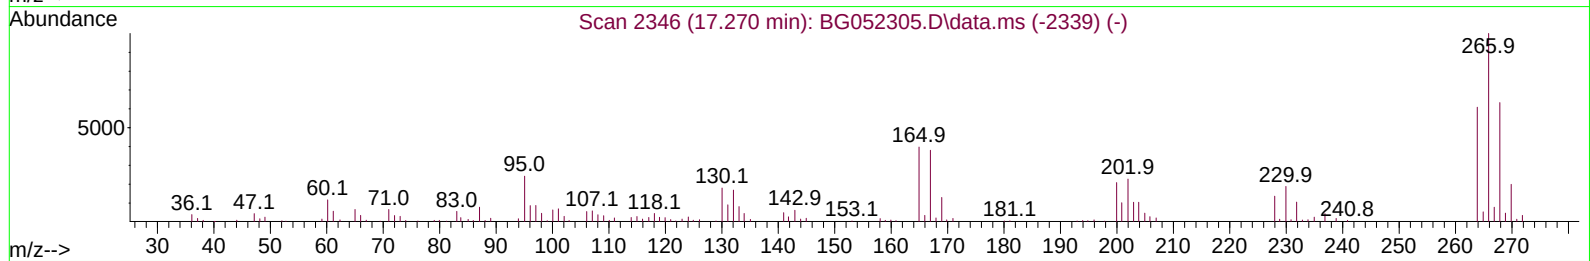
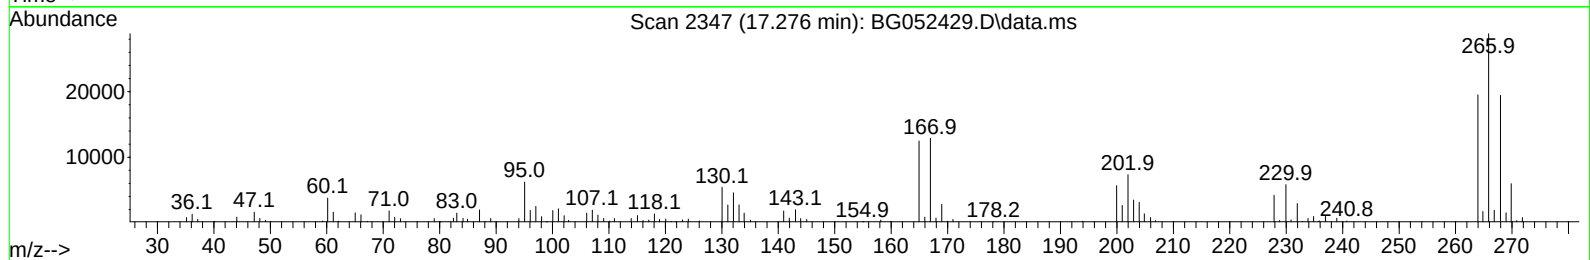


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022122\
Data File : BG052429.D
Acq On : 21 Feb 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 13:53:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

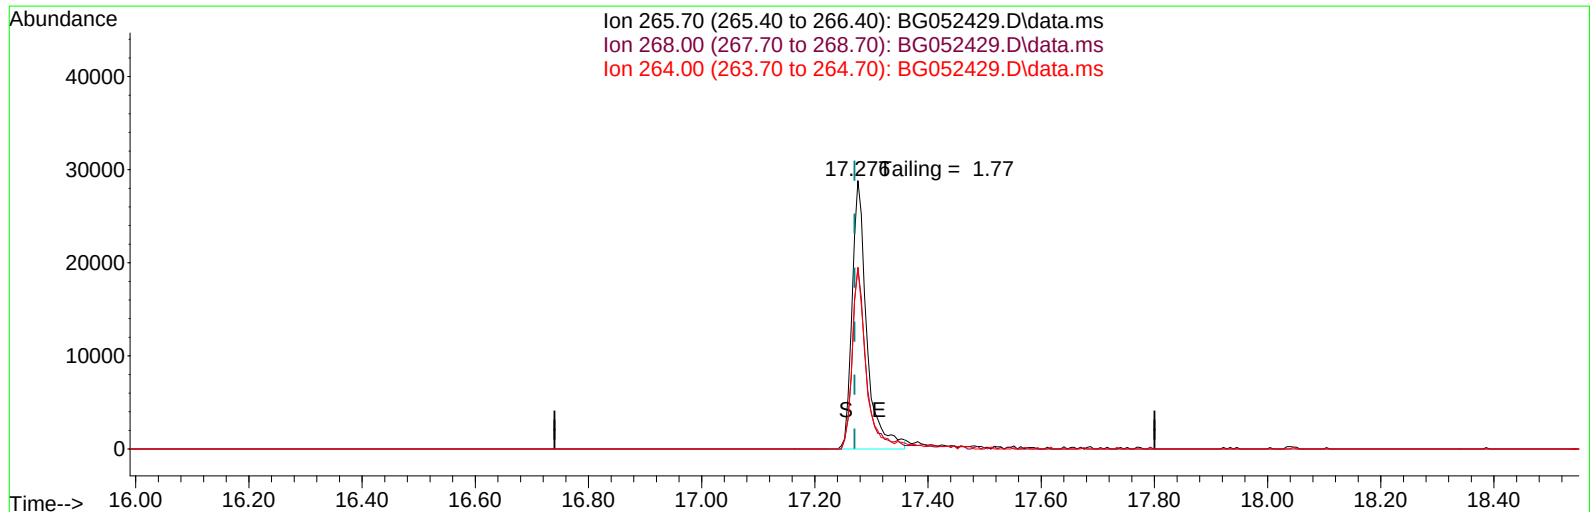

TIC: BG052429.D\data.ms

(70) Pentachlorophenol (C)




17.276min (+ 0.006) 148332.40 ng

response 52644

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	67.44
264.00	65.20	67.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022122\
Data File : BG052429.D
Acq On : 21 Feb 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 21 13:53:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

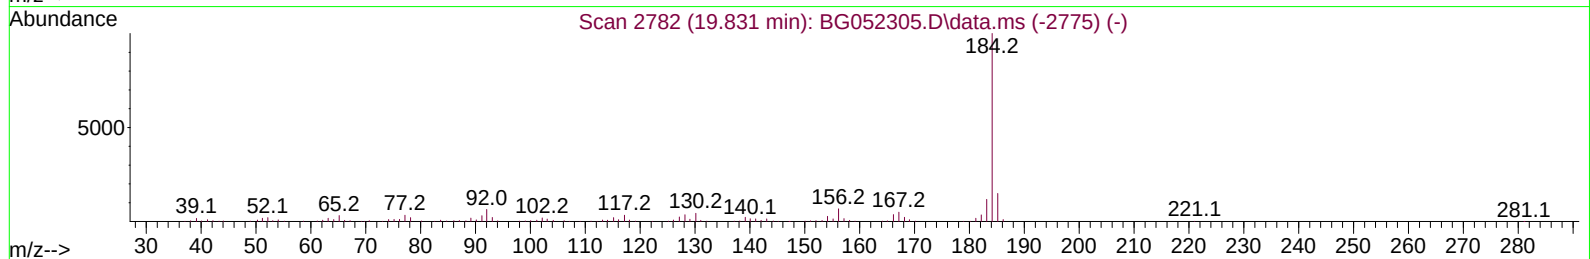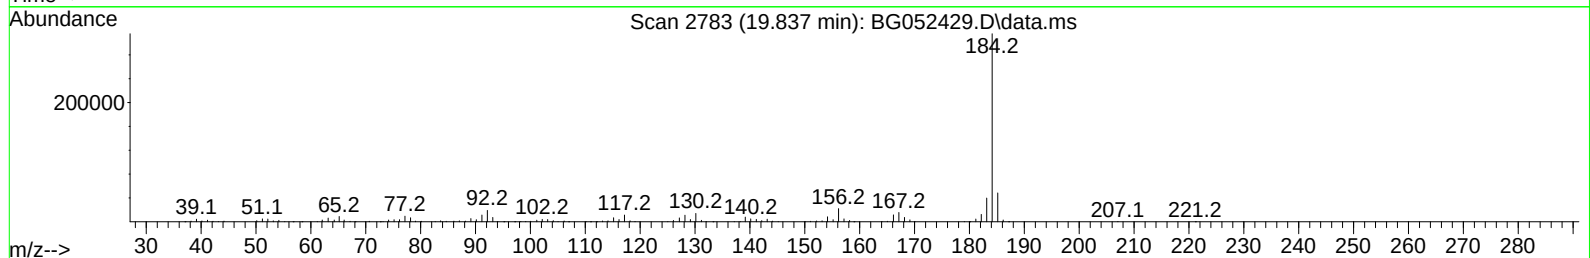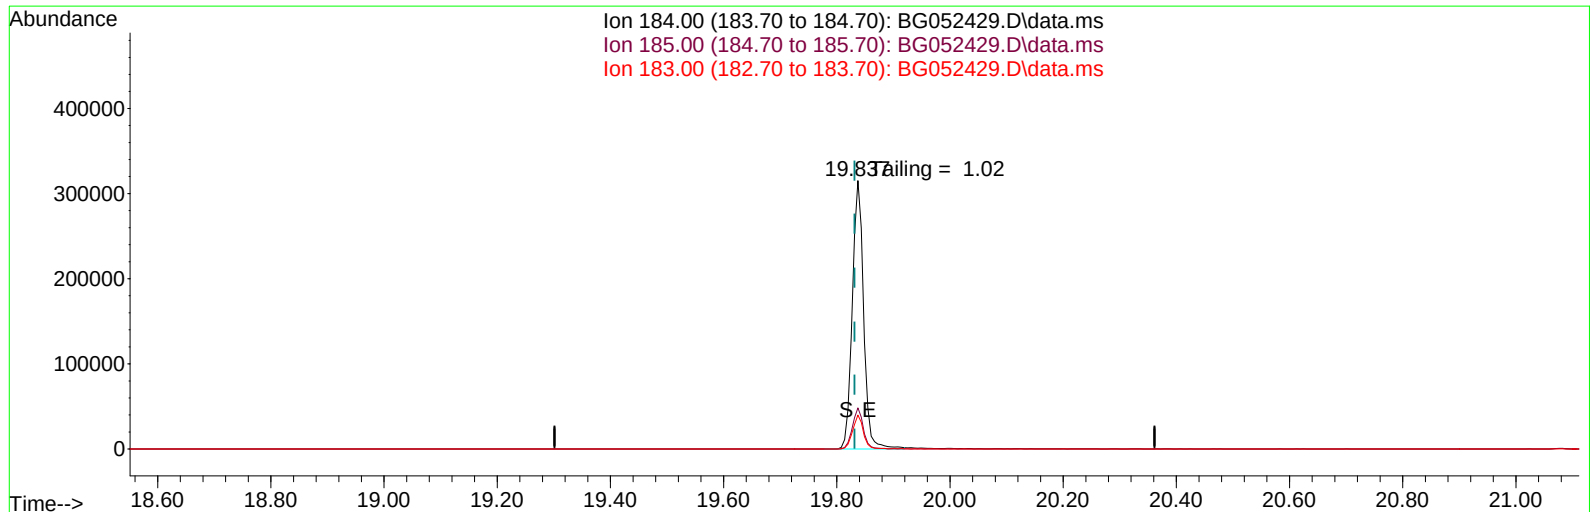

TIC: BG052429.D\data.ms

(77) Benzidine

19.837min (+ 0.006) 44004.87 ng

response 441934

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.35
183.00	12.20	12.68
0.00	0.00	0.00