


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022122\
 Data File : BG052429.D
 Acq On : 21 Feb 2022 9:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Feb 08 01:21:20 2022

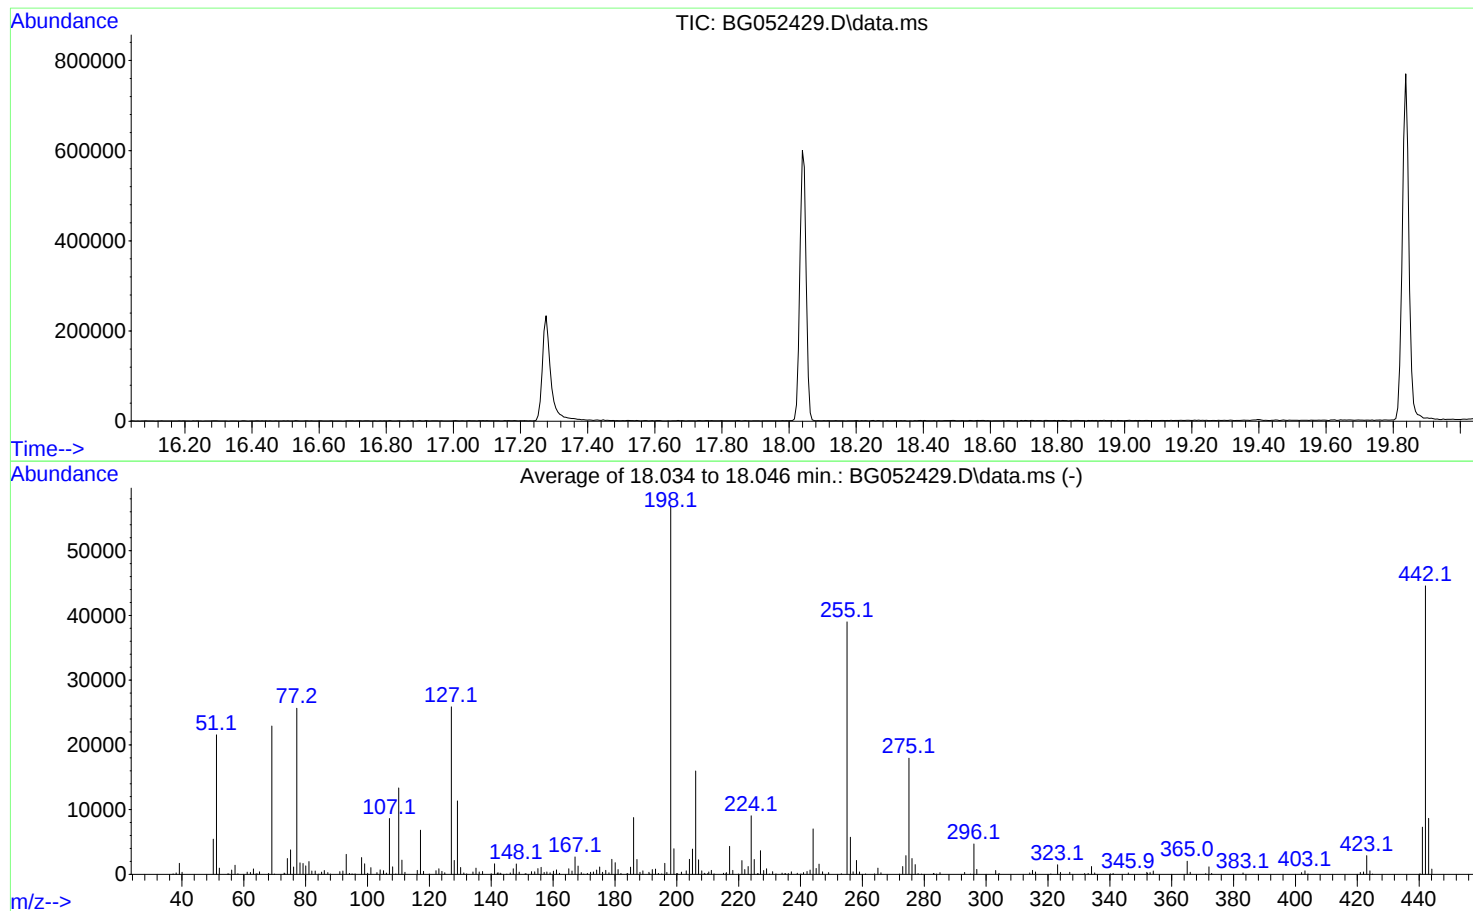




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	21557	PASS
68	69	0.00	2	0.6	143	PASS
69	198	0.00	100	40.3	22920	PASS
70	69	0.00	2	0.3	61	PASS
127	198	10	80	45.6	25883	PASS
197	198	0.00	2	0.5	296	PASS
198	198	100	100	100.0	56819	PASS
199	198	5	9	7.0	3957	PASS
275	198	10	60	31.6	17947	PASS
365	198	1	100	3.6	2038	PASS
441	198	0.01	100	12.8	7298	PASS
442	442	50	100	100.0	44557	PASS
443	442	15	24	19.4	8657	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022122\
Data File : BG052429.D
Acq On : 21 Feb 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 21 13:53:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

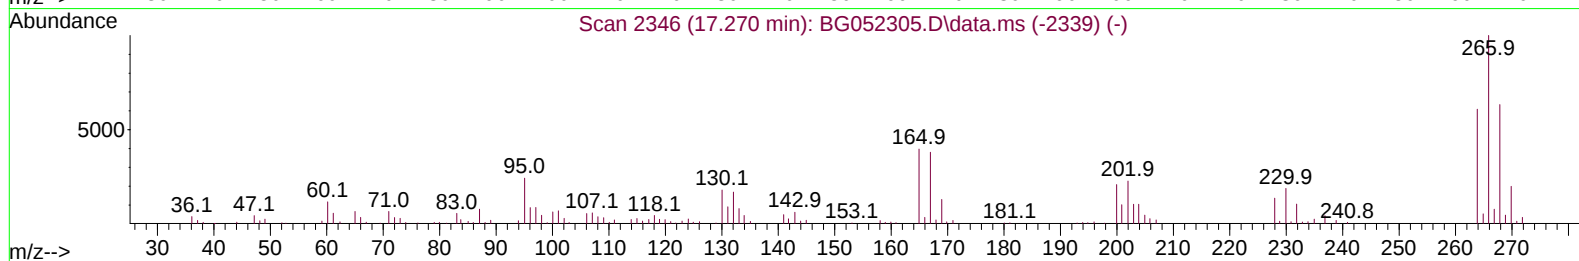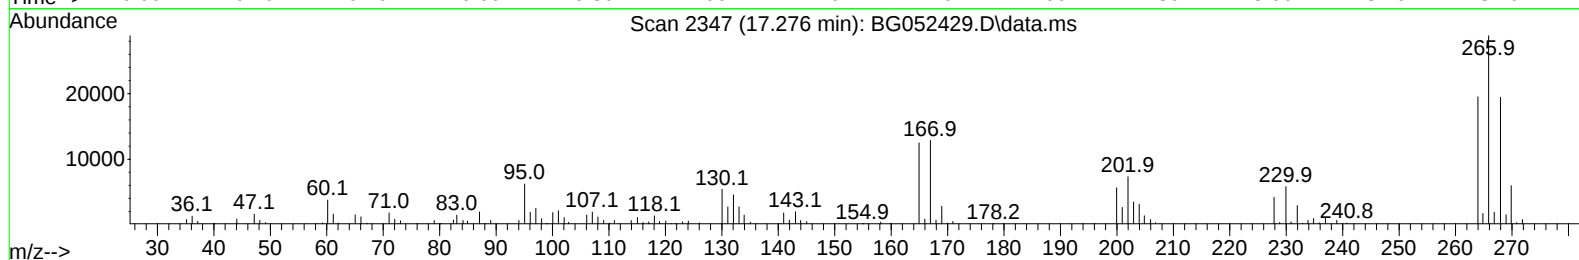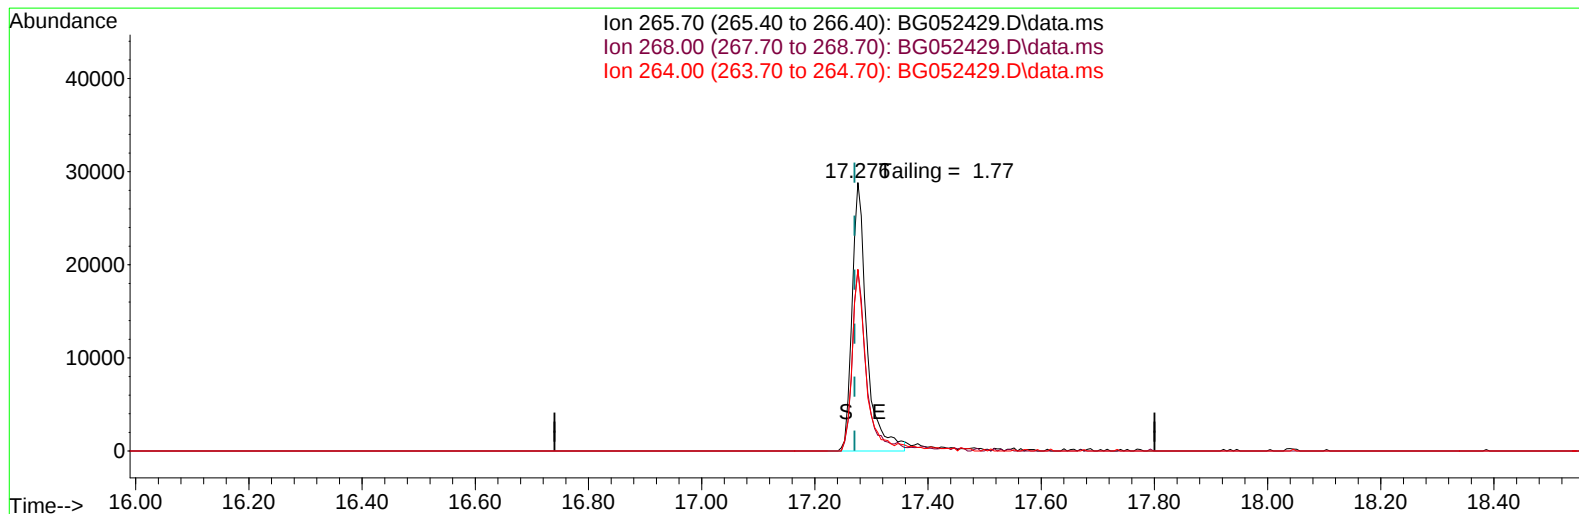

TIC: BG052429.D\data.ms

(70) Pentachlorophenol (C)

17.276min (+ 0.006) 148332.40 ng




response 52644

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	67.44
264.00	65.20	67.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022122\
Data File : BG052429.D
Acq On : 21 Feb 2022 9:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 21 13:53:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG020722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 08 01:21:20 2022
Response via : Initial Calibration

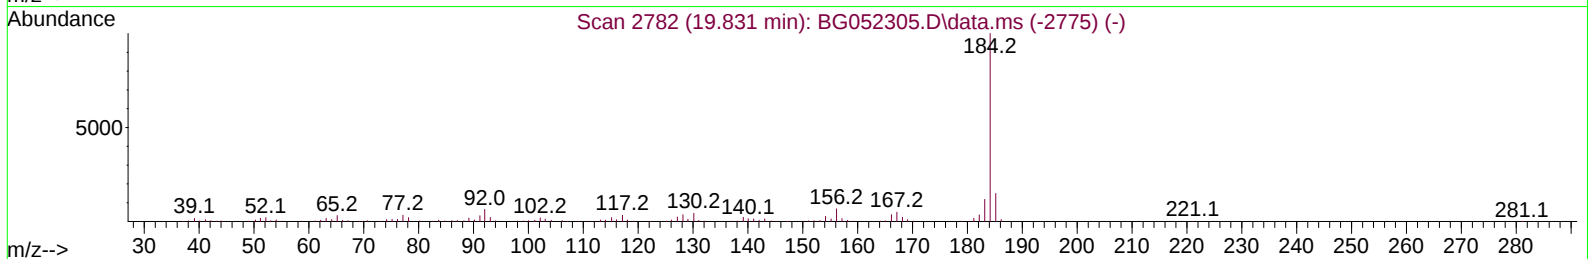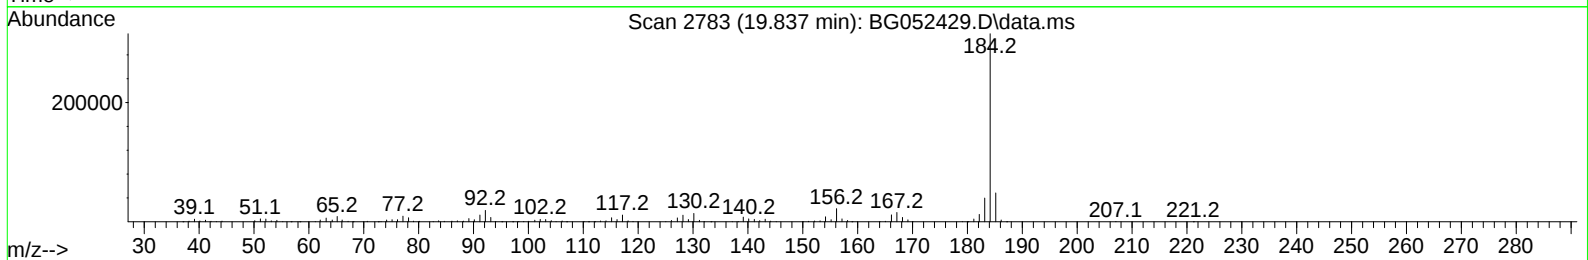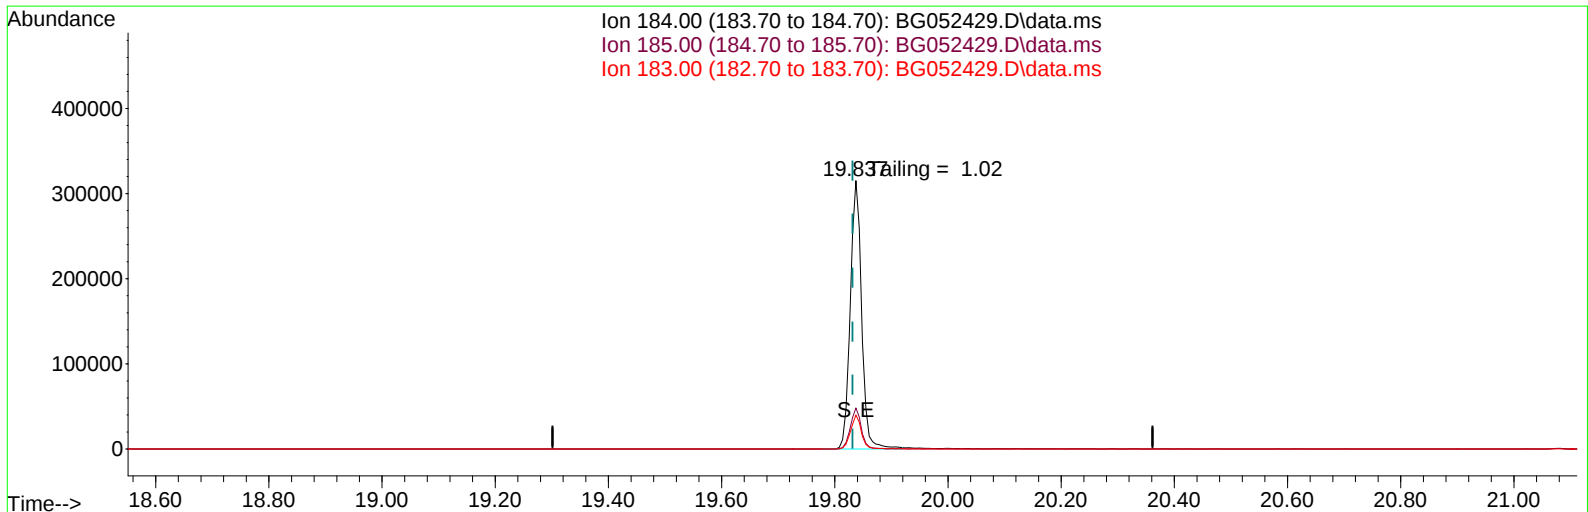

TIC: BG052429.D\data.ms

(77) Benzidine

19.837min (+ 0.006) 44004.87 ng

response 441934

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.35
183.00	12.20	12.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/21/2022	BNA_G	<u>BG052429.D</u>
Compound Name	Response	Retention Time
DDT	228980	21.07
DDD	2984	20.62
DDE	327	20.12
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3311	232291	1.43

Instrument :
BNA_G
ClientSampleId :
DFTPP