
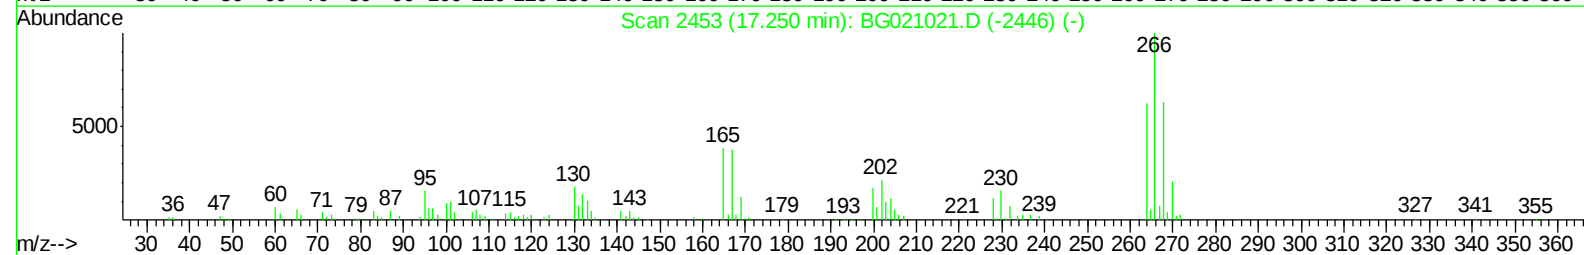
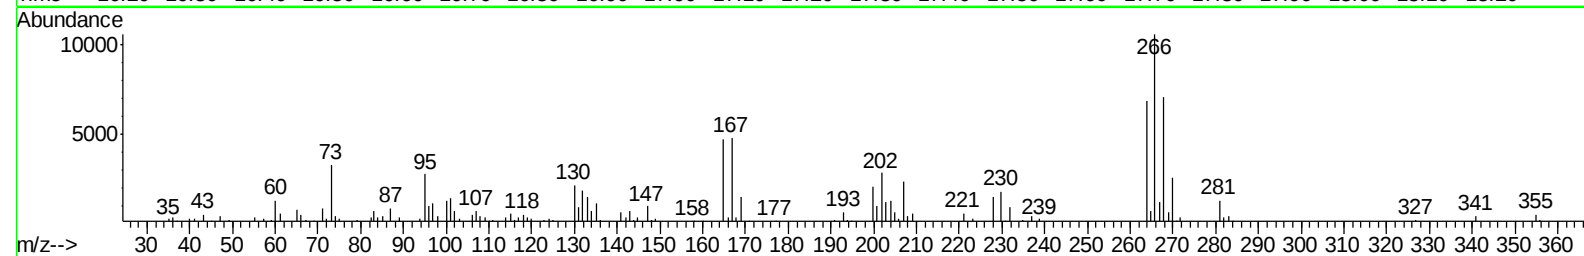


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022216\
Data File : BG021016.D
Acq On : 22 Feb 2016 13:06
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 07:47:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Feb 23 06:17:50 2016
Response via : Initial Calibration

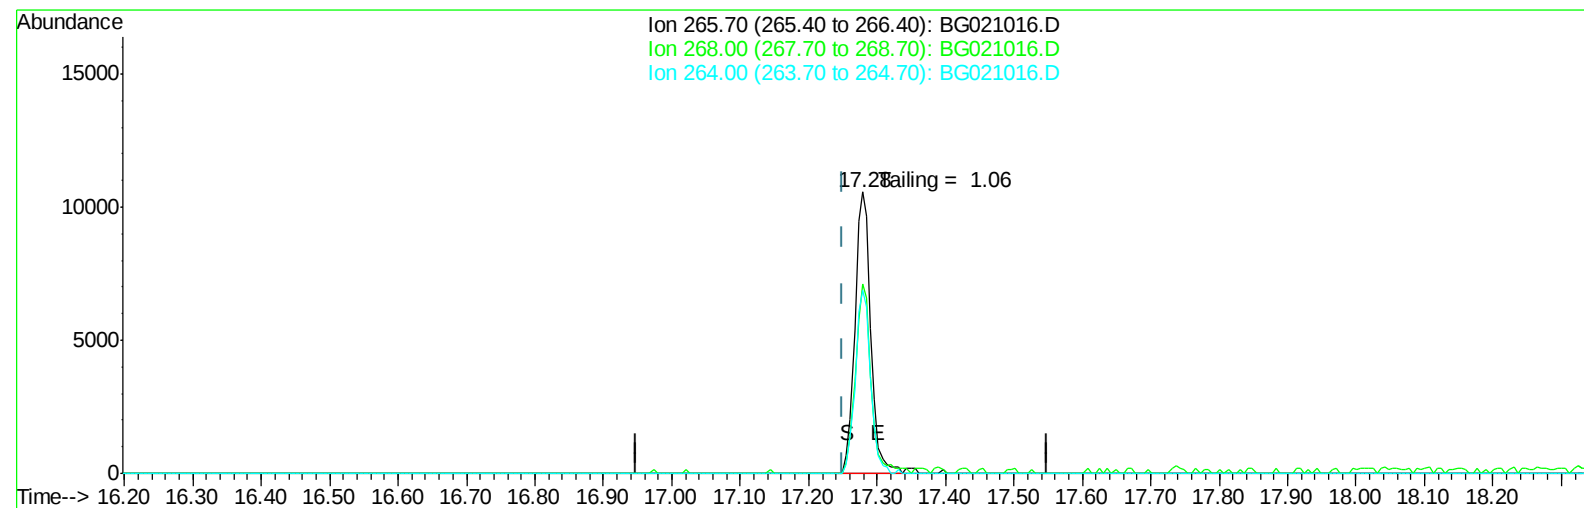

TIC: BG021016.D

(69) Pentachlorophenol (C)




17.279min (+0.029) 0.00ng

response 17128

Ion	Exp%	Act%
265.70	100	100
268.00	62.90	67.26
264.00	62.30	65.20
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG022216\
 Data File : BG021016.D
 Acq On : 22 Feb 2016 13:06
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 07:47:30 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Feb 23 06:17:50 2016
 Response via : Initial Calibration

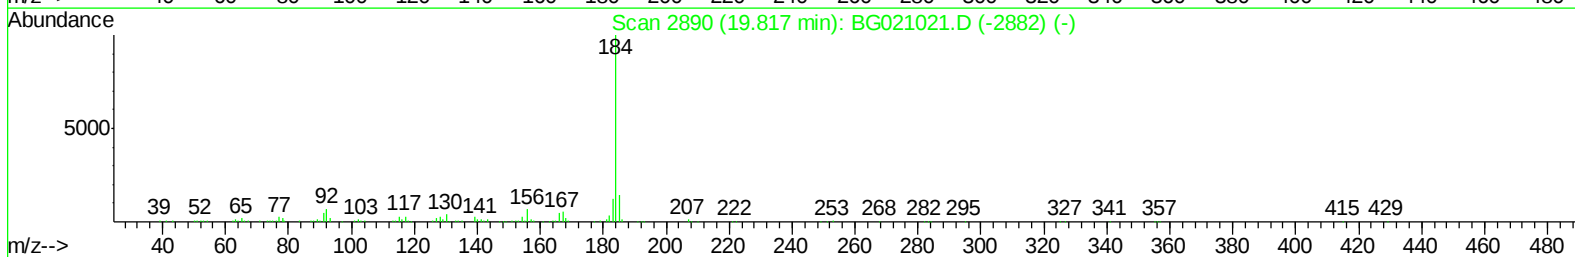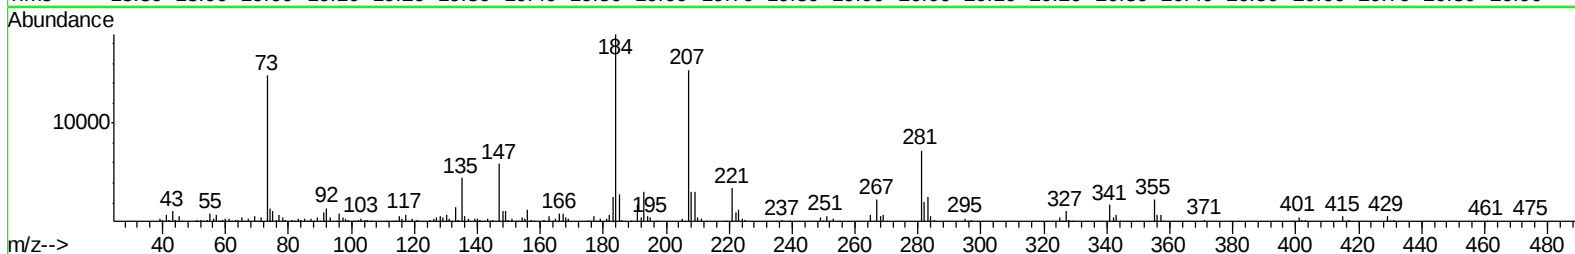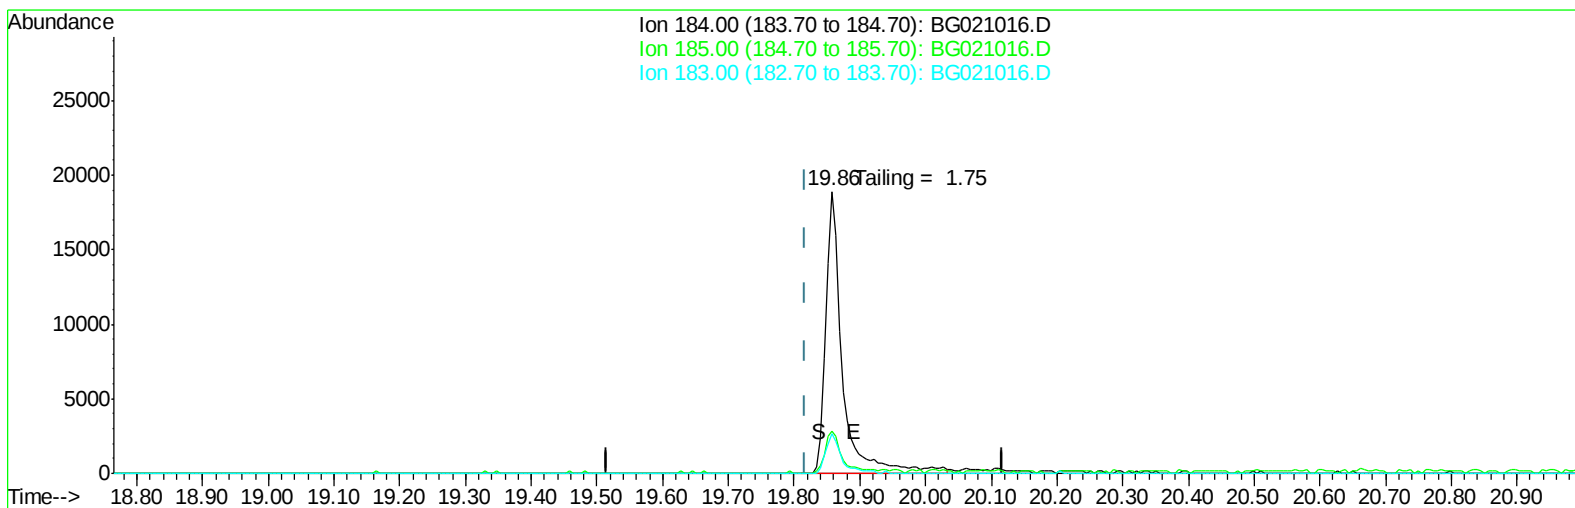

TIC: BG021016.D

(76) Benzidine

19.857min (+0.041) 0.00ng

response 32839

Ion	Exp%	Act%
184.00	100	100
185.00	14.50	14.81
183.00	12.20	13.96
0.00	0.00	0.00