
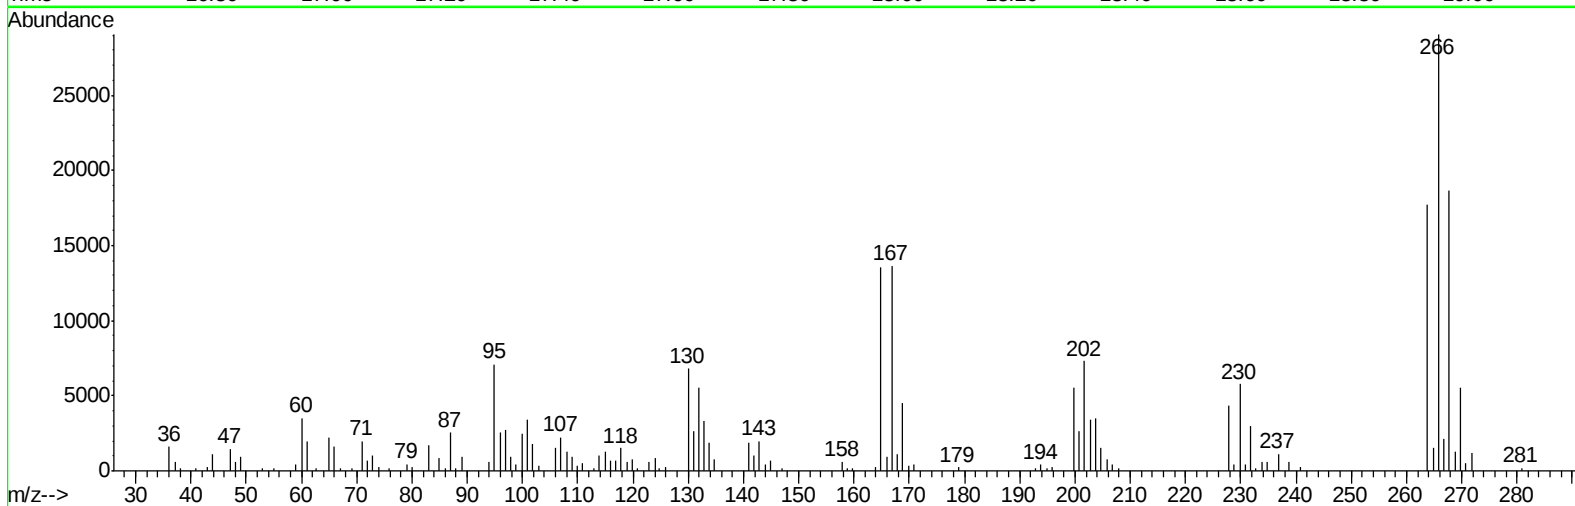


Data Path : Z:\HPCHEM1\BNA G\Data\BG022218\
Data File : BG032780.D
Acq On : 22 Feb 2018 14:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 01:34:56 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 21 15:45:53 2018
Response via : Initial Calibration

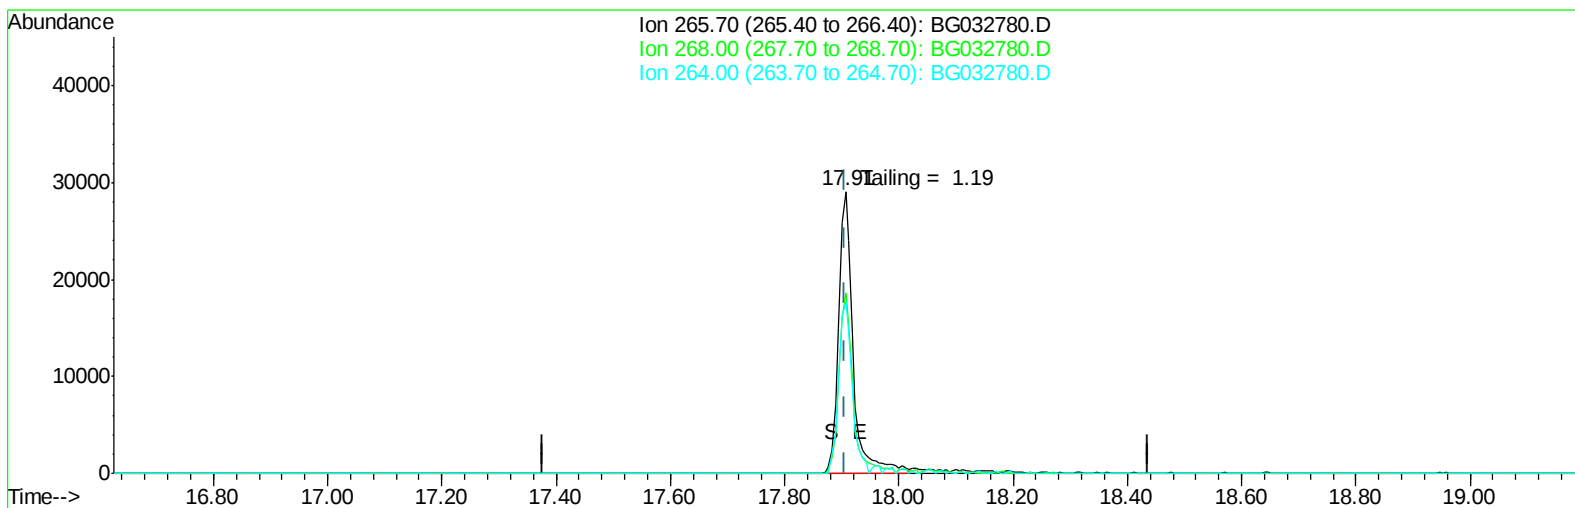

TIC: BG032780.D

(69) Pentachlorophenol (C)



17.906min (-0.000) 22878.65ng

response 51377

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.23
264.00	62.00	60.96
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG022218\
Data File : BG032780.D
Acq On : 22 Feb 2018 14:33
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 23 01:34:56 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 21 15:45:53 2018
Response via : Initial Calibration

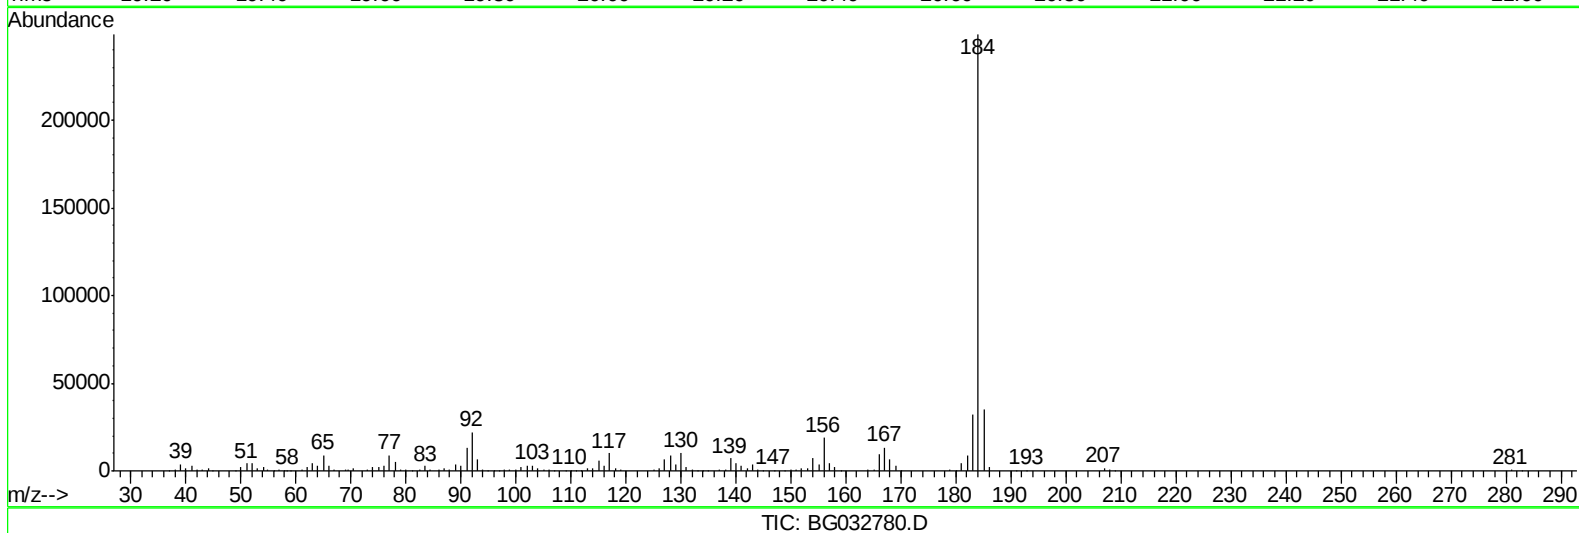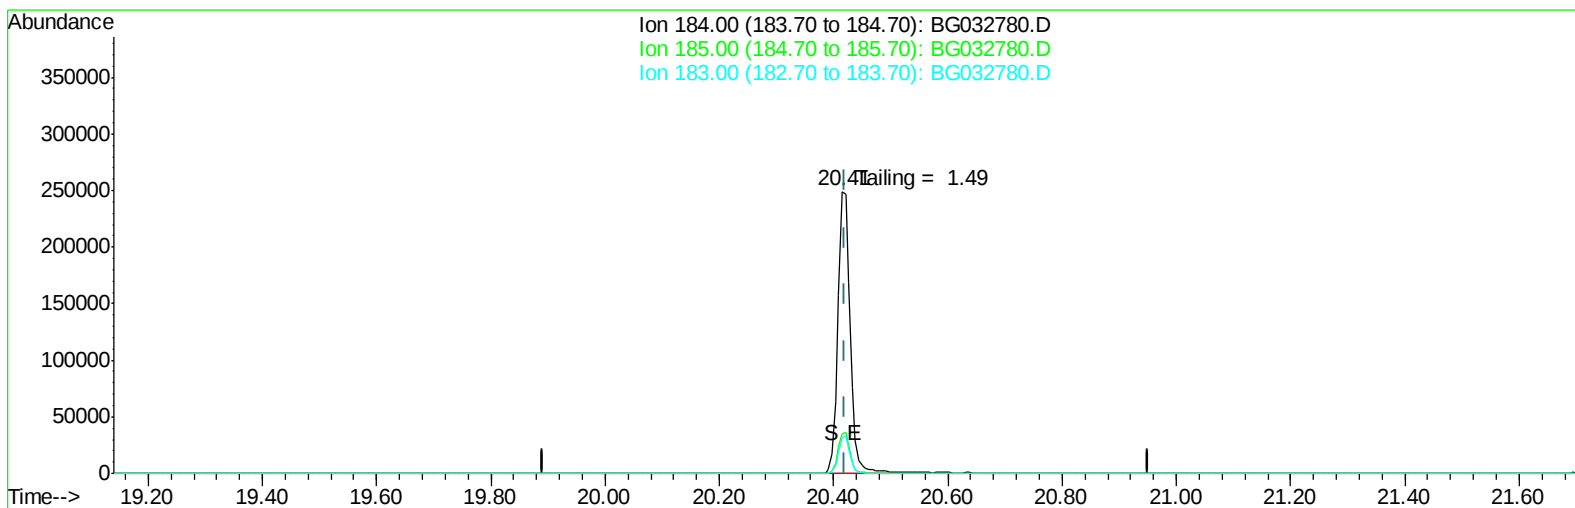

(76) Benzidine

20.415min (-0.006) 0.00ng

response 375978

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	14.07
183.00	13.30	12.91
0.00	0.00	0.00