


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG022218\
 Data File : BG032780.D
 Acq On : 22 Feb 2018 14:33
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 21 15:45:53 2018

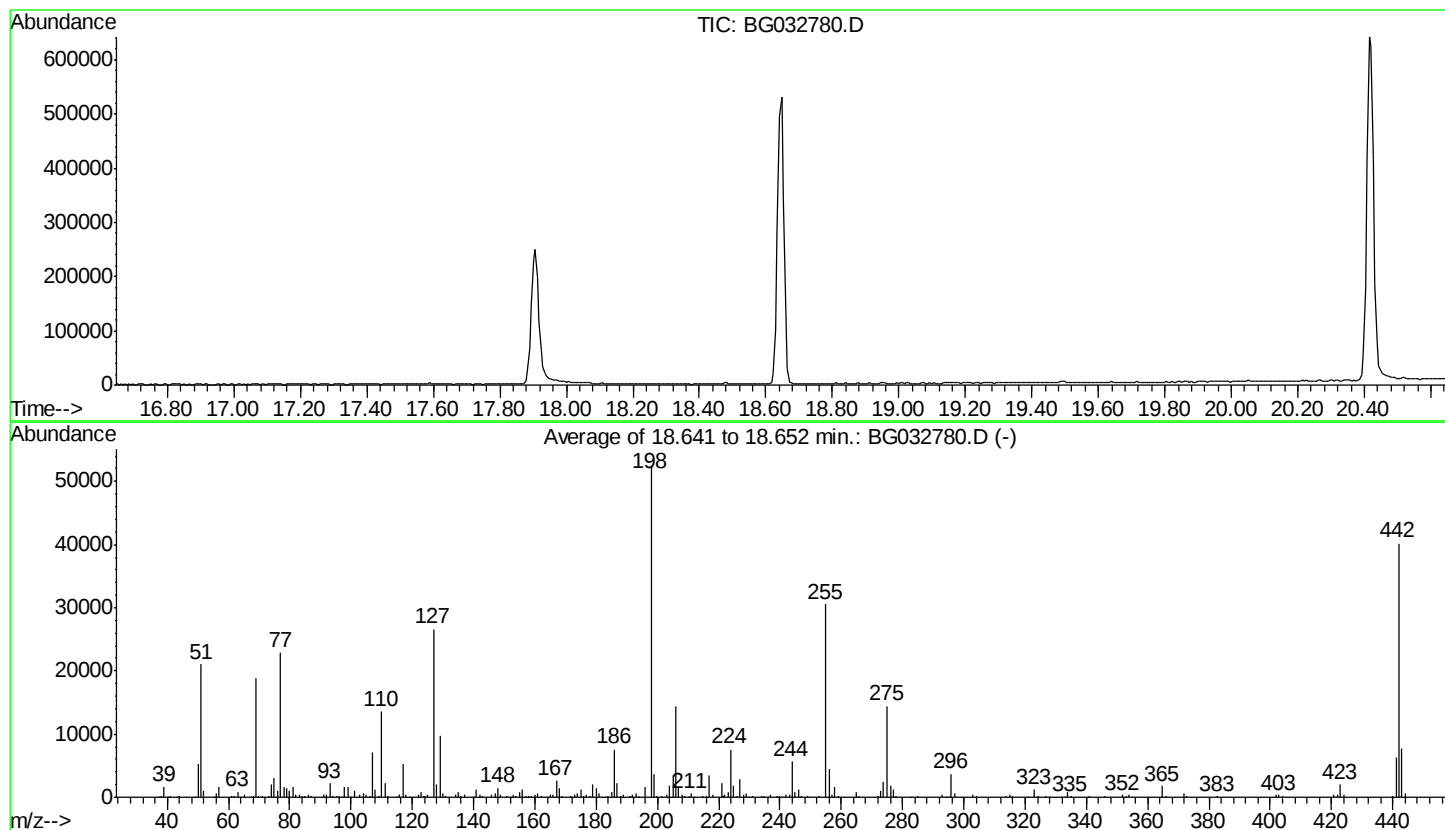

AutoFind: Scans 2613, 2614, 2615; Background Corrected with Scan 2606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.0	21024	PASS
68	69	0.00	2	1.0	182	PASS
69	198	0.00	100	35.8	18808	PASS
70	69	0.00	2	0.8	155	PASS
127	198	10	80	50.7	26610	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52506	PASS
199	198	5	9	7.1	3702	PASS
275	198	10	60	27.4	14401	PASS
365	198	1	100	3.4	1785	PASS
441	442	0.01	24	15.8	6347	PASS
442	198	50	100	76.6	40200	PASS
443	442	15	24	19.0	7645	PASS