

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022221\
 Data File : BG048284.D
 Acq On : 23 Feb 2021 1:30
 Operator : CG/JU
 Sample : M1429-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGS0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.452	15	19	20	rBV3	2576	2953	0.22%	0.026%
2	3.516	25	30	34	rVV	7521	10936	0.81%	0.097%
3	3.593	42	43	47	rBV2	1654	1734	0.13%	0.015%
4	3.669	53	56	58	rVB3	1790	2091	0.16%	0.019%
5	3.722	64	65	69	rVB3	1700	1692	0.13%	0.015%
6	3.863	88	89	93	rVB2	1809	1615	0.12%	0.014%
7	4.269	155	158	165	rVB2	1907	3643	0.27%	0.032%
8	6.795	587	588	593	rVB	1557	1641	0.12%	0.015%
9	6.854	593	598	603	rBV	1094	1998	0.15%	0.018%
10	7.347	676	682	692	rVB	43125	86605	6.42%	0.769%
11	7.447	692	699	708	rBV	116103	207975	15.43%	1.848%
12	7.670	730	737	749	rBV	143609	269982	20.03%	2.399%
13	7.864	767	770	773	rBV	1428	1795	0.13%	0.016%
14	8.117	806	813	824	rBV2	116338	206542	15.32%	1.835%
15	8.775	918	925	926	rVB	1003	1859	0.14%	0.017%
16	8.881	934	943	956	rBV2	120200	222290	16.49%	1.975%
17	9.298	1004	1014	1026	rBV	180936	331104	24.56%	2.942%
18	9.645	1071	1073	1076	rBV	1315	1588	0.12%	0.014%
19	10.021	1129	1137	1148	rVV	170336	315848	23.43%	2.806%
20	10.591	1226	1234	1244	rBV	219138	415659	30.84%	3.693%
21	10.679	1248	1249	1252	rVV3	2296	2230	0.17%	0.020%
22	10.708	1252	1254	1257	rVV2	1528	1805	0.13%	0.016%
23	10.937	1286	1293	1303	rBV	162678	293390	21.77%	2.606%
24	11.102	1315	1321	1329	rVB4	11322	20640	1.53%	0.183%
25	12.518	1558	1562	1566	rBV	2928	4371	0.32%	0.039%
26	12.800	1608	1610	1616	rVB	1064	1690	0.13%	0.015%
27	13.082	1656	1658	1662	rBV	1279	1917	0.14%	0.017%
28	13.252	1684	1687	1692	rVB	1633	2760	0.20%	0.025%
29	13.540	1729	1736	1738	rBV3	3920	6137	0.46%	0.055%
30	13.581	1738	1743	1747	rVB4	3263	5146	0.38%	0.046%
31	13.799	1773	1780	1788	rBV2	10166	16676	1.24%	0.148%
32	13.910	1796	1799	1803	rVB	1486	2033	0.15%	0.018%
33	14.028	1816	1819	1823	rBV	915	1611	0.12%	0.014%
34	14.069	1823	1826	1830	rBV	2195	2460	0.18%	0.022%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022221\
 Data File : BG048284.D
 Acq On : 23 Feb 2021 1:30
 Operator : CG/JU
 Sample : M1429-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGS0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

35	14.157	1834	1841	1846	rBV	420500	635839	47.17%	5.649%
36	14.198	1846	1848	1853	rVB2	14493	18609	1.38%	0.165%
37	14.351	1869	1874	1875	rBV	2067	2386	0.18%	0.021%
38	14.445	1883	1890	1898	rBV	452708	723830	53.70%	6.431%
39	14.562	1907	1910	1914	rVB2	1570	1924	0.14%	0.017%
40	14.603	1914	1917	1921	rBV4	3040	3849	0.29%	0.034%
41	14.750	1935	1942	1953	rVV2	257537	411765	30.55%	3.658%
42	14.897	1964	1967	1968	rVB2	2354	1875	0.14%	0.017%
43	14.915	1968	1970	1972	rVB2	3453	2336	0.17%	0.021%
44	14.932	1972	1973	1975	rBV2	2962	2351	0.17%	0.021%
45	14.974	1978	1980	1982	rBV	2207	2342	0.17%	0.021%
46	15.050	1986	1993	2000	rVV2	48930	91723	6.80%	0.815%
47	15.097	2000	2001	2005	rVV2	3650	4110	0.30%	0.037%
48	15.168	2009	2013	2014	rVV3	2574	3525	0.26%	0.031%
49	15.209	2018	2020	2021	rBV2	2461	2055	0.15%	0.018%
50	15.279	2029	2032	2033	rBV2	2092	1806	0.13%	0.016%
51	15.291	2033	2034	2037	rVB3	2545	1589	0.12%	0.014%
52	15.332	2040	2041	2044	rBV2	2258	2334	0.17%	0.021%
53	15.356	2044	2045	2047	rBV2	1880	1602	0.12%	0.014%
54	15.420	2053	2056	2059	rBV	1793	2592	0.19%	0.023%
55	15.473	2063	2065	2068	rVB3	1663	1723	0.13%	0.015%
56	15.520	2071	2073	2075	rVB2	2123	2146	0.16%	0.019%
57	15.555	2075	2079	2080	rBV3	5366	4524	0.34%	0.040%
58	15.602	2085	2087	2089	rBV3	2966	2599	0.19%	0.023%
59	15.743	2103	2111	2125	rBV	628251	1009007	74.85%	8.964%
60	15.884	2129	2135	2146	rVV	252351	390067	28.94%	3.465%
61	15.978	2146	2151	2155	rVB8	8992	16001	1.19%	0.142%
62	16.119	2173	2175	2176	rBV2	2253	1561	0.12%	0.014%
63	16.172	2181	2184	2185	rBV3	2967	2793	0.21%	0.025%
64	16.249	2193	2197	2198	rBV3	2039	2836	0.21%	0.025%
65	16.301	2204	2206	2210	rBV4	4041	3807	0.28%	0.034%
66	16.343	2210	2213	2214	rBV3	3280	2145	0.16%	0.019%
67	16.419	2225	2226	2229	rVB3	2257	1846	0.14%	0.016%
68	16.513	2241	2242	2243	rBV	4015	2554	0.19%	0.023%
69	16.648	2264	2265	2267	rVV3	3497	2129	0.16%	0.019%
70	16.689	2270	2272	2273	rBV2	2619	1707	0.13%	0.015%
71	16.736	2278	2280	2281	rBV	3329	1674	0.12%	0.015%

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022221\
 Data File : BG048284.D
 Acq On : 23 Feb 2021 1:30
 Operator : CG/JU
 Sample : M1429-08
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBGS0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
 Title : SVOA CALIBRATION

72	16.766	2284	2285	2288	rVB3	3779	2835	0.21%	0.025%
73	16.795	2288	2290	2293	rBV4	2284	3054	0.23%	0.027%
74	16.918	2309	2311	2313	rVB3	2419	2123	0.16%	0.019%
75	16.983	2320	2322	2325	rVB4	2068	2043	0.15%	0.018%
76	17.036	2330	2331	2333	rVV2	3819	2069	0.15%	0.018%
77	17.054	2333	2334	2337	rVB2	2904	2227	0.17%	0.020%
78	17.142	2348	2349	2350	rBV	3962	2044	0.15%	0.018%
79	17.177	2353	2355	2357	rVB3	3517	3138	0.23%	0.028%
80	17.271	2369	2371	2373	rBV3	3298	2018	0.15%	0.018%
81	17.289	2373	2374	2378	rVV4	3101	3348	0.25%	0.030%
82	17.353	2383	2385	2386	rVB2	5572	2589	0.19%	0.023%
83	17.377	2386	2389	2392	rBV5	3956	6355	0.47%	0.056%
84	17.494	2403	2409	2416	rBV	329743	517328	38.38%	4.596%
85	17.594	2420	2426	2438	rVV	765366	1205443	89.43%	10.709%
86	17.841	2466	2468	2470	rVB3	4806	4424	0.33%	0.039%
87	17.905	2477	2479	2480	rVB2	4192	2621	0.19%	0.023%
88	17.923	2480	2482	2484	rBV3	3108	2640	0.20%	0.023%
89	18.005	2494	2496	2500	rBV5	5651	7421	0.55%	0.066%
90	18.093	2509	2511	2512	rBV2	4856	3734	0.28%	0.033%
91	18.235	2534	2535	2538	rBV3	4854	4031	0.30%	0.036%
92	18.334	2550	2552	2555	rBV4	5091	5566	0.41%	0.049%
93	18.528	2583	2585	2589	rBV5	5767	7685	0.57%	0.068%
94	18.722	2616	2618	2620	rBV3	6228	7888	0.59%	0.070%
95	18.822	2633	2635	2637	rBV3	7025	5194	0.39%	0.046%
96	18.893	2645	2647	2648	rVB2	5498	2647	0.20%	0.024%
97	19.880	2809	2815	2822	rBV	907183	1347978	100.00%	11.975%
98	21.777	3133	3138	3146	rVB2	322290	538200	39.93%	4.781%
99	24.856	3654	3662	3673	rVB	459045	1233203	91.49%	10.956%
100	25.091	3695	3702	3713	rVB2	178575	506370	37.57%	4.499%


Sum of corrected areas: 11256193

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022221\
Data File : BG048284.D
Acq On : 23 Feb 2021 1:30
Operator : CG/JU
Sample : M1429-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBGS0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

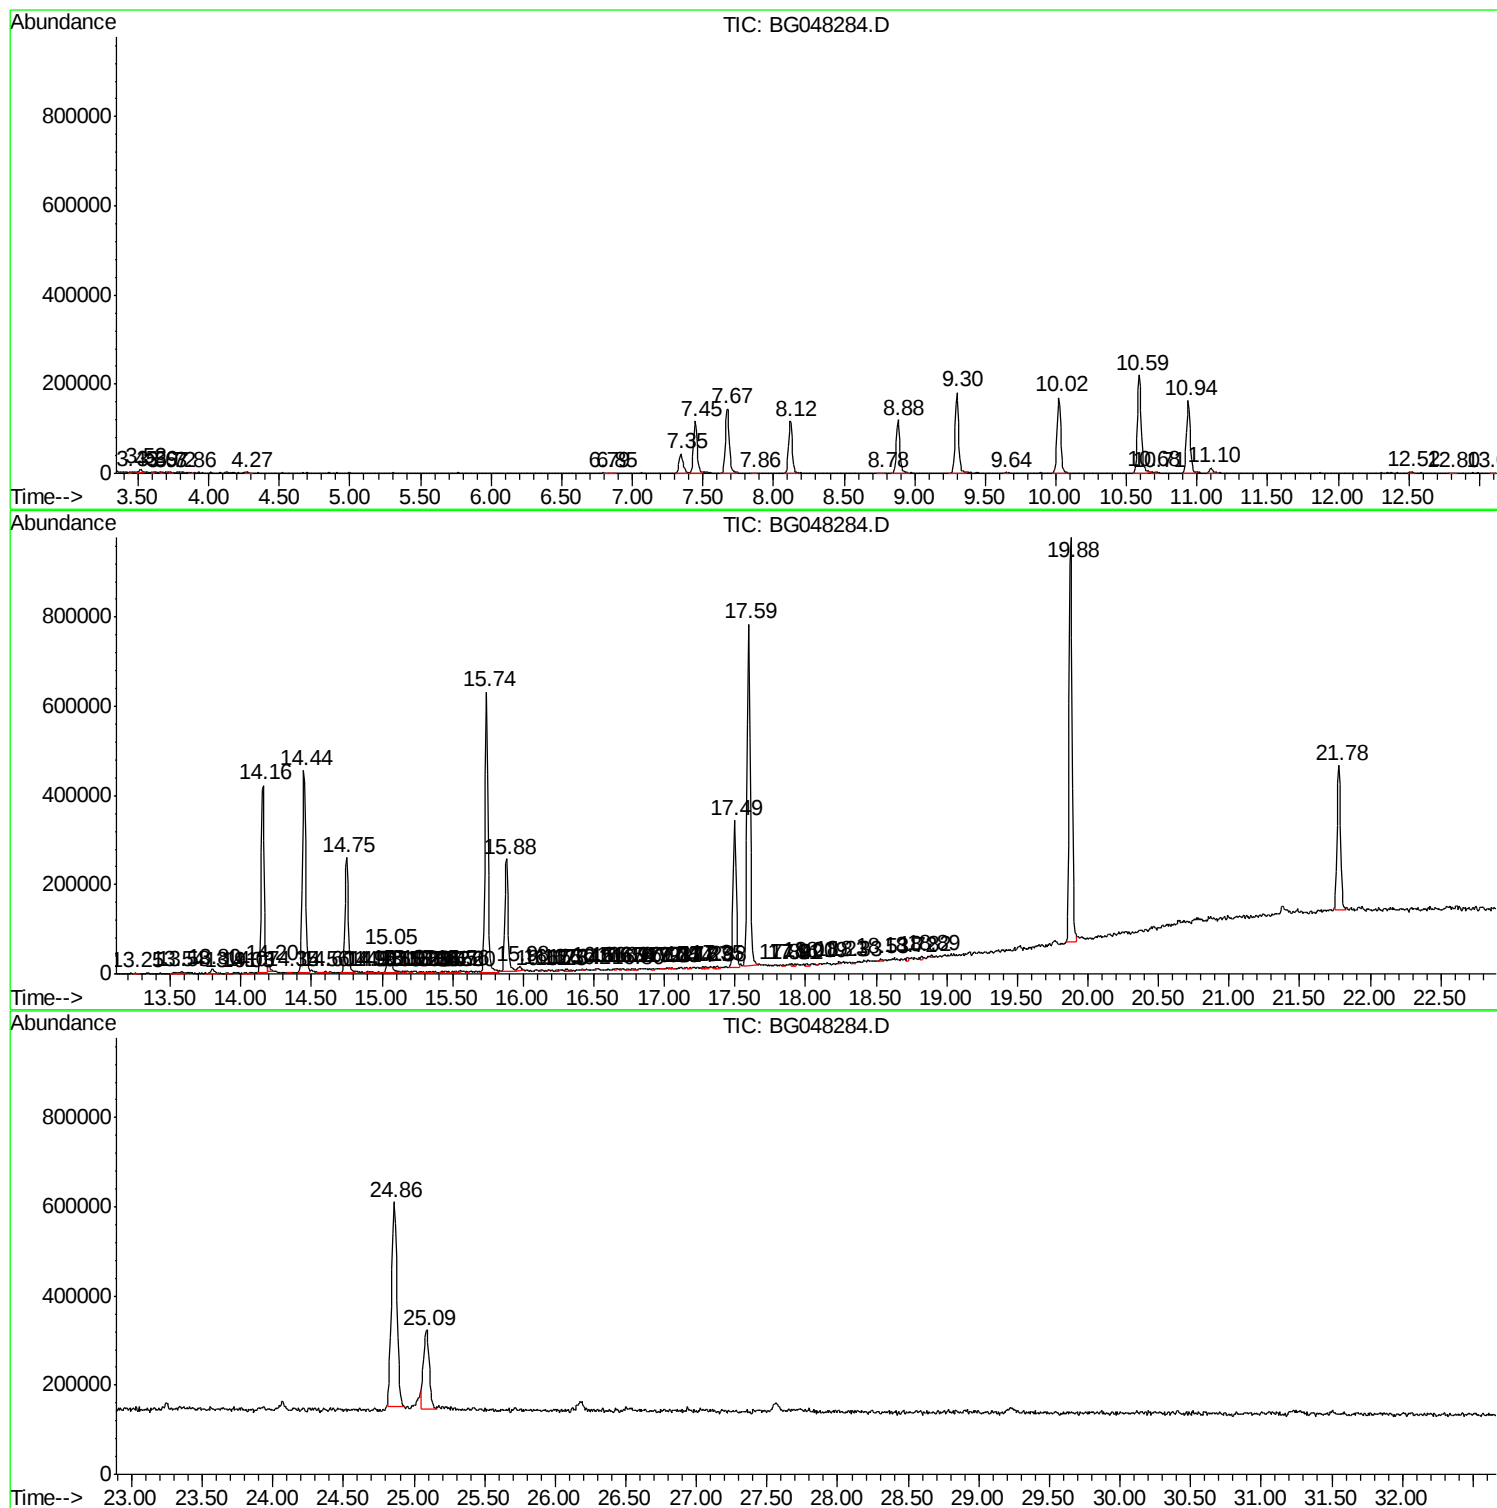

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022221\
Data File : BG048284.D
Acq On : 23 Feb 2021 1:30
Operator : CG/JU
Sample : M1429-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBGSO

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022221\
Data File : BG048284.D
Acq On : 23 Feb 2021 1:30
Operator : CG/JU
Sample : M1429-08
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBGS0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG021321MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc