
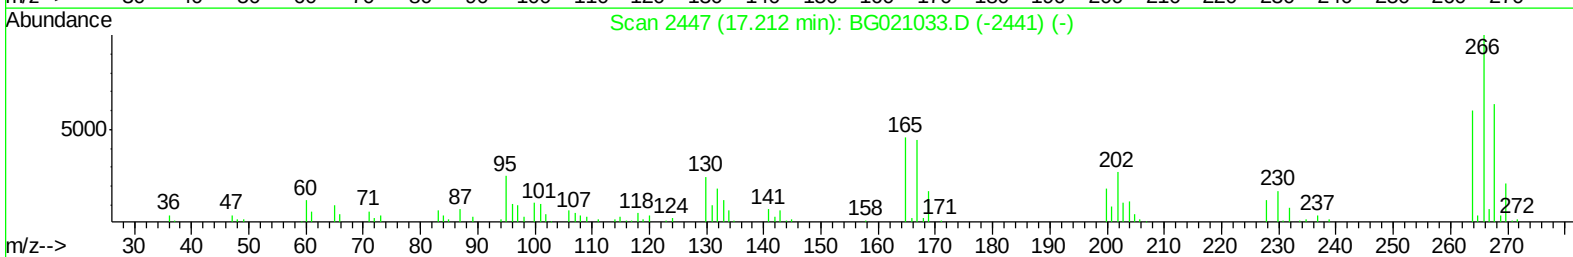
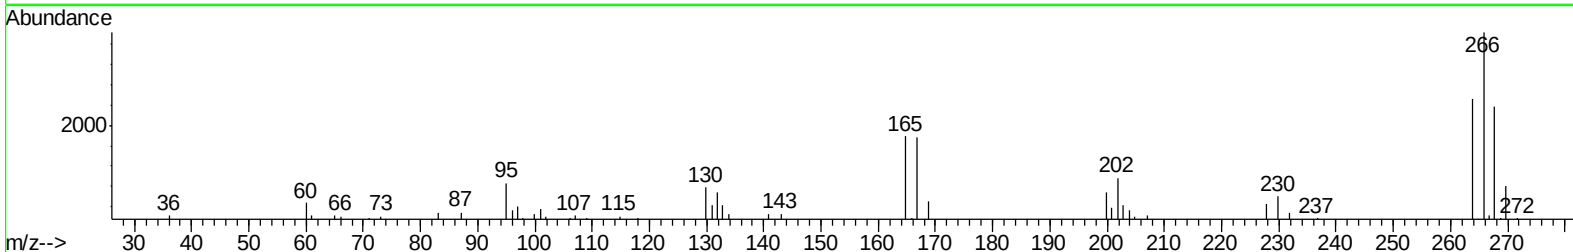


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022316\
Data File : BG021028.D
Acq On : 23 Feb 2016 13:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 07:47:29 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

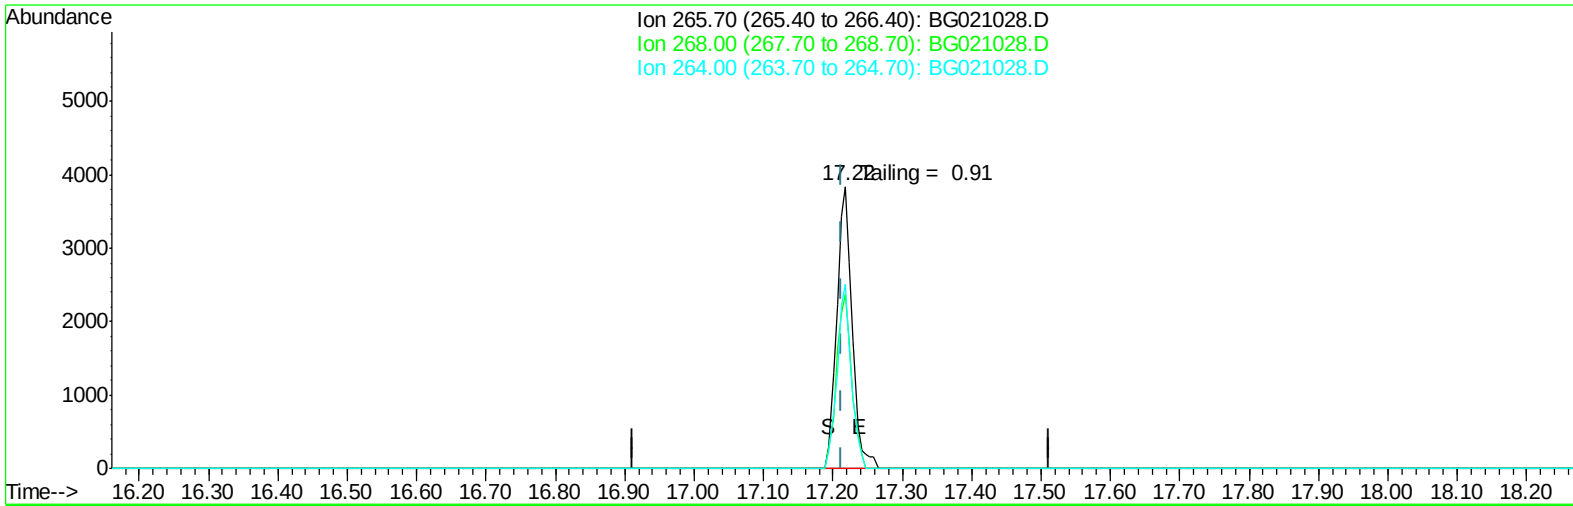

TIC: BG021028.D

(69) Pentachlorophenol (C)




17.218min (+0.006) 0.00ng

response 5983

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	61.89
264.00	59.80	65.62
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG022316\
Data File : BG021028.D
Acq On : 23 Feb 2016 13:25
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 07:47:29 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

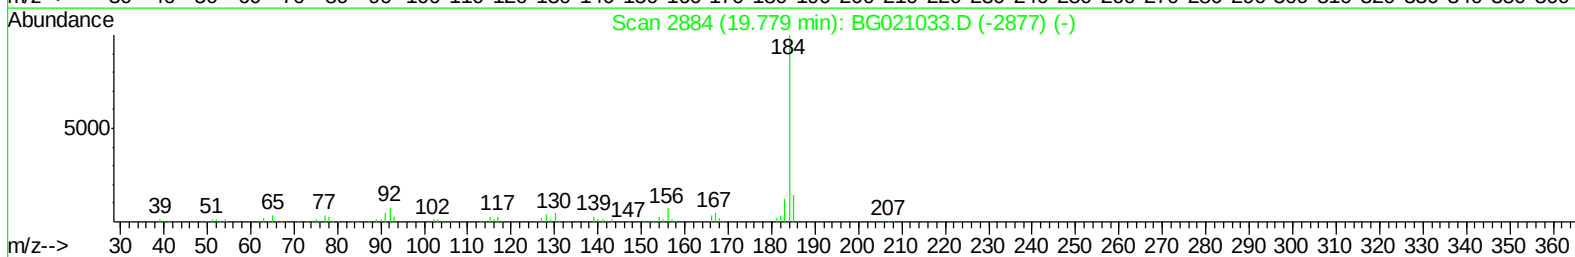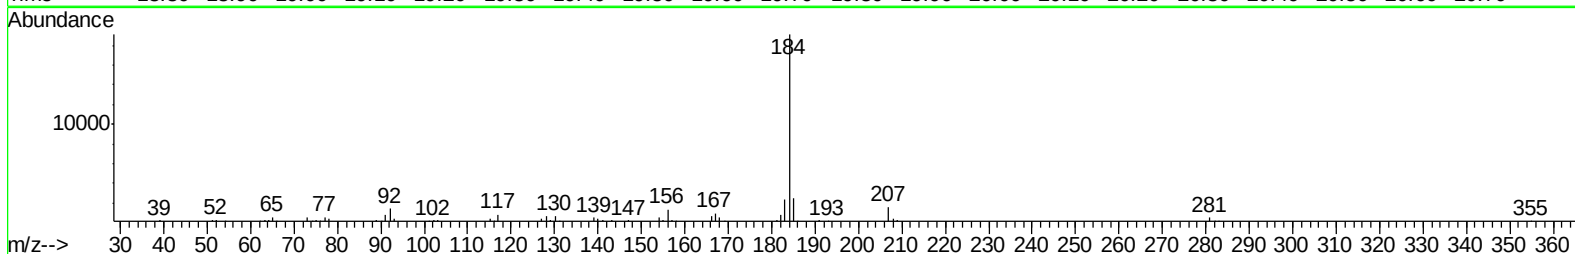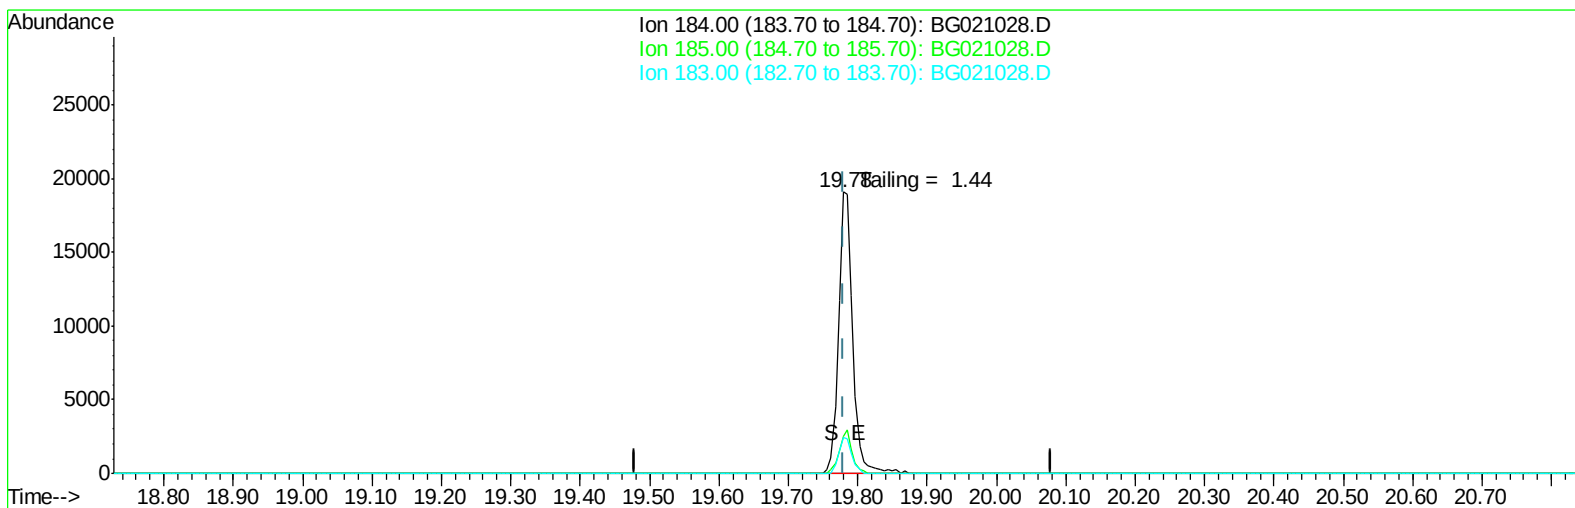

TIC: BG021028.D

(76) Benzidine

19.779min (-0.000) 0.00ng

response 27238

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.13
183.00	12.60	12.71
0.00	0.00	0.00