
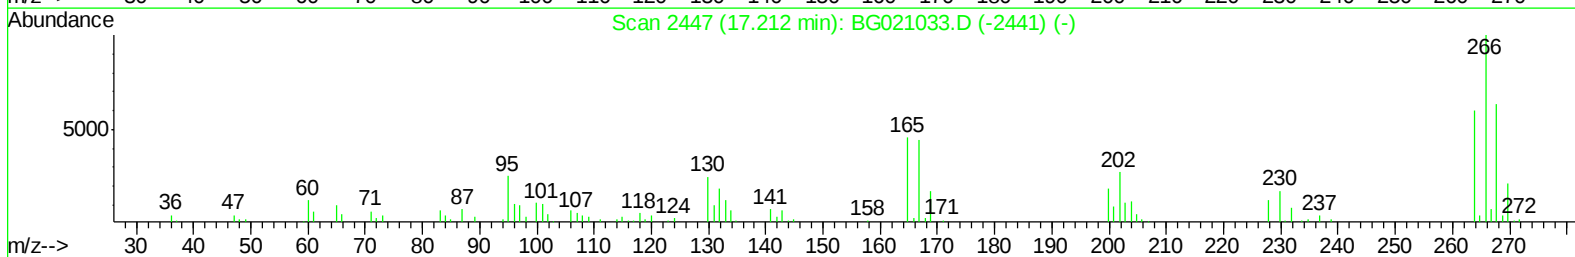
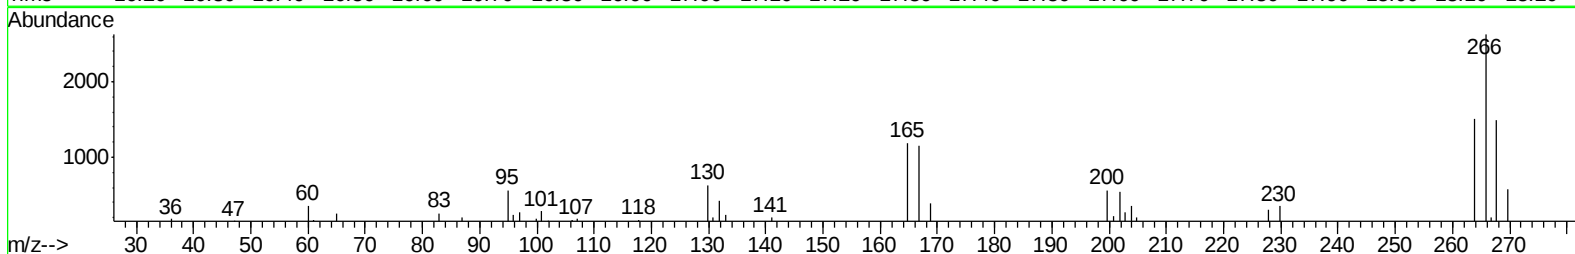


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022316\
Data File : BG021038.D
Acq On : 23 Feb 2016 21:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 07:48:26 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

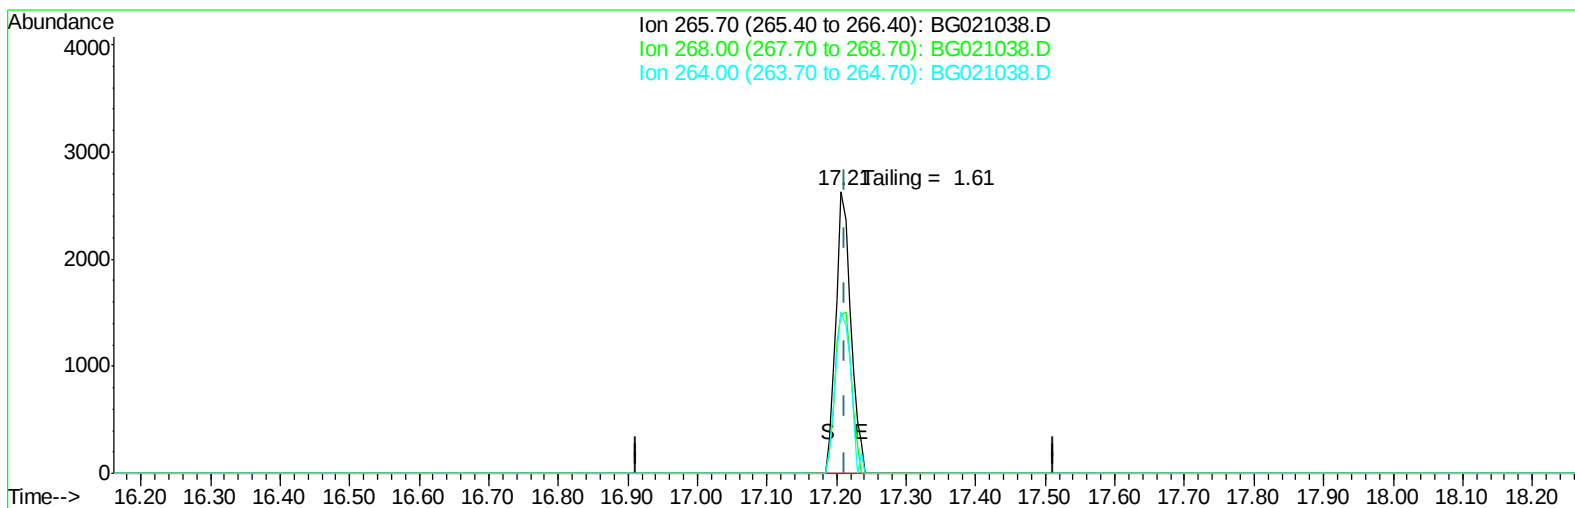

TIC: BG021038.D

(69) Pentachlorophenol (C)




17.207min (-0.006) 0.00ng

response 3929

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	56.51
264.00	59.80	57.46
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\Data\BG022316\
Data File : BG021038.D
Acq On : 23 Feb 2016 21:48
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 07:48:26 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

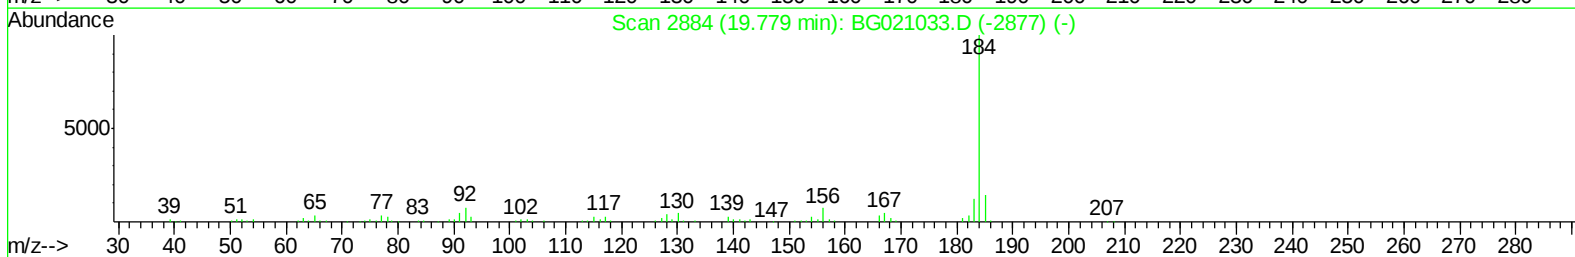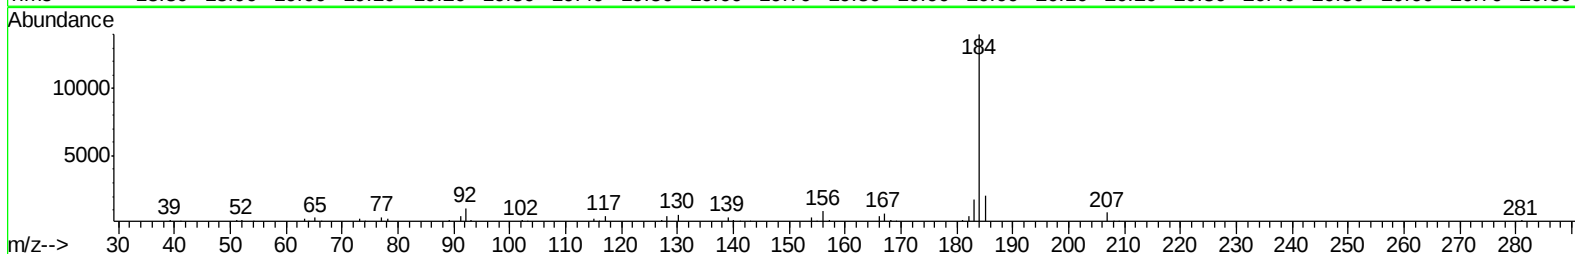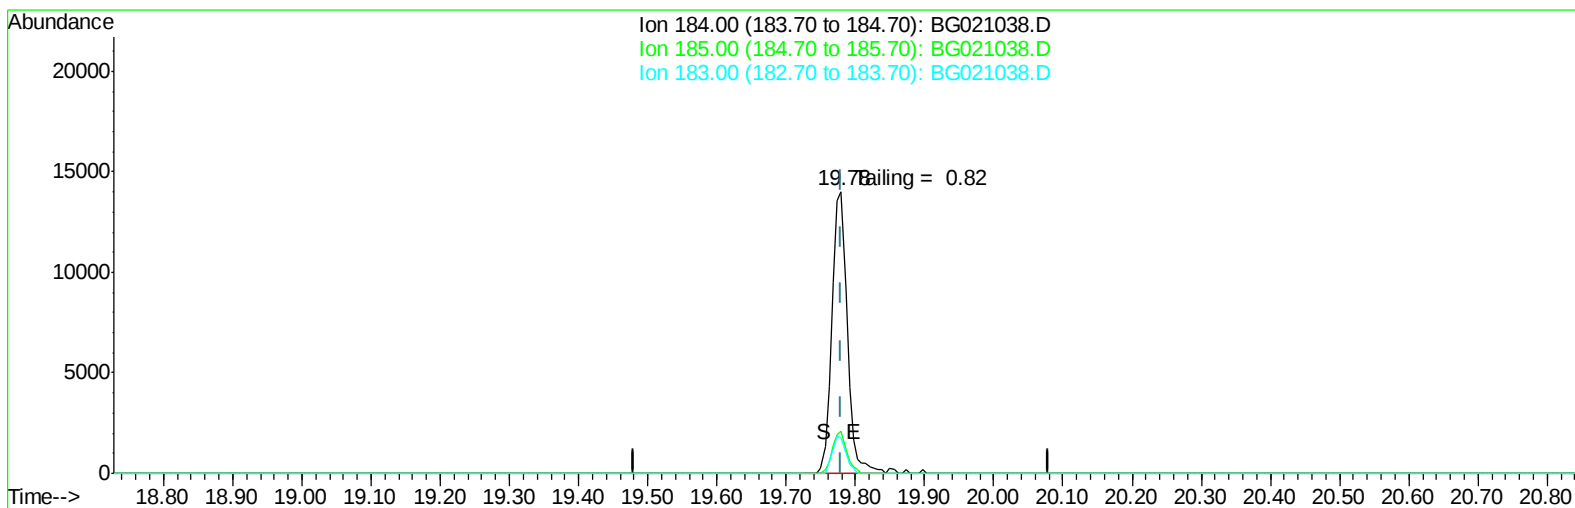

TIC: BG021038.D

(76) Benzidine

19.780min (+0.000) 0.00ng

response 21424

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.94
183.00	12.60	12.63
0.00	0.00	0.00