


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022316\
 Data File : BG021038.D
 Acq On : 23 Feb 2016 21:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022316.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 24 00:35:06 2016

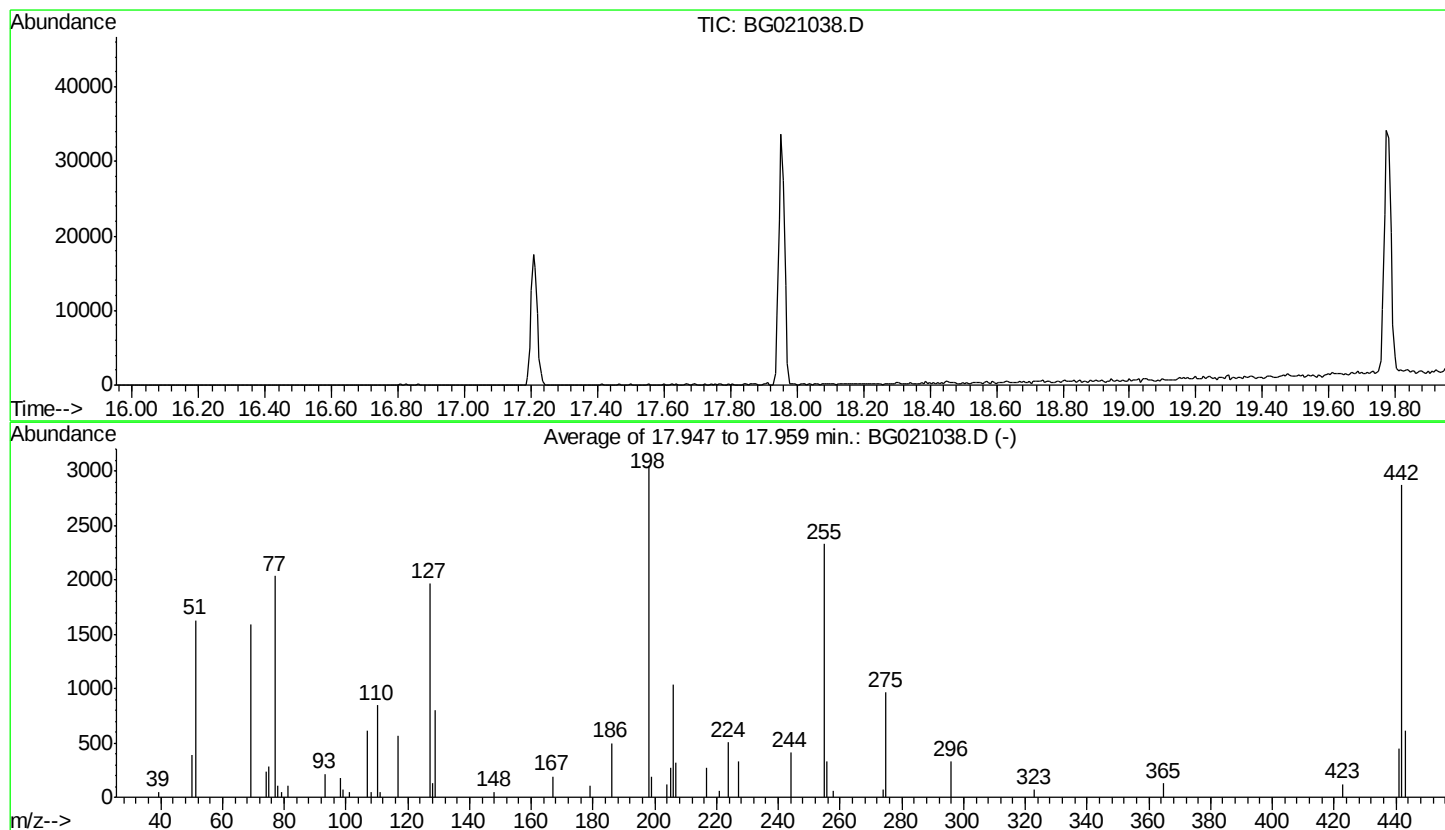

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	1632	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.3	1595	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	64.4	1964	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	3052	PASS
199	198	5	9	6.3	192	PASS
275	198	10	60	31.6	964	PASS
365	198	1	100	4.2	127	PASS
441	442	0.01	24	15.8	454	PASS
442	198	50	100	94.1	2873	PASS
443	442	15	24	21.4	615	PASS