
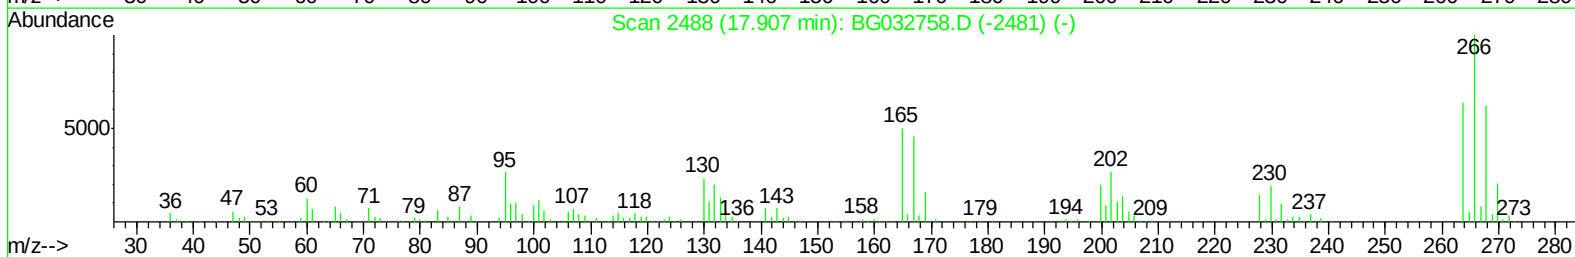
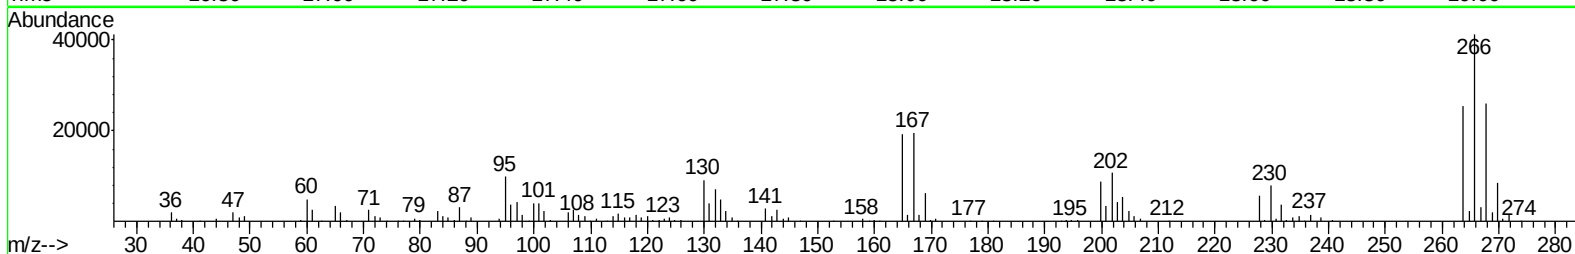


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022318\
Data File : BG032789.D
Acq On : 23 Feb 2018 14:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 00:15:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 17:04:54 2018
Response via : Initial Calibration

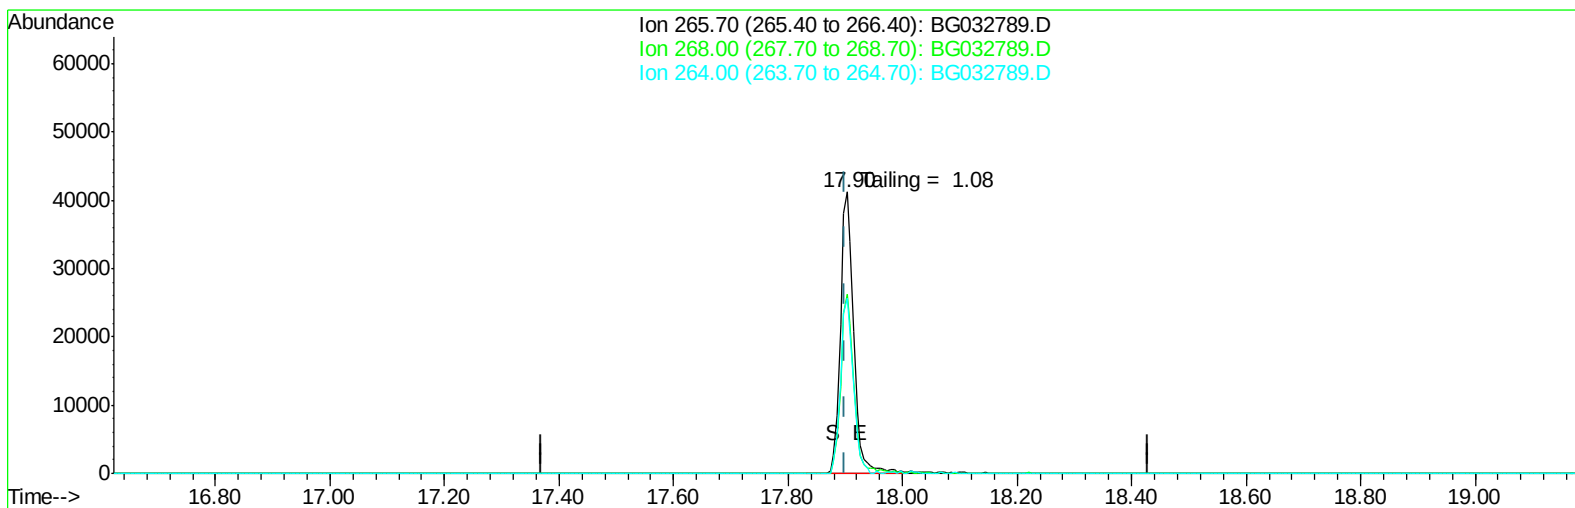

TIC: BG032789.D

(69) Pentachlorophenol (C)




17.903min (+0.003) 13497.15ng

response 67128

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.47
264.00	62.00	62.09
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022318\
Data File : BG032789.D
Acq On : 23 Feb 2018 14:31
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 00:15:13 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 23 17:04:54 2018
Response via : Initial Calibration

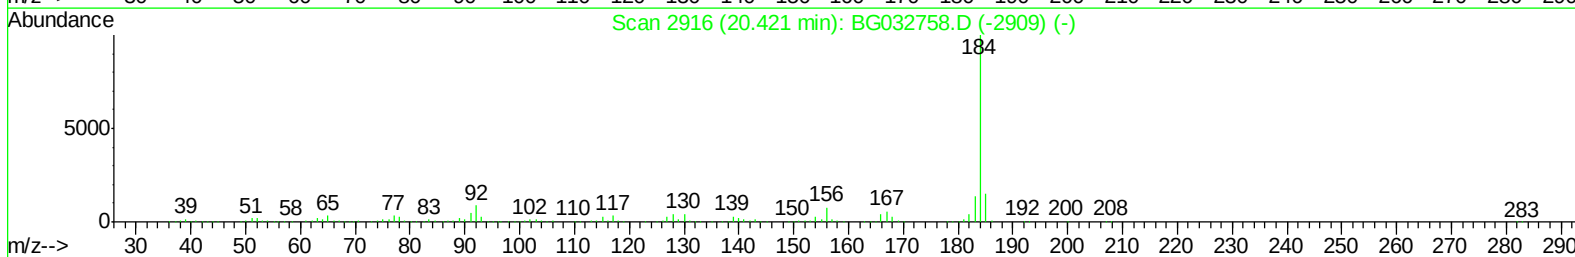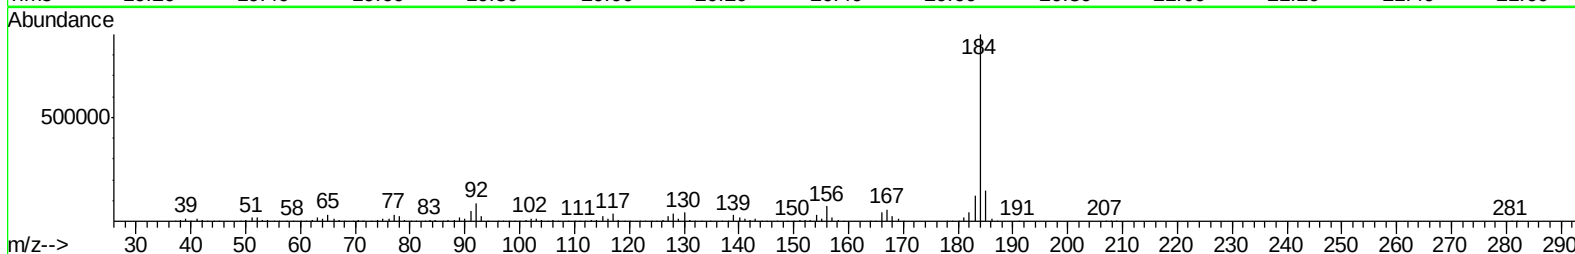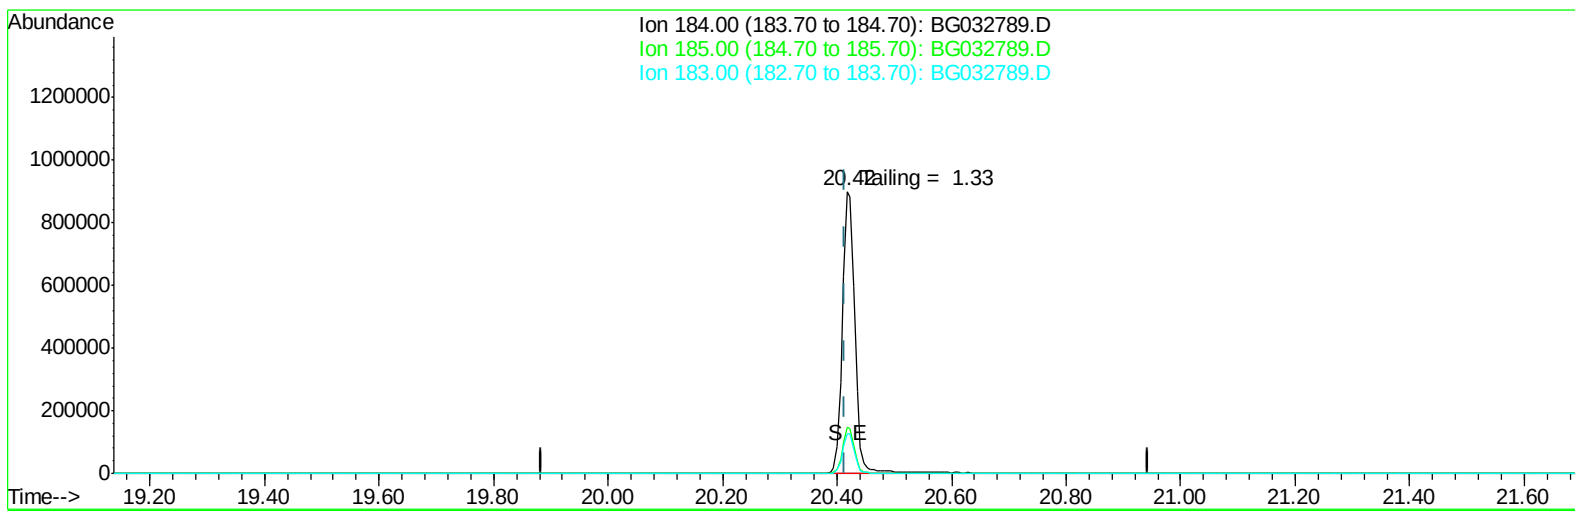

TIC: BG032789.D

(76) Benzidine

20.417min (+0.003) 75663.21ng

response 1379824

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	16.19
183.00	13.30	13.94
0.00	0.00	0.00