


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022318\
 Data File : BG032808.D
 Acq On : 24 Feb 2018 3:05
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 23 17:04:54 2018

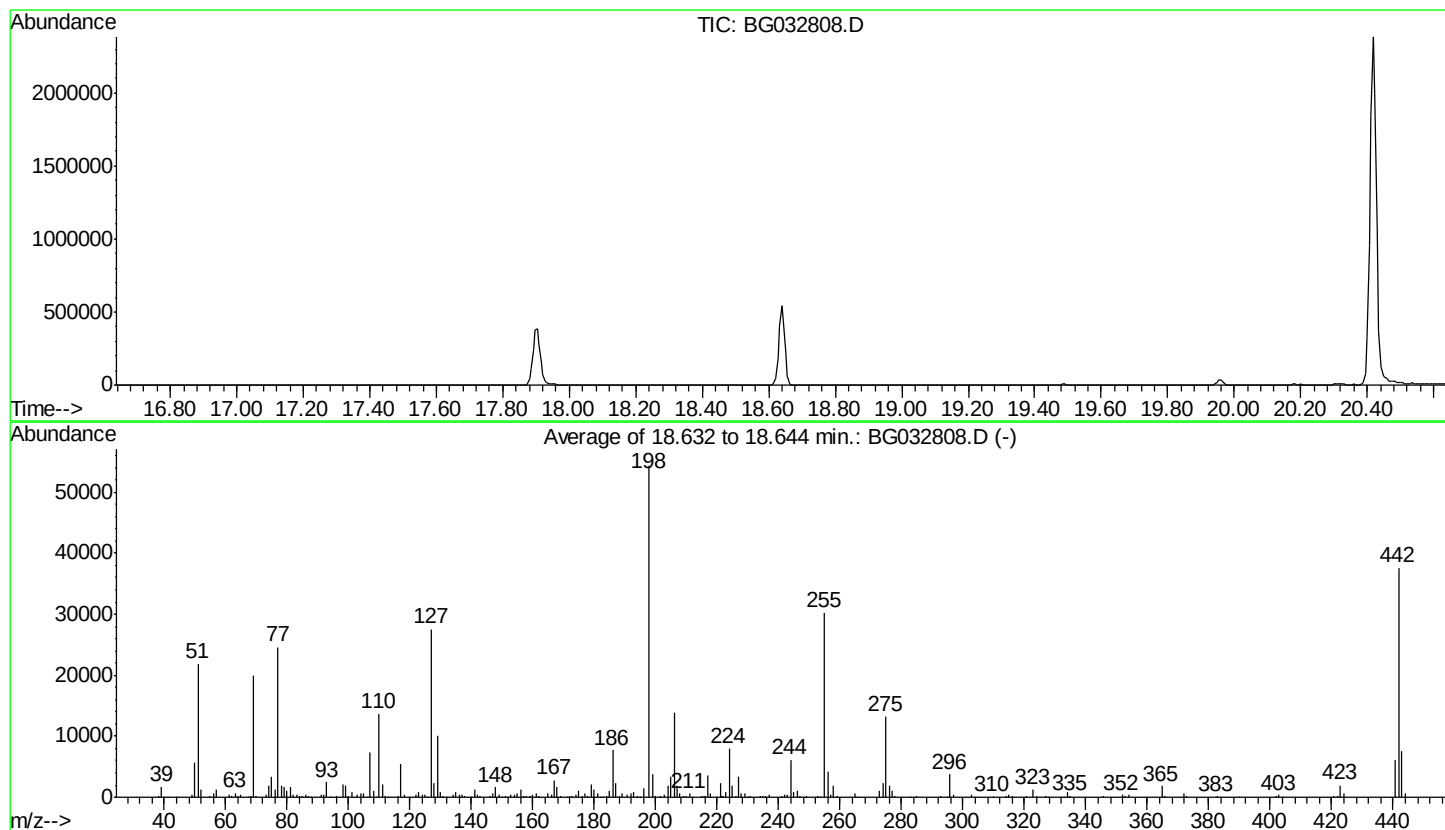

AutoFind: Scans 2612, 2613, 2614; Background Corrected with Scan 2606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	21928	PASS
68	69	0.00	2	1.6	317	PASS
69	198	0.00	100	36.7	19927	PASS
70	69	0.00	2	0.6	123	PASS
127	198	10	80	50.7	27565	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	54365	PASS
199	198	5	9	6.9	3765	PASS
275	198	10	60	24.2	13161	PASS
365	198	1	100	3.4	1860	PASS
441	442	0.01	24	16.2	6083	PASS
442	198	50	100	69.2	37594	PASS
443	442	15	24	20.1	7570	PASS