




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052465.D
 Acq On : 23 Feb 2022 15:43
 Operator : CG/JU
 Sample : N1621-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GBD34

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:08:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/24/2022
 Supervised By :mohammad ahmed 02/24/2022

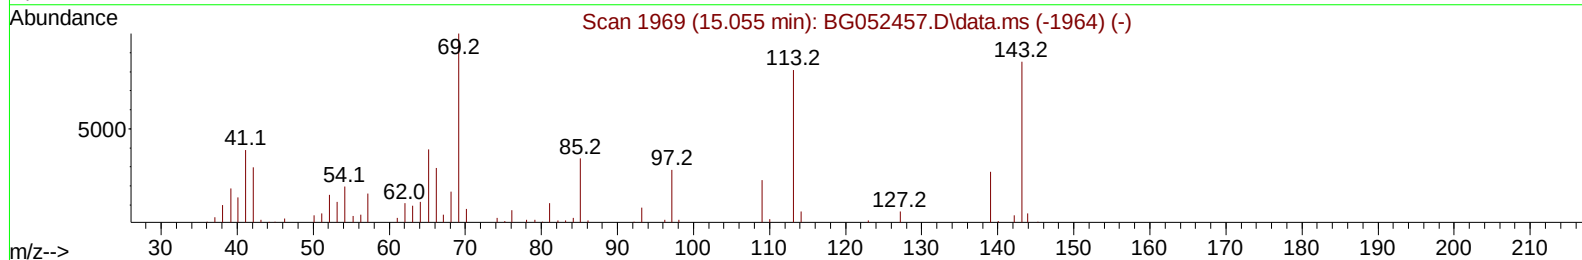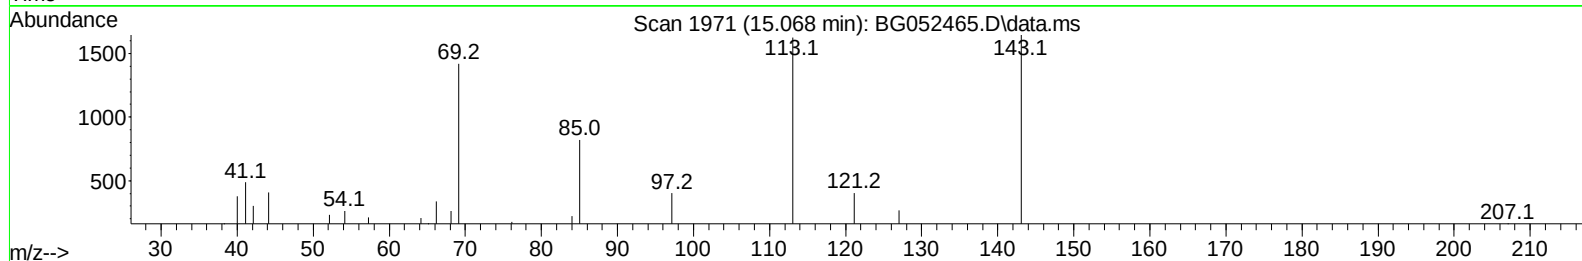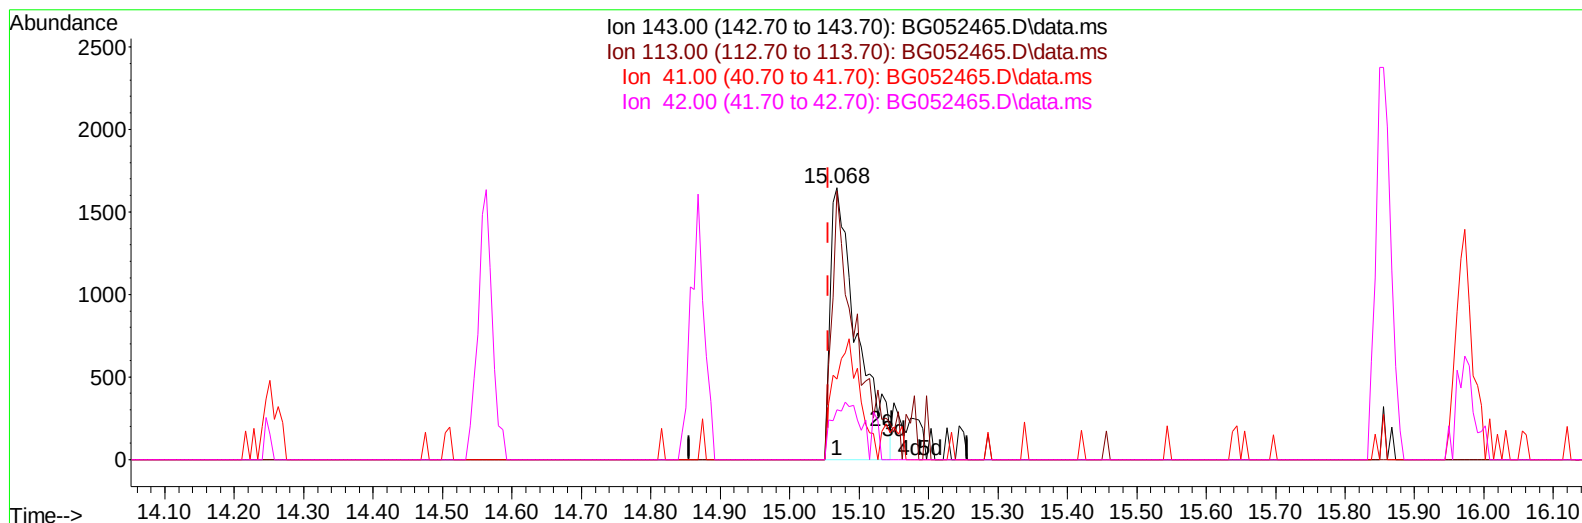

TIC: BG052465.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.068min (+ 0.013) 4.54 ng/ul m

response 4443

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.30	98.78#
41.00	44.40	29.53#
42.00	29.70	18.29#

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052465.D
 Acq On : 23 Feb 2022 15:43
 Operator : CG/JU
 Sample : N1621-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GBD34

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/24/2022
 Supervised By :mohammad ahmed 02/24/2022

Quant Time: Feb 24 00:08:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.224	152	24048	20.000	ng/ul	0.00
20) Naphthalene-d8	11.056	136	100643	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.868	164	75708	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.618	188	193298	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.935	240	204009	20.000	ng/ul	# 0.00
88) Perylene-d12	25.389	264	199374	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.543	96	1229	2.005	ng/uL	0.00
4) Pyridine-d5	3.983	84	13156	7.114	ng/ul	0.00
7) Phenol-d5	7.373	99	12414	5.444	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.531	67	36720	27.555	ng/ul	0.00
11) 2-Chlorophenol-d4	7.749	132	32415	20.239	ng/ul	0.00
15) 4-Methylphenol-d8	8.929	113	22527	12.697	ng/ul	0.00
21) Nitrobenzene-d5	9.393	128	23827	27.771	ng/ul	0.00
24) 2-Nitrophenol-d4	10.128	143	24843	26.435	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.680	165	40673	23.208	ng/ul	0.00
31) 4-Chloroaniline-d4	11.185	131	54271	22.346	ng/ul	0.00
46) Dimethylphthalate-d6	14.257	166	179517	29.168	ng/ul	0.00
49) Acenaphthylene-d8	14.563	160	213793	28.139	ng/ul	0.00
54) 4-Nitrophenol-d4	15.068	143	4443m	4.541	ng/ul	0.01
60) Fluorene-d10	15.855	176	160229	29.635	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.973	200	30249	24.680	ng/ul	0.00
73) Anthracene-d10	17.717	188	304311	32.587	ng/ul	0.00
81) Pyrene-d10	19.997	212	390581	32.719	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.160	264	356196	33.301	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052465.D
Acq On : 23 Feb 2022 15:43
Operator : CG/JU
Sample : N1621-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GBD34

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

Quant Time: Feb 24 00:08:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

