




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052470.D
Acq On : 23 Feb 2022 18:58
Operator : CG/JU
Sample : PB142864BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK864

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:09:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

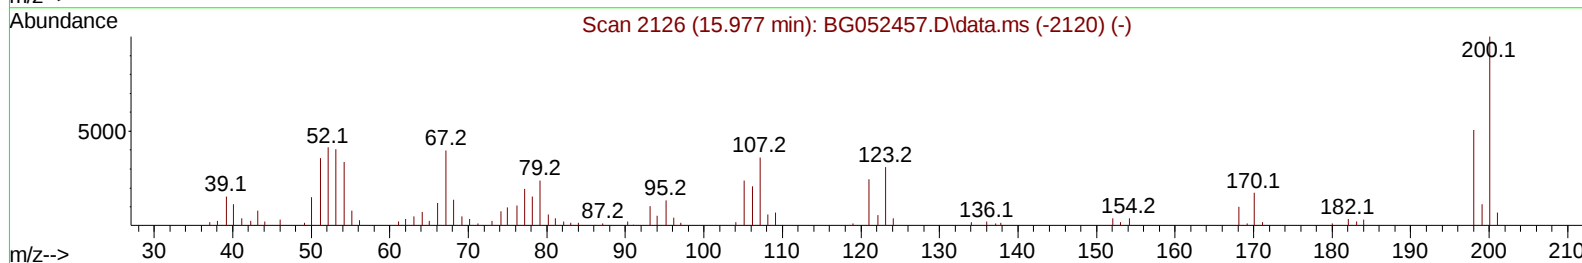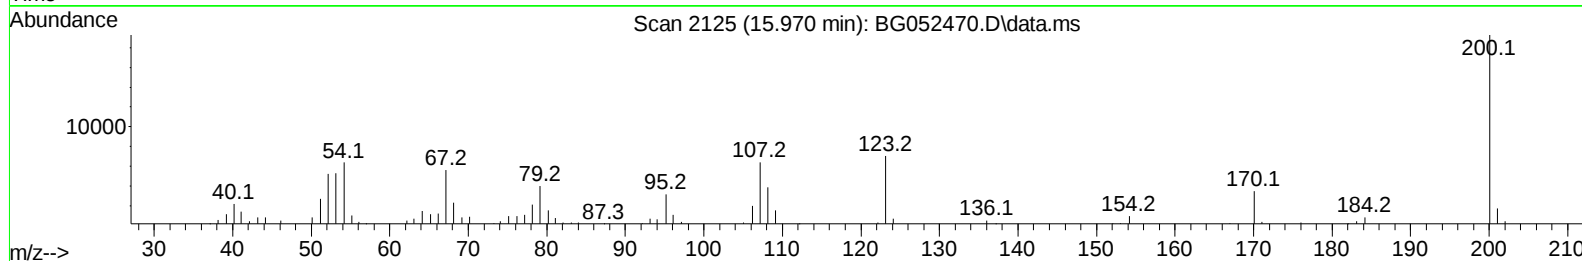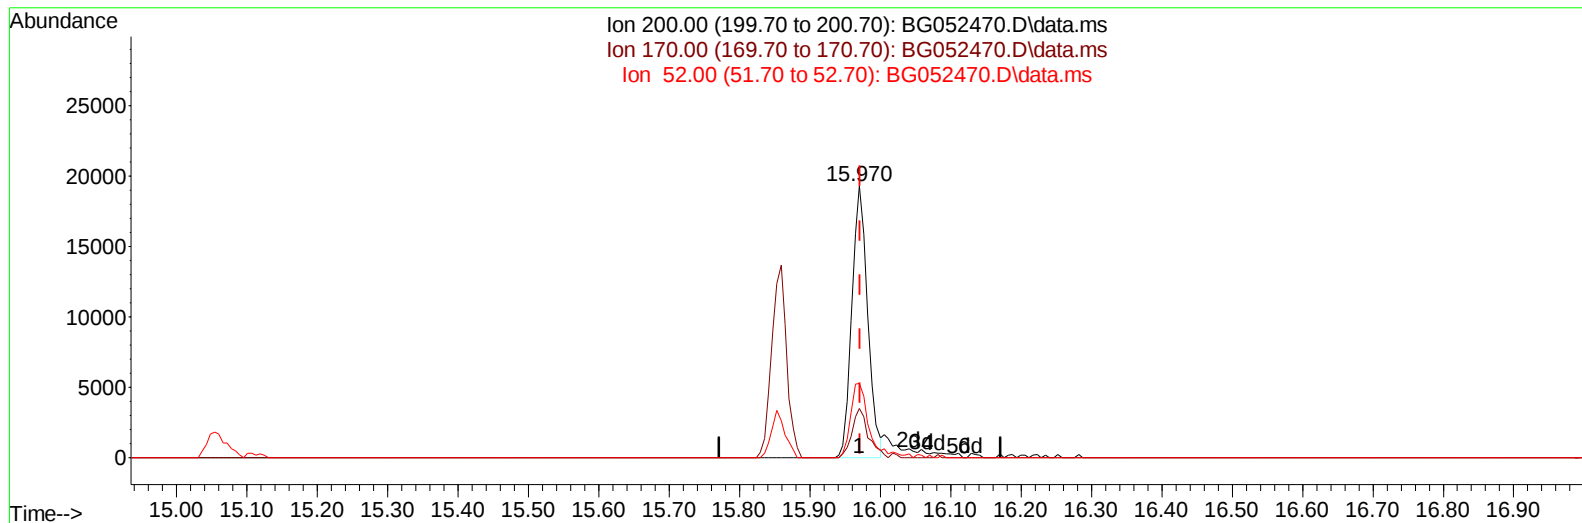

TIC: BG052470.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.970min (-0.001) 24.33 ng/u1

response 29828

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.80	18.01
52.00	47.40	27.16#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052470.D
 Acq On : 23 Feb 2022 18:58
 Operator : CG/JU
 Sample : PB142864BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK864

Manual IntegrationsAPPROVED

Quant Time: Feb 24 00:09:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 02/24/2022
 Supervised By :mohammad ahmed 02/24/2022

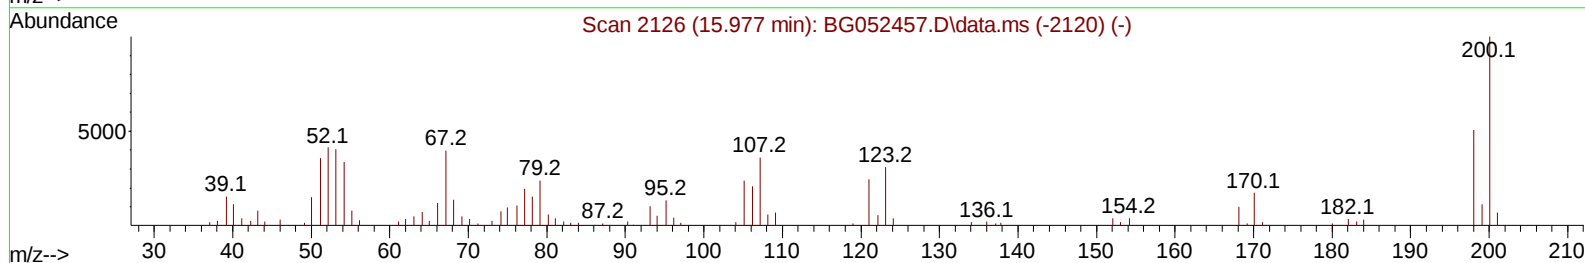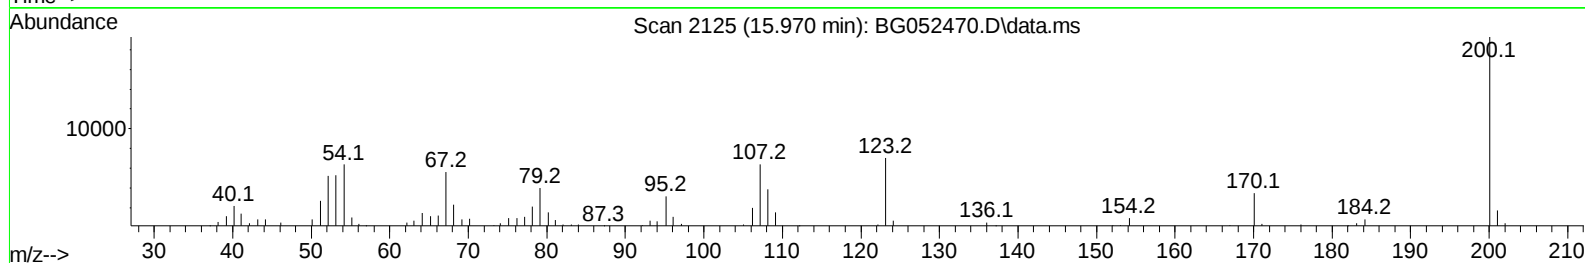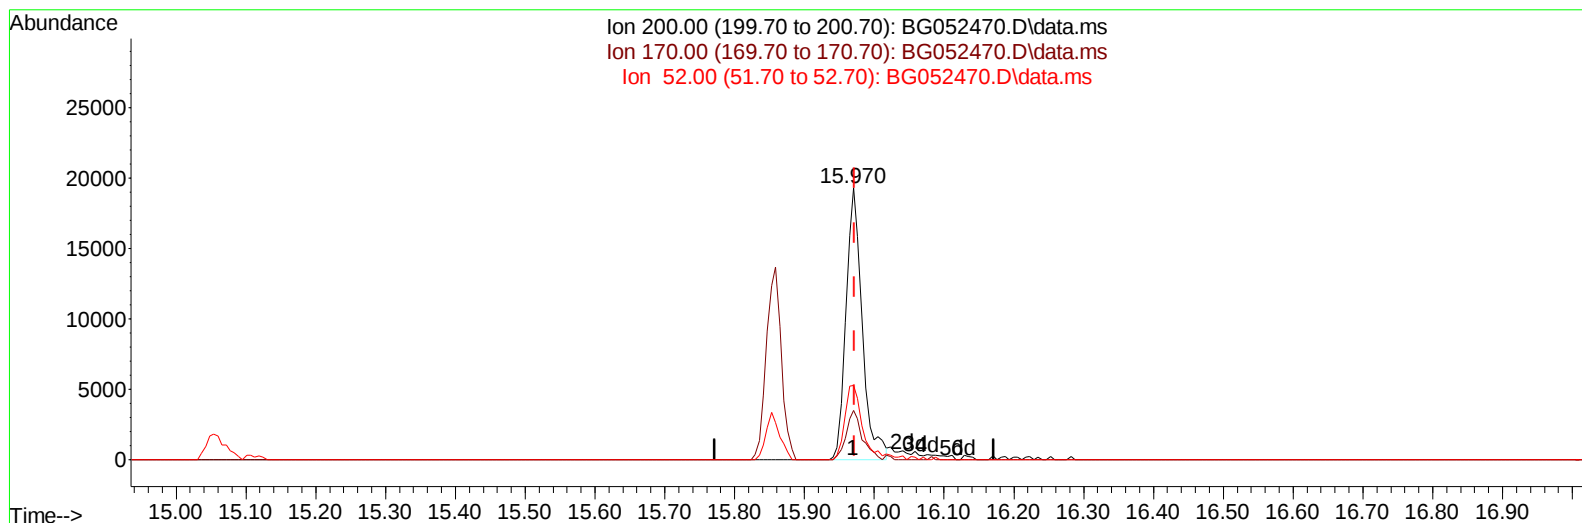

TIC: BG052470.D\data.ms

(65) 4,6-Dinitro-2-methylphenol-d2 (S)

15.970min (-0.001) 25.41 ng/ul m

response 31150

Ion	Exp%	Act%
200.00	100.00	100.00
170.00	19.80	18.01
52.00	47.40	27.16#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052470.D
 Acq On : 23 Feb 2022 18:58
 Operator : CG/JU
 Sample : PB142864BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK864

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/24/2022
 Supervised By :mohammad ahmed 02/24/2022

Quant Time: Feb 24 00:09:32 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.222	152	23894	20.000	ng/ul	0.00
20) Naphthalene-d8	11.059	136	100269	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.866	164	74331	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.615	188	193356	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.927	240	207779	20.000	ng/ul	# 0.00
88) Perylene-d12	25.393	264	204092	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.546	96	4181	6.864	ng/uL	0.00
4) Pyridine-d5	3.975	84	53437	29.080	ng/ul	0.00
7) Phenol-d5	7.364	99	69896	30.849	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.529	67	43622	32.945	ng/ul	0.00
11) 2-Chlorophenol-d4	7.752	132	51585	32.415	ng/ul	0.00
15) 4-Methylphenol-d8	8.927	113	53424	30.305	ng/ul	0.00
21) Nitrobenzene-d5	9.397	128	27502	32.174	ng/ul	0.00
24) 2-Nitrophenol-d4	10.125	143	30786	32.881	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.677	165	54906	31.447	ng/ul	0.00
31) 4-Chloroaniline-d4	11.189	131	72360	29.906	ng/ul	0.00
46) Dimethylphthalate-d6	14.255	166	212954	35.242	ng/ul	0.00
49) Acenaphthylene-d8	14.560	160	249833	33.492	ng/ul	0.00
54) 4-Nitrophenol-d4	15.054	143	28042	29.193	ng/ul	0.00
60) Fluorene-d10	15.859	176	177150	33.372	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.970	200	31150m	25.408	ng/ul	0.00
73) Anthracene-d10	17.715	188	317172	33.955	ng/ul	0.00
81) Pyrene-d10	19.994	212	405486	33.351	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.158	264	379450	34.655	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052470.D
Acq On : 23 Feb 2022 18:58
Operator : CG/JU
Sample : PB142864BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK864

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 02/24/2022
Supervised By :mohammad ahmed 02/24/2022

Quant Time: Feb 24 00:09:32 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

