

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052461.D
 Acq On : 23 Feb 2022 13:07
 Operator : CG/JU
 Sample : N1622-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 GBD34

Quant Time: Feb 23 16:06:58 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 22 17:32:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.240	152	24761	20.000	ng/ul	0.02
20) Naphthalene-d8	11.072	136	102985	20.000	ng/ul	# 0.01
38) Acenaphthene-d10	14.878	164	74267	20.000	ng/ul	0.01
64) Phenanthrene-d10	17.622	188	182901	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.939	240	192713	20.000	ng/ul	# 0.00
88) Perylene-d12	25.405	264	191940	20.000	ng/ul	0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.553	96	3745	5.933	ng/uL	0.01
4) Pyridine-d5	3.981	84	53127	27.899	ng/ul	0.00
7) Phenol-d5	7.383	99	68098	29.003	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.541	67	43735	31.874	ng/ul	0.01
11) 2-Chlorophenol-d4	7.765	132	49647	30.105	ng/ul	0.02
15) 4-Methylphenol-d8	8.945	113	53621	29.352	ng/ul	0.01
21) Nitrobenzene-d5	9.409	128	26953	30.700	ng/ul	0.01
24) 2-Nitrophenol-d4	10.138	143	30928	32.161	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.690	165	52835	29.463	ng/ul	0.02
31) 4-Chloroaniline-d4	11.201	131	71018	28.577	ng/ul	0.01
46) Dimethylphthalate-d6	14.268	166	193834	32.106	ng/ul	0.01
49) Acenaphthylene-d8	14.573	160	238642	32.019	ng/ul	0.01
54) 4-Nitrophenol-d4	15.061	143	25217	26.274	ng/ul	0.00
60) Fluorene-d10	15.865	176	165878	31.276	ng/ul	0.01
65) 4,6-Dinitro-2-methylph...	15.977	200	26741	23.058	ng/ul	0.00
73) Anthracene-d10	17.722	188	288551	32.656	ng/ul	0.00
81) Pyrene-d10	20.001	212	352041	31.219	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.170	264	331251	32.168	ng/ul	0.01
Target Compounds						
8) Phenol	7.412	94	3460	1.457	ng/ul	Qvalue 93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052461.D
Acq On : 23 Feb 2022 13:07
Operator : CG/JU
Sample : N1622-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
GBD34

Quant Time: Feb 23 16:06:58 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 22 17:32:12 2022
Response via : Initial Calibration

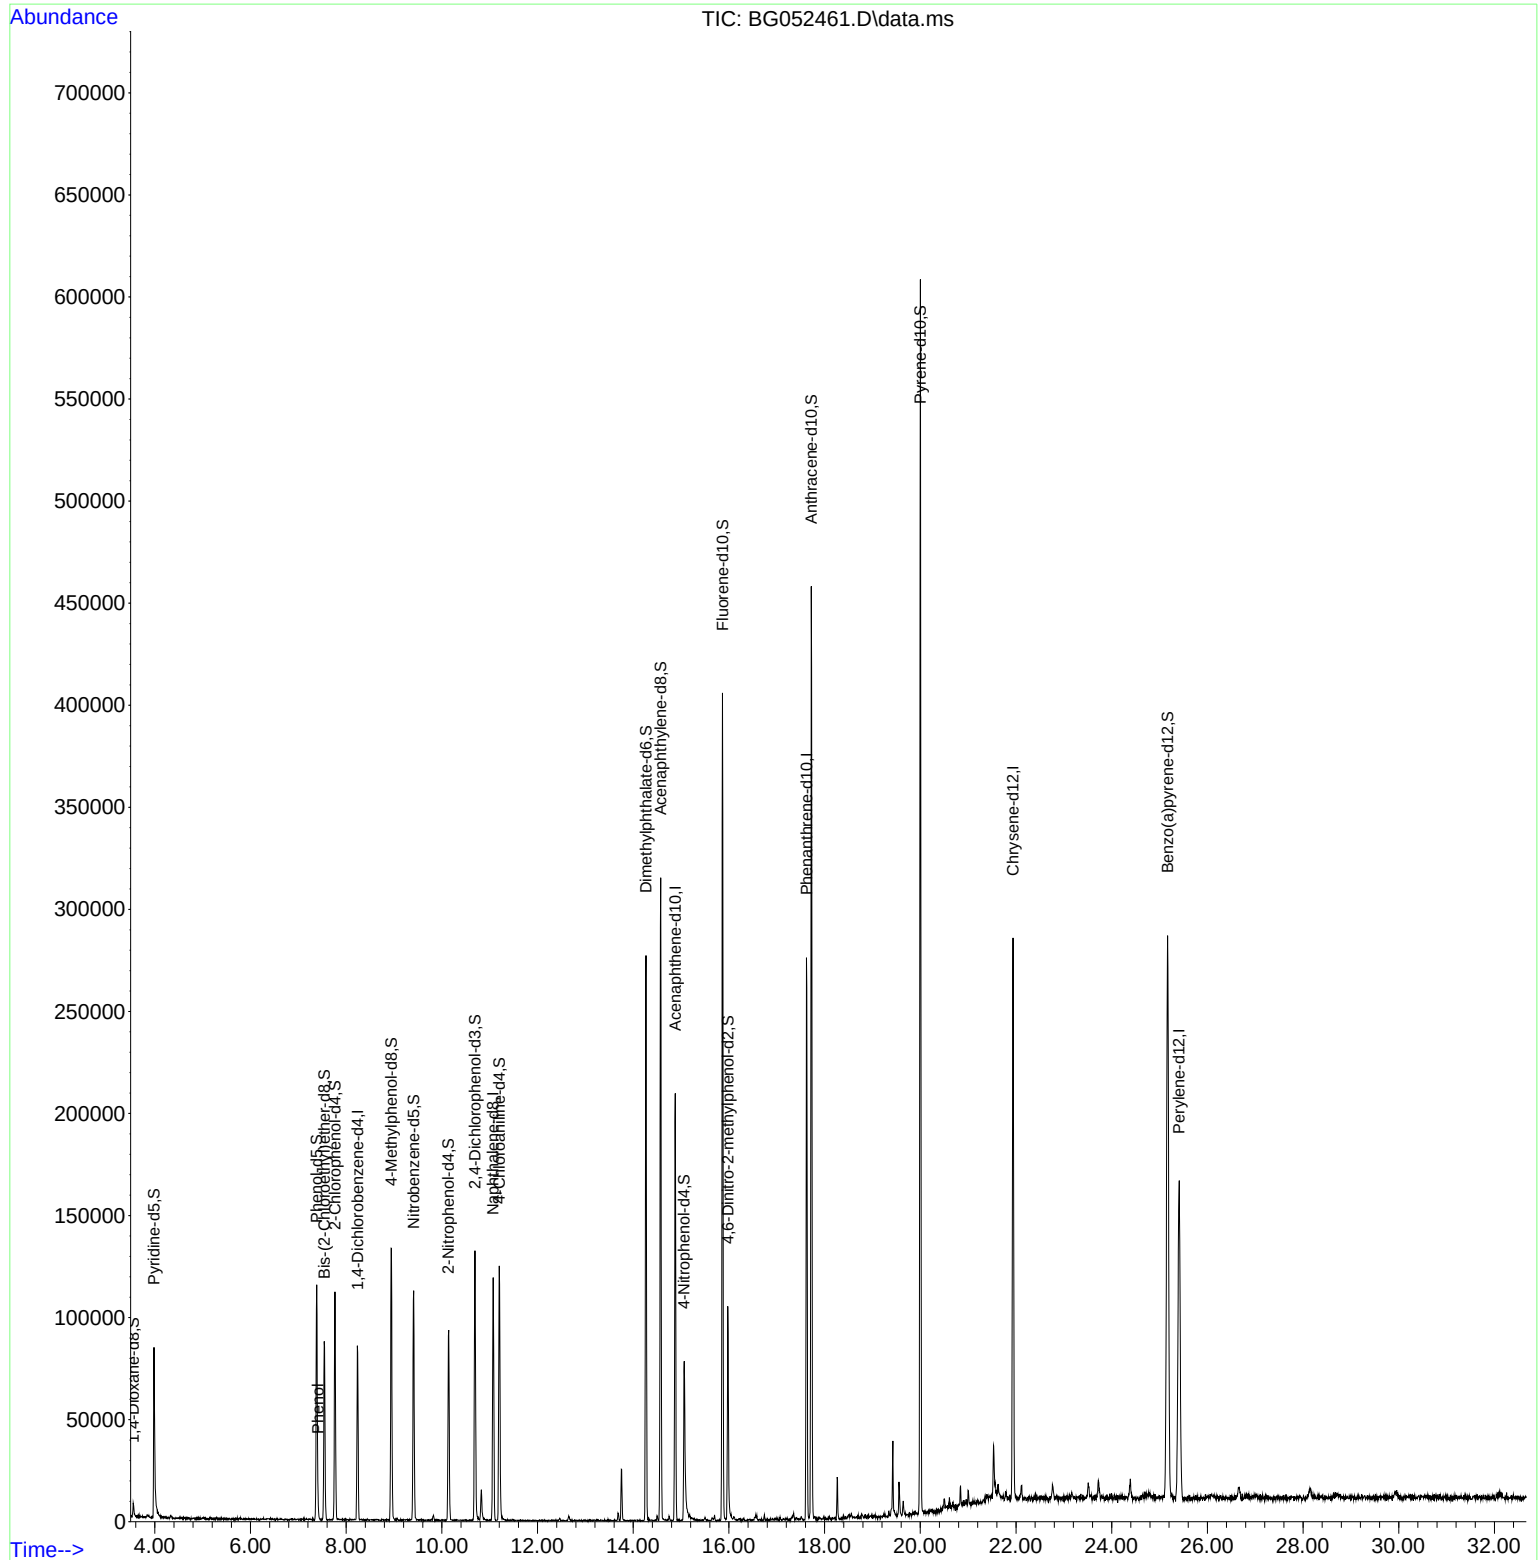

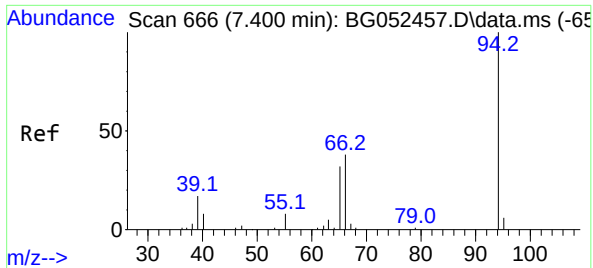

#8
Phenol
Concen: 1.457 ng/ul
RT: 7.412 min Scan# 60
Delta R.T. 0.017 min
Lab File: BG052461.D
Acq: 23 Feb 2022 13:07

Instrument :
BNA_G
ClientSampleId :
GBD34

Tgt Ion: 94	Resp:	3460
Ion	Ratio	Lower Upper
94	100	
65	25.5	25.1 37.7
66	37.2	31.6 47.4

