

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052458.D
 Acq On : 23 Feb 2022 10:22
 Operator : CG/JU
 Sample : PB142851BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK851

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052458.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.548	6	10	17	rVB2	6671	10046	1.29%	0.138%
2	3.830	55	58	62	rBV4	816	1449	0.19%	0.020%
3	3.977	80	83	96	rBV	69465	125570	16.14%	1.720%
4	4.330	140	143	145	rBV3	1350	1580	0.20%	0.022%
5	7.378	655	662	672	rBV	93693	162934	20.94%	2.232%
6	7.537	683	689	699	rVB	72688	120474	15.49%	1.651%
7	7.760	720	727	735	rVV	90884	155073	19.93%	2.125%
8	8.236	801	808	815	rVB	76238	128991	16.58%	1.767%
9	8.935	921	927	937	rBV	107022	192284	24.72%	2.634%
10	9.405	998	1007	1017	rVB	88381	163667	21.04%	2.242%
11	10.139	1123	1132	1140	rVB	75141	137323	17.65%	1.881%
12	10.686	1219	1225	1239	rBV	98863	191560	24.62%	2.624%
13	10.797	1242	1244	1249	rVV2	1105	1790	0.23%	0.025%
14	11.067	1283	1290	1299	rVB	107522	190167	24.44%	2.605%
15	11.197	1304	1312	1325	rBV	108746	201066	25.85%	2.755%
16	12.642	1556	1558	1560	rBV3	1339	1623	0.21%	0.022%
17	14.263	1827	1834	1843	rBV	234676	349528	44.93%	4.789%
18	14.569	1878	1886	1896	rBV	257847	402709	51.77%	5.517%
19	14.874	1931	1938	1944	rVV	183480	291371	37.45%	3.992%
20	15.068	1964	1971	1981	rBV2	60662	131924	16.96%	1.807%
21	15.861	2100	2106	2116	rBV	335018	508310	65.34%	6.964%
22	15.973	2120	2125	2135	rBV	76932	130019	16.71%	1.781%
23	17.623	2399	2406	2412	rBV	262208	400903	51.53%	5.492%
24	17.717	2415	2422	2431	rBV2	388858	606570	77.97%	8.310%
25	19.568	2732	2737	2741	rBV4	7167	7902	1.02%	0.108%
26	19.638	2743	2749	2754	rBV3	5114	8805	1.13%	0.121%
27	19.897	2790	2793	2798	rVB5	1554	2054	0.26%	0.028%
28	19.997	2804	2810	2819	rVB	531705	777944	100.00%	10.658%
29	20.760	2937	2940	2941	rBV3	1734	1728	0.22%	0.024%
30	20.907	2964	2965	2967	rBV2	1842	1395	0.18%	0.019%
31	21.083	2993	2995	2999	rBV3	1648	2109	0.27%	0.029%
32	21.418	3050	3052	3053	rVB2	3315	1934	0.25%	0.026%
33	21.442	3053	3056	3058	rVB3	3921	4041	0.52%	0.055%
34	21.630	3086	3088	3089	rBV	2638	1718	0.22%	0.024%
35	21.647	3089	3091	3092	rVV2	2853	1687	0.22%	0.023%
36	21.935	3132	3140	3149	rVB	280956	493105	63.39%	6.756%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052458.D
 Acq On : 23 Feb 2022 10:22
 Operator : CG/JU
 Sample : PB142851BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK851

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	21.994	3149	3150	3154	rBV4	3380	3925	0.50%	0.054%
38	22.111	3168	3170	3172	rVV3	1816	1357	0.17%	0.019%
39	22.687	3266	3268	3270	rBV2	1940	1531	0.20%	0.021%
40	22.799	3285	3287	3291	rVB4	2897	1973	0.25%	0.027%
41	22.981	3317	3318	3321	rBV3	2031	2507	0.32%	0.034%
42	23.028	3324	3326	3327	rBV2	2149	1723	0.22%	0.024%
43	23.292	3369	3371	3374	rVB3	2631	1784	0.23%	0.024%
44	23.474	3399	3402	3403	rBV2	1985	1614	0.21%	0.022%
45	23.509	3404	3408	3412	rVV6	3982	7714	0.99%	0.106%
46	23.562	3416	3417	3418	rBV	1958	1286	0.17%	0.018%
47	23.950	3482	3483	3486	rBV3	2557	3227	0.41%	0.044%
48	24.120	3510	3512	3514	rBV2	2564	1983	0.25%	0.027%
49	24.144	3514	3516	3518	rVV3	1835	1706	0.22%	0.023%
50	24.179	3521	3522	3524	rBV2	2258	1588	0.20%	0.022%
51	24.385	3552	3557	3564	rVB8	4785	11118	1.43%	0.152%
52	24.655	3601	3603	3605	rBV3	2180	2327	0.30%	0.032%
53	24.708	3610	3612	3613	rVB2	2469	1302	0.17%	0.018%
54	24.725	3613	3615	3616	rBV2	1938	1810	0.23%	0.025%
55	24.919	3646	3648	3649	rBV2	2051	1424	0.18%	0.020%
56	24.955	3652	3654	3655	rBV2	3043	2203	0.28%	0.030%
57	25.019	3663	3665	3668	rBV4	2062	2128	0.27%	0.029%
58	25.160	3679	3689	3708	rVB2	252144	755553	97.12%	10.351%
59	25.401	3719	3730	3744	rVB3	153335	482529	62.03%	6.611%
60	25.671	3774	3776	3777	rBV2	1634	1400	0.18%	0.019%
61	26.218	3867	3869	3871	rBV3	2084	2004	0.26%	0.027%
62	26.441	3903	3907	3908	rBV5	2282	2769	0.36%	0.038%
63	26.641	3935	3941	3942	rBV5	5197	7238	0.93%	0.099%
64	27.187	4032	4034	4035	rVB2	2658	1453	0.19%	0.020%
65	27.251	4043	4045	4046	rBV2	1871	1533	0.20%	0.021%
66	27.445	4076	4078	4080	rBV3	2211	2975	0.38%	0.041%
67	27.751	4128	4130	4132	rBV2	2178	2014	0.26%	0.028%
68	27.839	4143	4145	4148	rVB3	2080	2033	0.26%	0.028%
69	28.138	4189	4196	4198	rBV6	3937	9662	1.24%	0.132%
70	28.279	4218	4220	4223	rBV4	2551	1585	0.20%	0.022%
71	28.379	4235	4237	4239	rVB3	2125	1743	0.22%	0.024%
72	28.397	4239	4240	4242	rBV	2843	1842	0.24%	0.025%
73	28.556	4265	4267	4271	rBV3	2268	2972	0.38%	0.041%
74	28.608	4274	4276	4279	rBV4	2498	1945	0.25%	0.027%
75	28.673	4285	4287	4291	rBV4	2300	1840	0.24%	0.025%
76	28.908	4325	4327	4328	rBV2	2106	1313	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052458.D
 Acq On : 23 Feb 2022 10:22
 Operator : CG/JU
 Sample : PB142851BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK851

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	29.325	4396	4398	4400	rBV3	2213	1835	0.24%	0.025%
78	29.419	4412	4414	4415	rVB2	2467	1286	0.17%	0.018%
79	29.466	4420	4422	4423	rBV2	2266	1558	0.20%	0.021%
80	29.542	4433	4435	4437	rVB2	2661	1915	0.25%	0.026%
81	29.566	4437	4439	4443	rBV5	2252	2787	0.36%	0.038%
82	29.648	4451	4453	4454	rBV2	2105	1408	0.18%	0.019%
83	29.725	4464	4466	4467	rBV2	2210	1424	0.18%	0.020%
84	29.772	4472	4474	4476	rBV3	1910	1531	0.20%	0.021%
85	29.889	4491	4494	4496	rBV4	2950	3113	0.40%	0.043%
86	30.012	4513	4515	4516	rVB2	2192	1342	0.17%	0.018%
87	30.148	4534	4538	4539	rBV3	3172	2876	0.37%	0.039%
88	30.441	4586	4588	4589	rBV2	2178	1392	0.18%	0.019%
89	30.459	4589	4591	4593	rVB2	2668	2040	0.26%	0.028%
90	30.682	4627	4629	4630	rBV2	1687	1558	0.20%	0.021%
91	30.805	4648	4650	4651	rBV2	2146	1580	0.20%	0.022%
92	30.852	4656	4658	4659	rBV2	1876	1532	0.20%	0.021%
93	31.087	4696	4698	4701	rBV3	1700	2366	0.30%	0.032%
94	31.405	4748	4752	4753	rBV4	2046	2304	0.30%	0.032%
95	31.669	4795	4797	4800	rBV4	2585	2434	0.31%	0.033%
96	31.698	4800	4802	4804	rBV2	2182	2297	0.30%	0.031%
97	31.916	4837	4839	4840	rBV3	2245	1423	0.18%	0.019%
98	32.380	4916	4918	4920	rBV3	3176	3315	0.43%	0.045%
99	32.521	4940	4942	4944	rBV3	1695	1816	0.23%	0.025%
100	32.609	4955	4957	4959	rVB3	2248	2012	0.26%	0.028%




Sum of corrected areas: 7299130

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052458.D
Acq On : 23 Feb 2022 10:22
Operator : CG/JU
Sample : PB142851BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK851

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

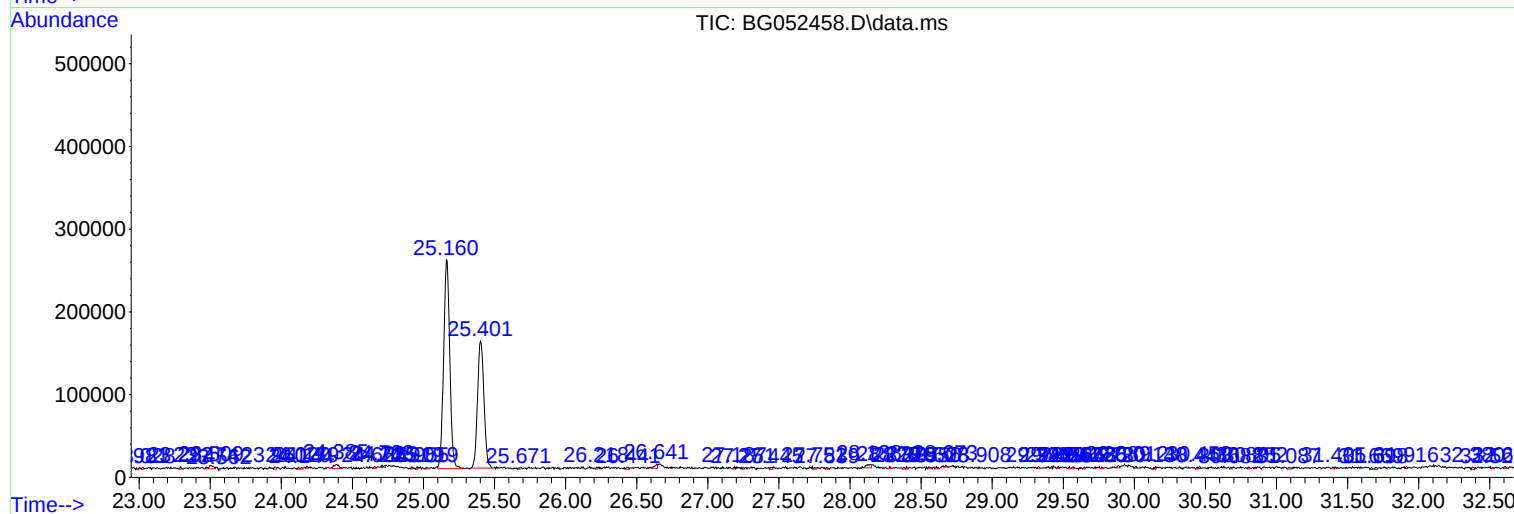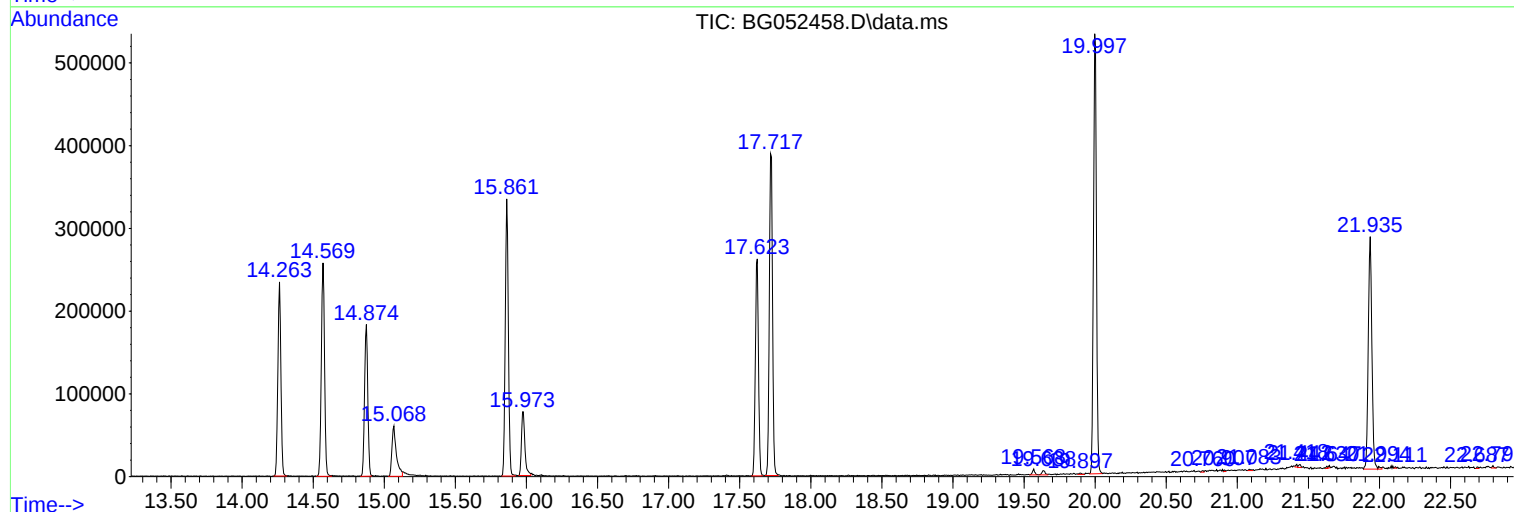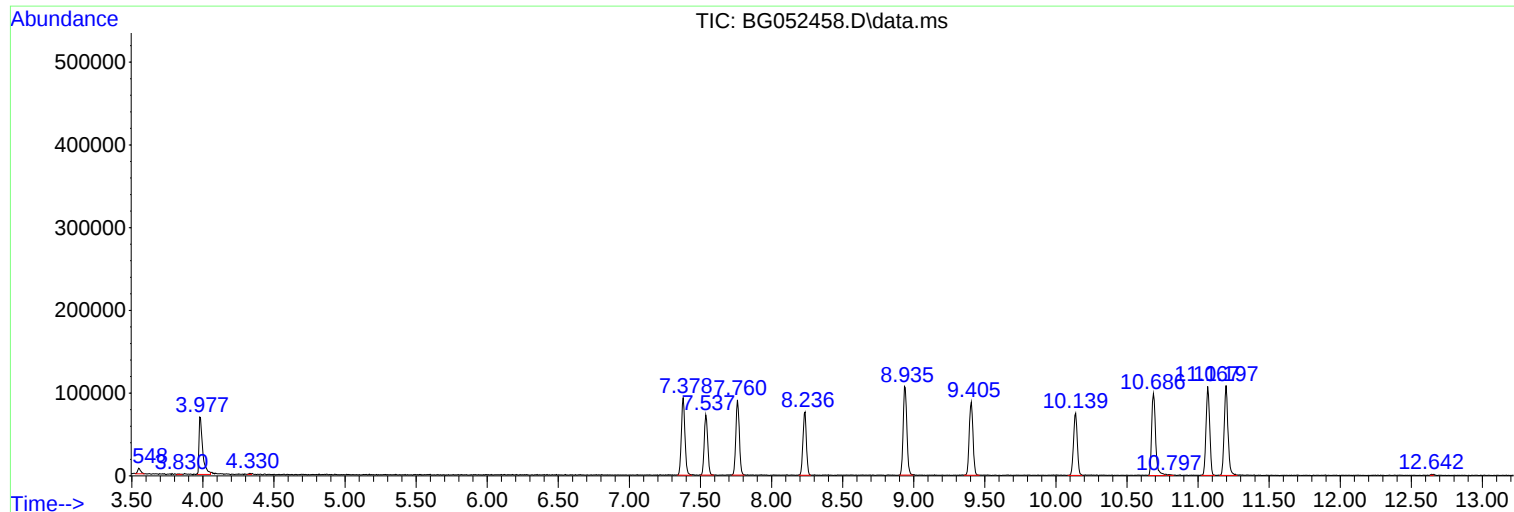

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052458.D
Acq On : 23 Feb 2022 10:22
Operator : CG/JU
Sample : PB142851BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK851

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052458.D
Acq On : 23 Feb 2022 10:22
Operator : CG/JU
Sample : PB142851BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK851

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
