

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052459.D
 Acq On : 23 Feb 2022 11:01
 Operator : CG/JU
 Sample : N1616-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.664	28	30	31	rBV2	909	706	0.14%	0.033%
2	3.770	47	48	50	rBV	776	606	0.12%	0.028%
3	3.799	52	53	55	rBV	780	715	0.14%	0.033%
4	4.022	89	91	94	rVB3	951	854	0.17%	0.040%
5	4.181	116	118	121	rVB3	1068	992	0.19%	0.046%
6	4.334	140	144	146	rBV4	1545	1717	0.33%	0.080%
7	4.527	175	177	178	rBV	1302	767	0.15%	0.036%
8	4.586	184	187	190	rVB2	1142	1109	0.21%	0.052%
9	4.616	190	192	193	rBV	719	619	0.12%	0.029%
10	4.645	196	197	199	rBV	954	598	0.12%	0.028%
11	4.792	219	222	223	rBV	773	704	0.14%	0.033%
12	5.091	272	273	276	rBV	752	860	0.17%	0.040%
13	5.121	276	278	282	rVB3	785	976	0.19%	0.045%
14	5.279	301	305	306	rBV	438	569	0.11%	0.026%
15	5.462	333	336	338	rVB	725	756	0.15%	0.035%
16	5.597	356	359	363	rBV2	653	1034	0.20%	0.048%
17	5.702	376	377	379	rBV	899	659	0.13%	0.031%
18	5.826	396	398	400	rBV	660	755	0.15%	0.035%
19	6.460	503	506	509	rBV	652	816	0.16%	0.038%
20	6.507	512	514	516	rBV2	774	738	0.14%	0.034%
21	6.648	536	538	540	rVB	861	661	0.13%	0.031%
22	6.724	548	551	553	rVB2	666	818	0.16%	0.038%
23	6.865	572	575	576	rBV	712	593	0.11%	0.028%
24	6.971	592	593	597	rBV	689	681	0.13%	0.032%
25	7.118	616	618	622	rVB2	796	873	0.17%	0.041%
26	7.153	622	624	627	rBV2	819	850	0.16%	0.040%
27	7.300	646	649	651	rBV	646	610	0.12%	0.028%
28	7.341	655	656	659	rBV	560	633	0.12%	0.029%
29	7.870	743	746	748	rBV	597	693	0.13%	0.032%
30	8.222	800	806	814	rBV	81228	136332	26.35%	6.343%
31	8.399	832	836	837	rBV2	709	666	0.13%	0.031%
32	9.151	960	964	967	rBV2	544	907	0.18%	0.042%
33	9.209	970	974	976	rVB2	557	771	0.15%	0.036%
34	10.026	1110	1113	1115	rBV2	556	784	0.15%	0.036%
35	10.367	1169	1171	1175	rBV2	632	623	0.12%	0.029%
36	10.555	1199	1203	1206	rBV2	534	732	0.14%	0.034%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052459.D
 Acq On : 23 Feb 2022 11:01
 Operator : CG/JU
 Sample : N1616-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	10.631	1213	1216	1218	rVB2	658	859	0.17%	0.040%
38	10.672	1220	1223	1227	rVB2	640	932	0.18%	0.043%
39	10.889	1256	1260	1262	rVB	711	828	0.16%	0.039%
40	11.060	1281	1289	1300	rBV	108443	197478	38.17%	9.188%
41	11.136	1300	1302	1307	rVV2	1046	1499	0.29%	0.070%
42	11.171	1307	1308	1312	rVB2	905	649	0.13%	0.030%
43	11.776	1407	1411	1415	rVB2	421	677	0.13%	0.031%
44	12.534	1537	1540	1541	rBV2	664	638	0.12%	0.030%
45	12.699	1564	1568	1570	rVB	538	576	0.11%	0.027%
46	13.462	1696	1698	1699	rBV	628	628	0.12%	0.029%
47	14.866	1930	1937	1949	rBV	187766	304244	58.81%	14.156%
48	15.219	1993	1997	2000	rBV2	367	572	0.11%	0.027%
49	15.577	2055	2058	2061	rBV	630	710	0.14%	0.033%
50	15.765	2084	2090	2092	rBV2	454	701	0.14%	0.033%
51	16.176	2159	2160	2164	rVB2	742	593	0.11%	0.028%
52	16.464	2205	2209	2211	rVB2	655	977	0.19%	0.045%
53	16.500	2211	2215	2216	rBV2	742	801	0.15%	0.037%
54	16.535	2216	2221	2224	rBV3	492	771	0.15%	0.036%
55	16.723	2250	2253	2255	rBV	616	645	0.12%	0.030%
56	16.993	2296	2299	2302	rVB2	454	663	0.13%	0.031%
57	17.263	2343	2345	2348	rVB3	597	627	0.12%	0.029%
58	17.398	2365	2368	2369	rBV2	654	614	0.12%	0.029%
59	17.616	2399	2405	2419	rBV	264278	432874	83.68%	20.141%
60	17.710	2419	2421	2423	rVB3	990	802	0.16%	0.037%
61	17.792	2433	2435	2439	rVB4	644	569	0.11%	0.026%
62	17.886	2448	2451	2455	rBV3	501	801	0.15%	0.037%
63	18.344	2526	2529	2531	rVB2	946	760	0.15%	0.035%
64	18.708	2588	2591	2594	rBV3	711	927	0.18%	0.043%
65	18.738	2594	2596	2600	rVV3	733	1116	0.22%	0.052%
66	18.908	2623	2625	2628	rVB3	729	859	0.17%	0.040%
67	18.932	2628	2629	2632	rBV2	935	714	0.14%	0.033%
68	18.973	2632	2636	2637	rBV2	644	648	0.13%	0.030%
69	19.055	2648	2650	2652	rVB2	963	719	0.14%	0.033%
70	19.090	2652	2656	2658	rBV3	871	1273	0.25%	0.059%
71	19.131	2660	2663	2665	rVV2	599	669	0.13%	0.031%
72	19.219	2675	2678	2679	rVB2	766	592	0.11%	0.028%
73	19.284	2687	2689	2691	rVB3	806	713	0.14%	0.033%
74	19.302	2691	2692	2693	rBV	1317	603	0.12%	0.028%
75	19.319	2693	2695	2696	rBV	765	649	0.13%	0.030%
76	19.413	2710	2711	2713	rBV2	1037	705	0.14%	0.033%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052459.D
 Acq On : 23 Feb 2022 11:01
 Operator : CG/JU
 Sample : N1616-10
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	19.437	2713	2715	2716	rBV2	1006	664	0.13%	0.031%
78	19.548	2732	2734	2736	rBV2	838	665	0.13%	0.031%
79	19.672	2753	2755	2756	rBV2	1363	819	0.16%	0.038%
80	19.742	2764	2767	2768	rBV2	1352	1083	0.21%	0.050%
81	19.819	2776	2780	2781	rVB3	1313	1441	0.28%	0.067%
82	19.830	2781	2782	2785	rBV3	1462	1735	0.34%	0.081%
83	20.036	2816	2817	2818	rBV	1664	736	0.14%	0.034%
84	20.077	2823	2824	2827	rBV2	1273	1292	0.25%	0.060%
85	20.283	2857	2859	2860	rBV	1336	843	0.16%	0.039%
86	21.933	3133	3140	3151	rVV	287059	517317	100.00%	24.070%
87	22.033	3155	3157	3158	rBV2	3406	1737	0.34%	0.081%
88	25.393	3720	3729	3744	rVB2	159274	494460	95.58%	23.006%




Sum of corrected areas: 2149244

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052459.D
Acq On : 23 Feb 2022 11:01
Operator : CG/JU
Sample : N1616-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

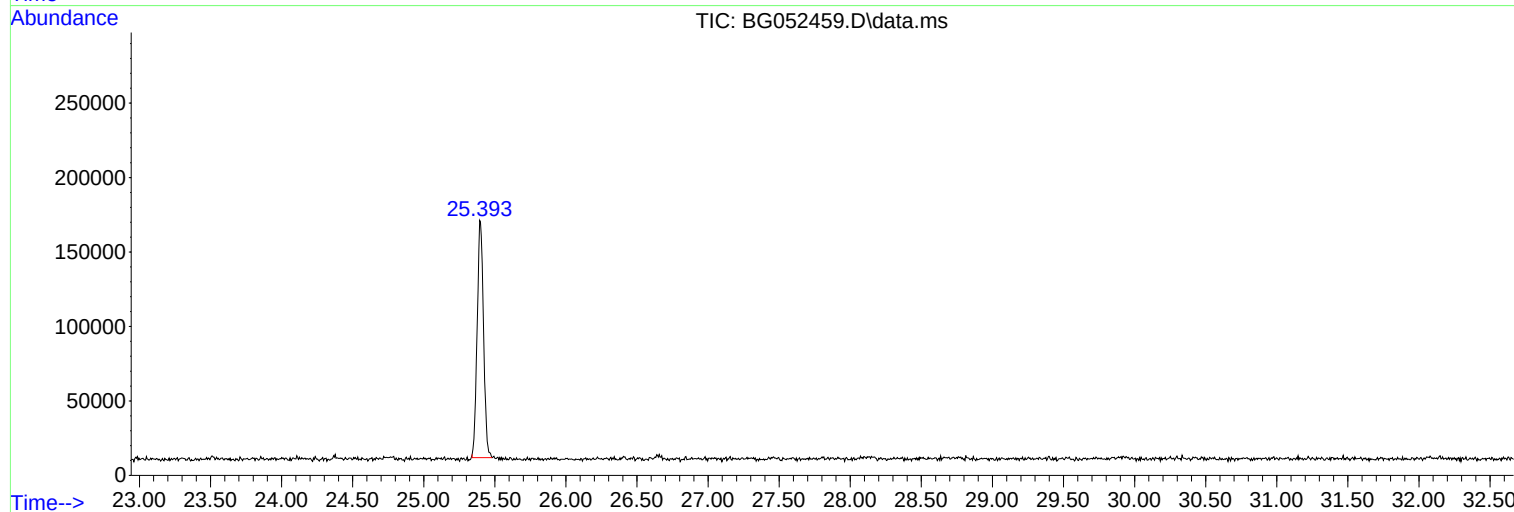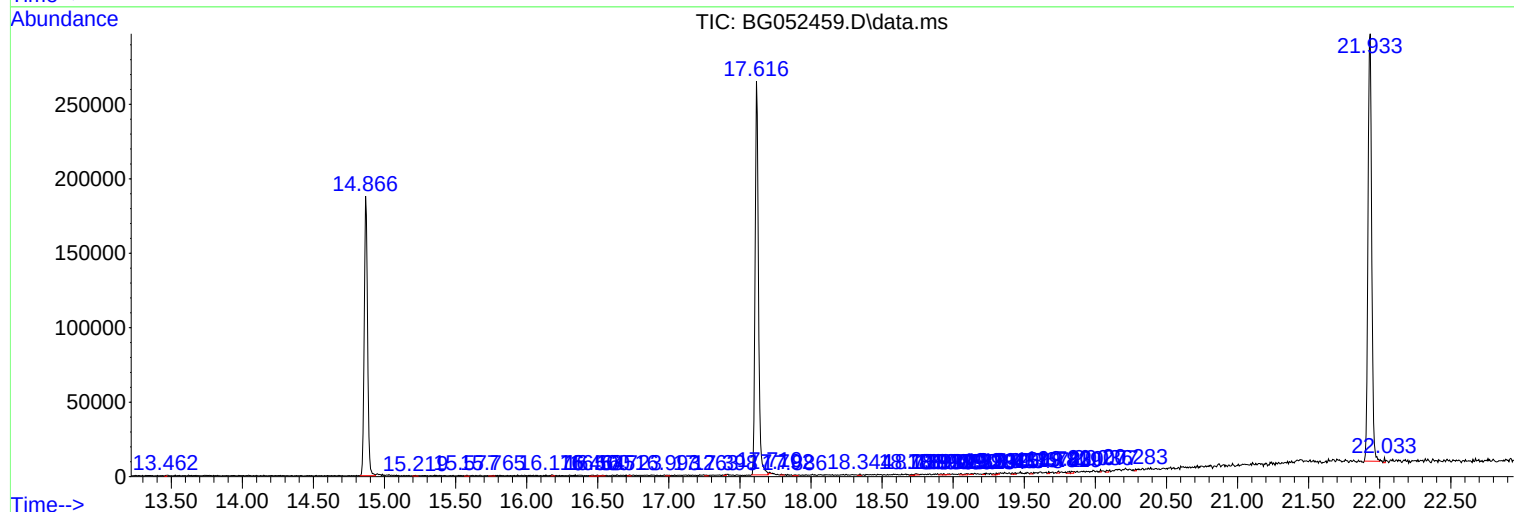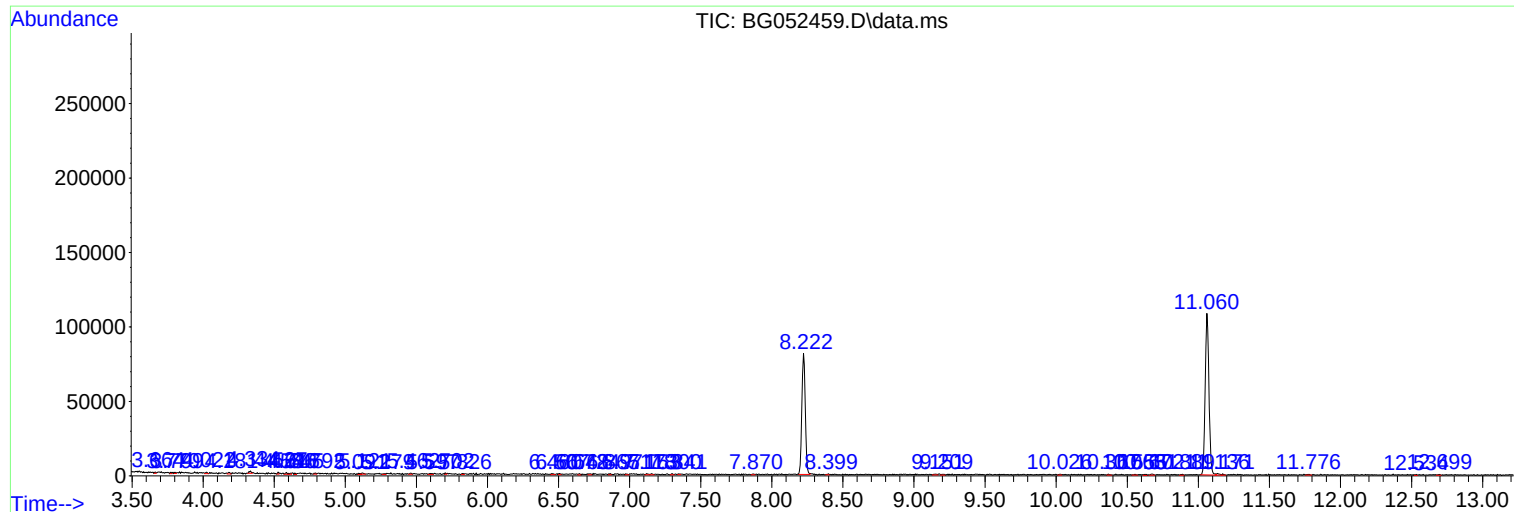

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052459.D
Acq On : 23 Feb 2022 11:01
Operator : CG/JU
Sample : N1616-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052459.D
Acq On : 23 Feb 2022 11:01
Operator : CG/JU
Sample : N1616-10
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc