

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052471.D
 Acq On : 23 Feb 2022 19:37
 Operator : CG/JU
 Sample : PB142851BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK851

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

Signal : TIC: BG052471.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.547	6	10	17	rVB2	8227	12666	1.44%	0.151%
2	3.975	79	83	98	rBV	81750	144315	16.40%	1.719%
3	4.322	140	142	147	rBV2	1486	2336	0.27%	0.028%
4	7.365	653	660	671	rBV	107807	184056	20.92%	2.192%
5	7.529	682	688	696	rBV	82037	138310	15.72%	1.647%
6	7.747	715	725	735	rBV	102273	175674	19.97%	2.092%
7	8.223	797	806	814	rVV	85851	149164	16.95%	1.777%
8	8.928	919	926	941	rVB	125053	222746	25.32%	2.653%
9	9.392	997	1005	1016	rVB	102685	187995	21.37%	2.239%
10	10.126	1123	1130	1140	rVV2	89085	160178	18.21%	1.908%
11	10.678	1217	1224	1239	rBV	113564	217015	24.67%	2.585%
12	11.060	1282	1289	1296	rBV	119658	215335	24.48%	2.565%
13	11.183	1304	1310	1323	rBV	117263	228074	25.92%	2.716%
14	12.640	1551	1558	1566	rBV4	1981	4249	0.48%	0.051%
15	14.256	1826	1833	1845	rBV	271428	401034	45.58%	4.777%
16	14.561	1878	1885	1899	rBV	289794	456802	51.92%	5.441%
17	14.867	1930	1937	1945	rVB	212910	326943	37.16%	3.894%
18	15.055	1961	1969	1984	rBV3	76318	163147	18.54%	1.943%
19	15.166	1987	1988	1992	rVV3	2267	2914	0.33%	0.035%
20	15.219	1992	1997	1999	rVV5	1715	2630	0.30%	0.031%
21	15.854	2099	2105	2113	rBV	372758	575244	65.38%	6.851%
22	15.971	2119	2125	2135	rBV	96619	156050	17.74%	1.859%
23	16.041	2135	2137	2140	rVV2	1757	2305	0.26%	0.027%
24	16.100	2143	2147	2150	rBV2	1377	1815	0.21%	0.022%
25	17.616	2398	2405	2415	rVV	304539	456817	51.92%	5.441%
26	17.716	2415	2422	2434	rVB2	447618	686963	78.08%	8.182%
27	19.337	2695	2698	2705	rBV3	864	2193	0.25%	0.026%
28	19.560	2732	2736	2742	rVB5	6332	10208	1.16%	0.122%
29	19.631	2742	2748	2752	rBV4	6509	11070	1.26%	0.132%
30	19.883	2787	2791	2794	rBV4	1291	1466	0.17%	0.017%
31	19.995	2803	2810	2822	rVV	620219	879792	100.00%	10.479%
32	20.136	2831	2834	2836	rBV3	1394	1349	0.15%	0.016%
33	20.224	2845	2849	2850	rBV3	1432	1722	0.20%	0.021%
34	20.806	2946	2948	2951	rBV3	2180	2296	0.26%	0.027%
35	21.205	3012	3016	3017	rVB4	1590	1809	0.21%	0.022%
36	21.381	3044	3046	3048	rVB3	2665	1673	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052471.D
 Acq On : 23 Feb 2022 19:37
 Operator : CG/JU
 Sample : PB142851BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK851

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

37	21.422	3052	3053	3061	rVB7	3225	5789	0.66%	0.069%
38	21.522	3068	3070	3073	rBV4	2538	2031	0.23%	0.024%
39	21.575	3077	3079	3081	rVB3	2270	1597	0.18%	0.019%
40	21.622	3086	3087	3091	rBV3	2911	3345	0.38%	0.040%
41	21.928	3132	3139	3147	rBV	319169	543957	61.83%	6.479%
42	22.004	3150	3152	3153	rVV2	2915	1681	0.19%	0.020%
43	22.039	3157	3158	3160	rBV2	2199	1713	0.19%	0.020%
44	22.110	3168	3170	3173	rVB3	2048	1403	0.16%	0.017%
45	22.315	3203	3205	3207	rBV2	1676	1732	0.20%	0.021%
46	22.374	3213	3215	3217	rBV3	1751	1468	0.17%	0.017%
47	22.456	3226	3229	3230	rBV3	1718	1573	0.18%	0.019%
48	22.856	3296	3297	3299	rVB2	2137	1478	0.17%	0.018%
49	23.167	3348	3350	3351	rVB2	3340	1833	0.21%	0.022%
50	23.414	3390	3392	3394	rBV3	2311	2664	0.30%	0.032%
51	23.467	3396	3401	3402	rVV5	2893	4145	0.47%	0.049%
52	23.502	3402	3407	3414	rVB6	9199	19324	2.20%	0.230%
53	24.183	3521	3523	3526	rBV4	1705	1409	0.16%	0.017%
54	24.272	3535	3538	3539	rBV3	2204	2590	0.29%	0.031%
55	24.319	3543	3546	3547	rVV3	2496	2524	0.29%	0.030%
56	24.371	3550	3555	3563	rVB6	11097	25122	2.86%	0.299%
57	24.512	3577	3579	3583	rVB5	1672	2052	0.23%	0.024%
58	24.565	3586	3588	3589	rBV2	2087	1684	0.19%	0.020%
59	24.706	3611	3612	3615	rBV3	2505	2178	0.25%	0.026%
60	24.747	3617	3619	3621	rVB2	1919	1791	0.20%	0.021%
61	25.153	3675	3688	3701	rBV3	281150	854293	97.10%	10.175%
62	25.394	3718	3729	3744	rVB2	182127	565693	64.30%	6.738%
63	25.681	3776	3778	3780	rBV2	1596	1547	0.18%	0.018%
64	25.769	3789	3793	3796	rBV5	2017	3103	0.35%	0.037%
65	25.846	3805	3806	3811	rVB5	2270	2214	0.25%	0.026%
66	26.345	3889	3891	3893	rVB3	2013	1558	0.18%	0.019%
67	26.580	3930	3931	3933	rBV2	2098	1829	0.21%	0.022%
68	26.639	3933	3941	3950	rVB5	15705	43942	4.99%	0.523%
69	26.815	3969	3971	3973	rBV3	1713	1471	0.17%	0.018%
70	27.203	4036	4037	4039	rBV2	1782	1521	0.17%	0.018%
71	27.350	4060	4062	4063	rVB2	2424	1333	0.15%	0.016%
72	27.450	4075	4079	4080	rBV4	2805	2656	0.30%	0.032%
73	27.491	4084	4086	4089	rBV3	1727	2051	0.23%	0.024%
74	27.579	4099	4101	4104	rVB3	2443	2570	0.29%	0.031%
75	27.814	4139	4141	4142	rBV2	2167	1376	0.16%	0.016%
76	27.855	4145	4148	4149	rBV3	2304	1533	0.17%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
 Data File : BG052471.D
 Acq On : 23 Feb 2022 19:37
 Operator : CG/JU
 Sample : PB142851BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK851

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
 Title : SVOA CALIBRATION

77	27.908	4155	4157	4159	rVB3	2639	1742	0.20%	0.021%
78	27.967	4166	4167	4170	rVV2	1766	1374	0.16%	0.016%
79	28.119	4184	4193	4194	rBV6	13032	27088	3.08%	0.323%
80	28.243	4212	4214	4215	rBV2	2234	1832	0.21%	0.022%
81	28.284	4219	4221	4222	rBV2	1692	1520	0.17%	0.018%
82	28.337	4229	4230	4232	rVB2	2218	1449	0.16%	0.017%
83	28.442	4245	4248	4249	rBV3	2486	2699	0.31%	0.032%
84	28.936	4330	4332	4333	rVB2	2714	1386	0.16%	0.017%
85	29.177	4370	4373	4376	rBV3	2807	3320	0.38%	0.040%
86	29.206	4376	4378	4380	rVB2	2295	1512	0.17%	0.018%
87	29.617	4446	4448	4450	rBV3	2721	2171	0.25%	0.026%
88	29.652	4452	4454	4457	rVB4	1678	1375	0.16%	0.016%
89	29.899	4488	4496	4497	rBV7	8455	16445	1.87%	0.196%
90	30.381	4574	4578	4579	rBV4	2063	2259	0.26%	0.027%
91	30.516	4599	4601	4603	rBV3	1587	1408	0.16%	0.017%
92	30.586	4611	4613	4615	rVB3	2001	1800	0.20%	0.021%
93	31.133	4704	4706	4707	rVB2	2181	1509	0.17%	0.018%
94	31.244	4723	4725	4727	rVV2	2287	1678	0.19%	0.020%
95	31.268	4727	4729	4730	rVB2	2966	1718	0.20%	0.020%
96	31.421	4753	4755	4758	rBV4	1872	2344	0.27%	0.028%
97	31.579	4780	4782	4785	rVB4	1936	1423	0.16%	0.017%
98	32.026	4856	4858	4859	rBV2	3071	2169	0.25%	0.026%
99	32.278	4899	4901	4904	rVB2	3025	2285	0.26%	0.027%
100	32.302	4904	4905	4907	rBV2	2230	1332	0.15%	0.016%




Sum of corrected areas: 8395966

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052471.D
Acq On : 23 Feb 2022 19:37
Operator : CG/JU
Sample : PB142851BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK851

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

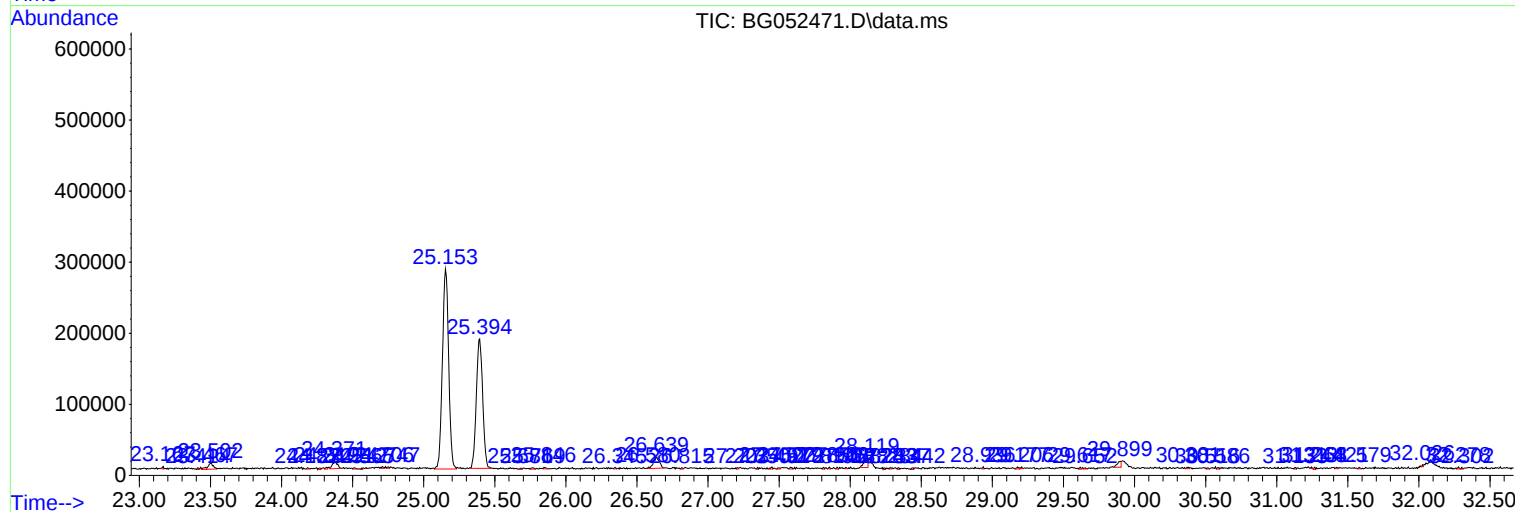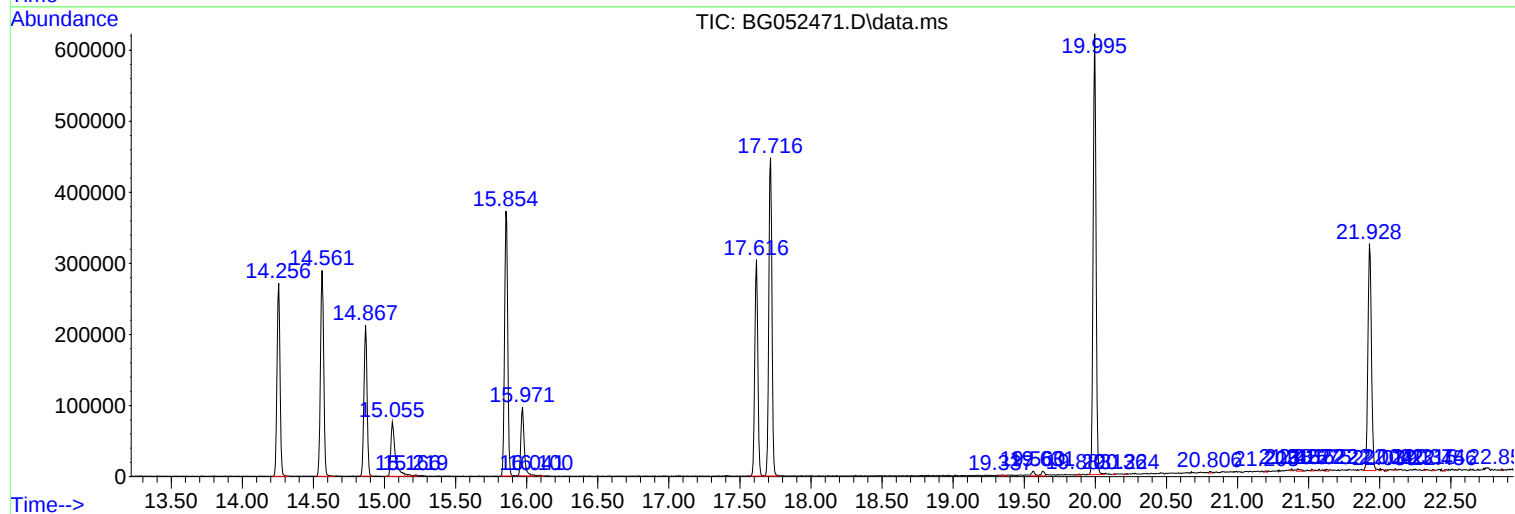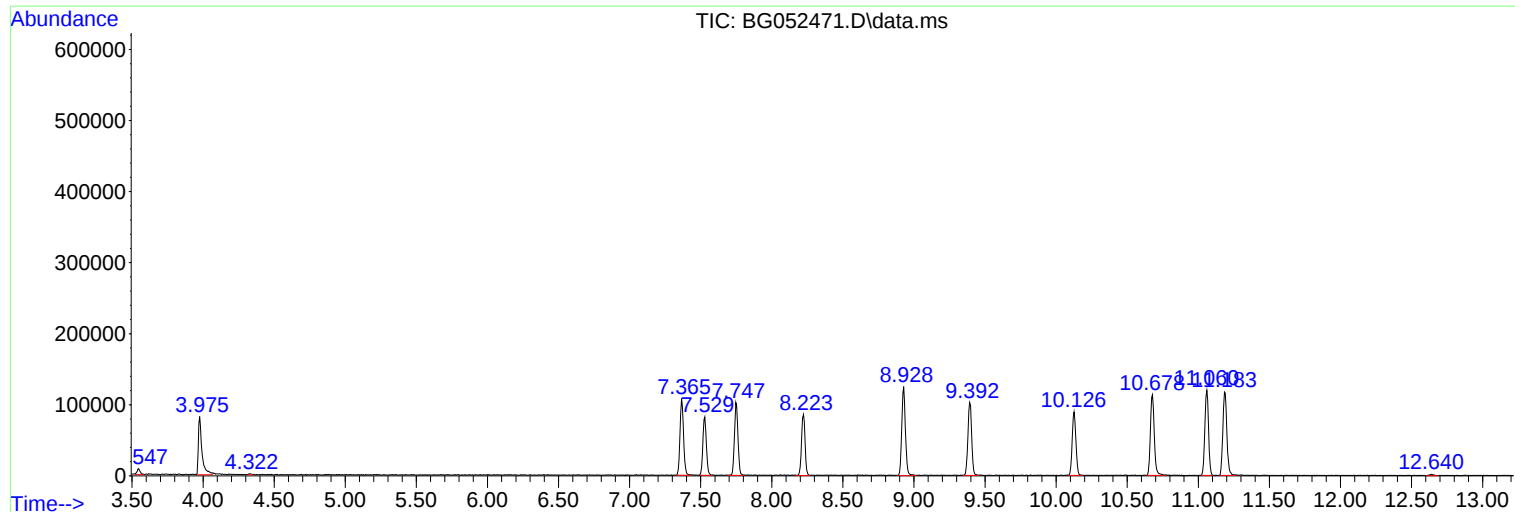

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052471.D
Acq On : 23 Feb 2022 19:37
Operator : CG/JU
Sample : PB142851BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK851

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022322\
Data File : BG052471.D
Acq On : 23 Feb 2022 19:37
Operator : CG/JU
Sample : PB142851BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK851

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------