

Data Path : U:\HPCHEM1\BNA G\DATA\BG022416\
 Data File : BG021063.D
 Acq On : 24 Feb 2016 22:31
 Operator : UM/SJ
 Sample : H1521-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Feb 24 23:59:44 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022316.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 24 00:35:06 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.20	152	4987	20.00	ng	0.00
21) Naphthalene-d8	11.02	136	25898	20.00	ng	0.00
38) Acenaphthene-d10	14.82	164	12558	20.00	ng	0.00
63) Phenanthrene-d10	17.55	188	22140	20.00	ng	0.00
75) Chrysene-d12	21.83	240	16144	20.00	ng	0.00
86) Perylene-d12	25.16	264	14651	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.78	112	40506	142.40	ng	0.00
7) Phenol-d6	7.41	99	63139	144.13	ng	0.00
23) Nitrobenzene-d5	9.39	82	42935	97.34	ng	0.00
41) 2,4,6-Tribromophenol	16.31	330	19886	132.18	ng	0.00
44) 2-Fluorobiphenyl	13.45	172	81087	89.89	ng	0.00
78) Terphenyl-d14	20.14	244	60318	48.48	ng	0.00
Target Compounds						Qvalue
49) Dimethylphthalate	14.27	163	18580	18.14	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : U:\HPCHEM1\BNA G\DATA\BG022416\
Data File : BG021063.D
Acq On : 24 Feb 2016 22:31
Operator : UM/SJ
Sample : H1521-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Feb 24 23:59:44 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

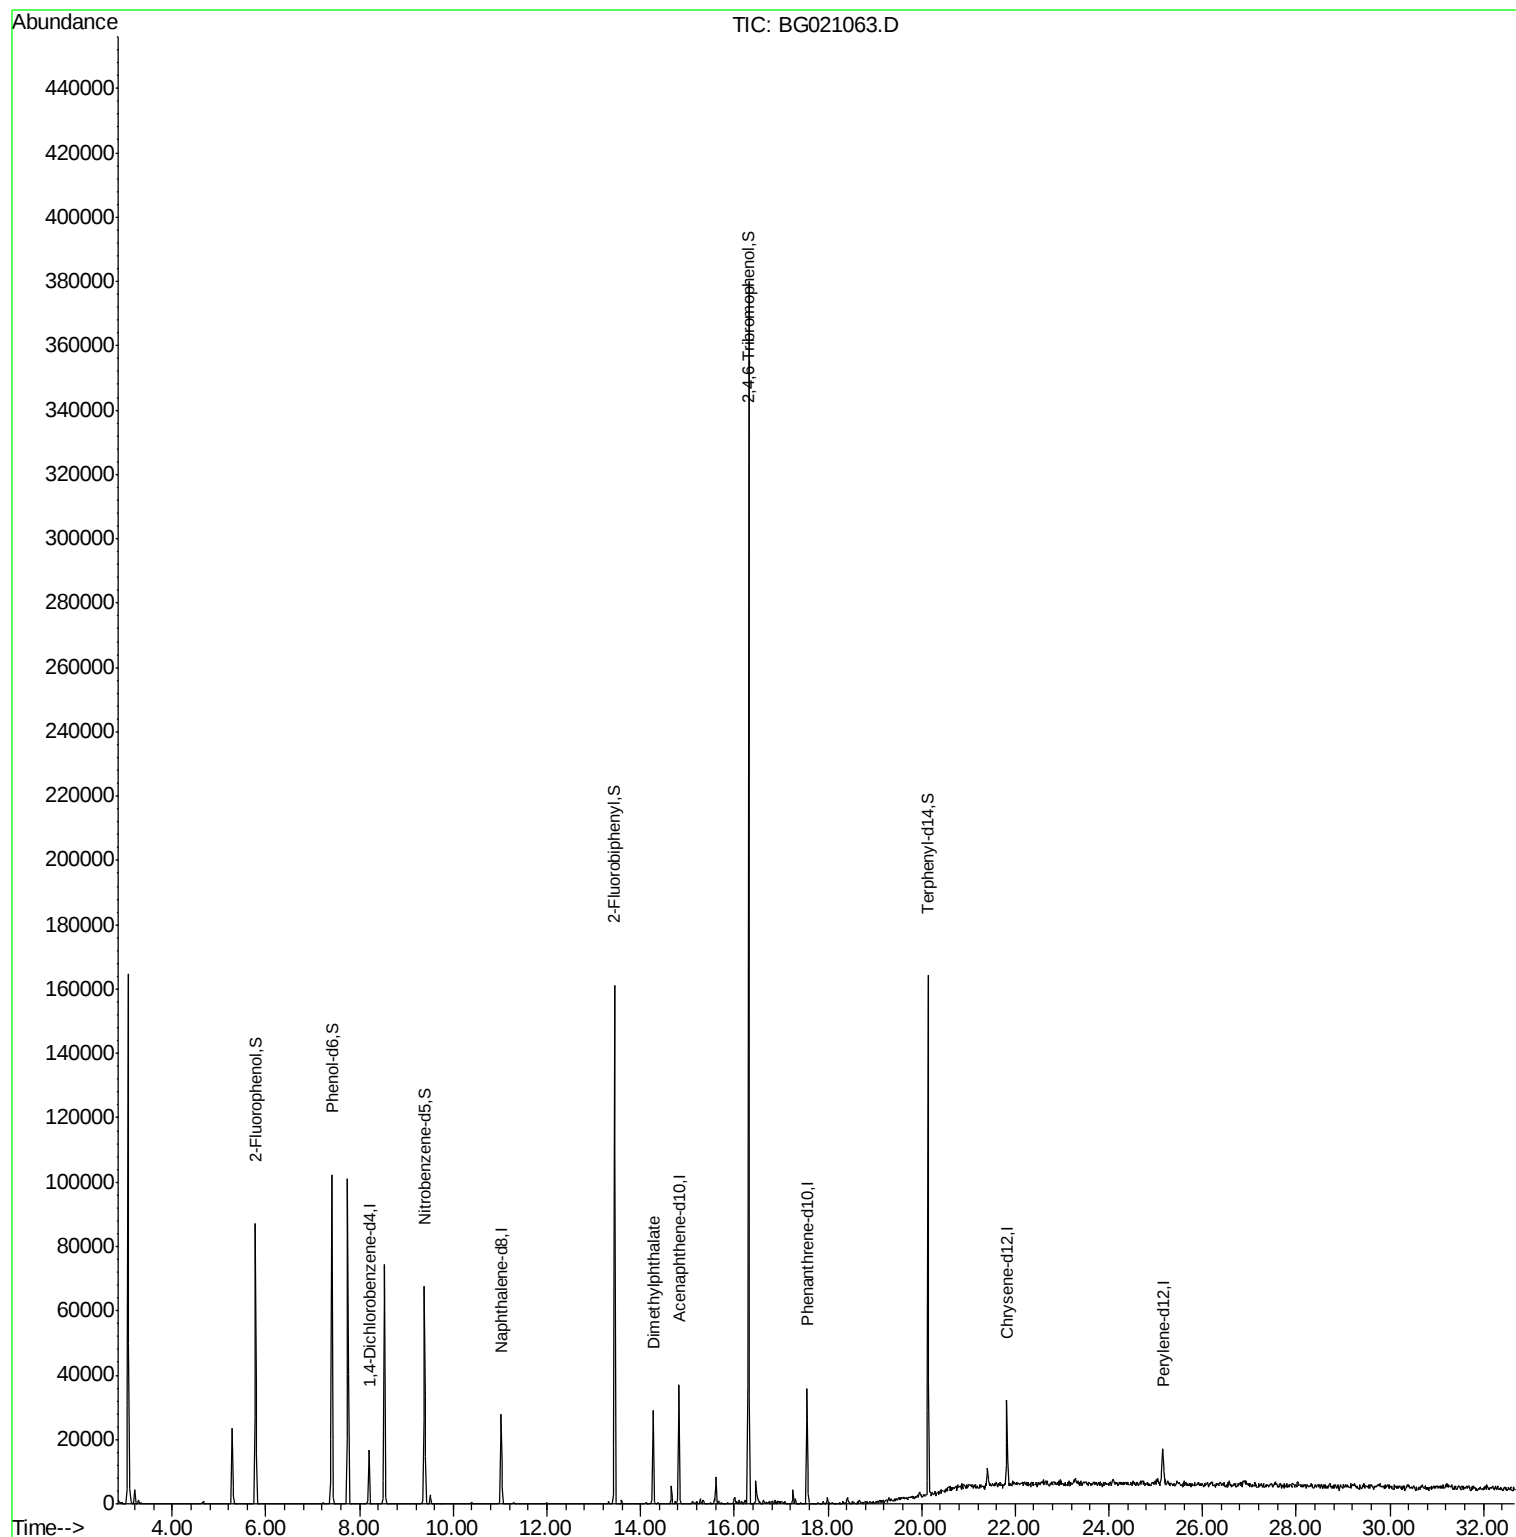

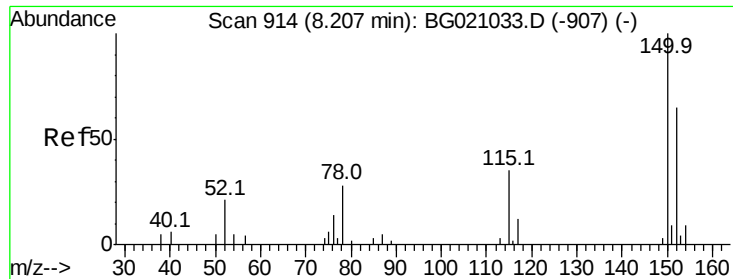


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.20 min Scan# 913
Delta R.T. -0.00 min
Lab File: BG021063.D
Acq: 24 Feb 2016 22:31

Instrument :
BNA_G
ClientSampleId :

Tot Ion:152 Resp: 4987
Ion Ratio Lower Upper
152 100
150 161.8 123.4 185.2
115 61.2 43.3 64.9

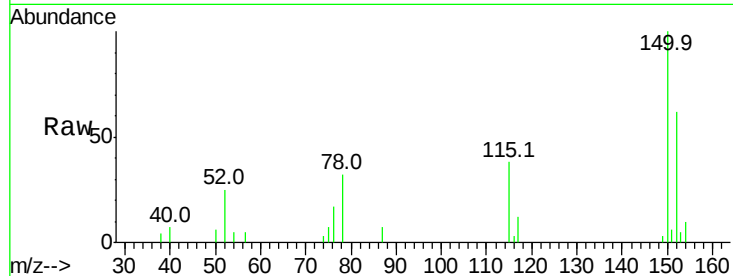


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

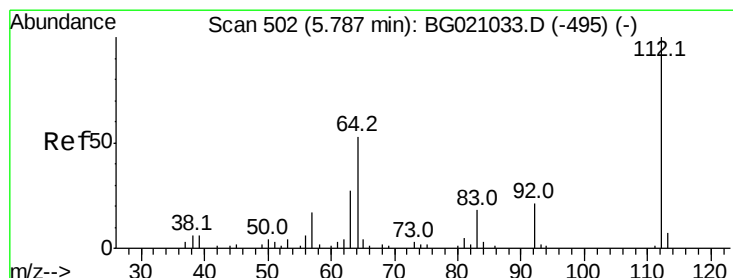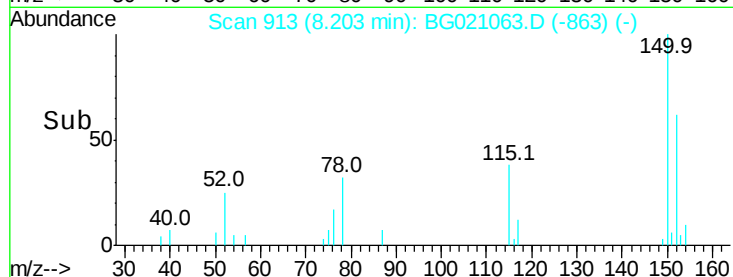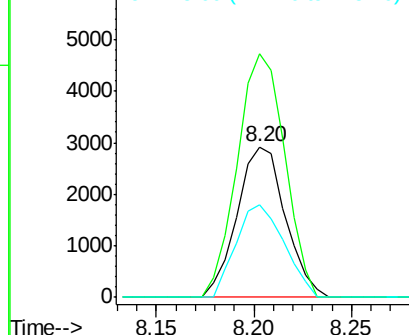



#5


2-Fluorophenol
Concen: 142.40 ng
RT: 5.78 min Scan# 501
Delta R.T. -0.00 min
Lab File: BG021063.D
Acq: 24 Feb 2016 22:31

Tgt Ion:112 Resp: 40506
Ion Ratio Lower Upper
112 100
64 60.0 42.6 63.8
63 30.9 21.7 32.5

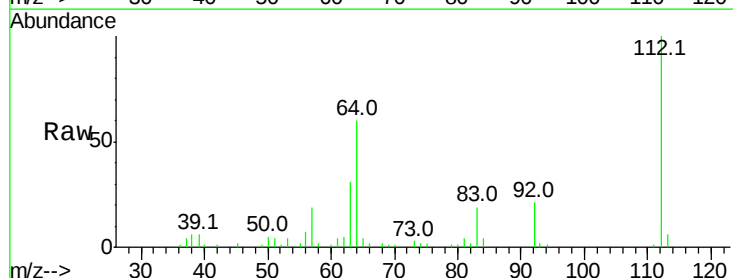

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGC
Ion 63.00 (62.70 to 63.70): BGC

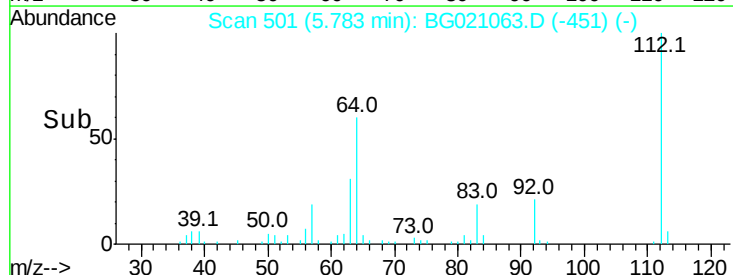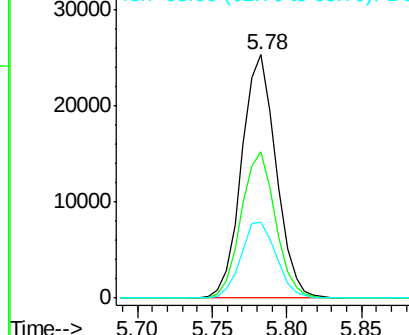

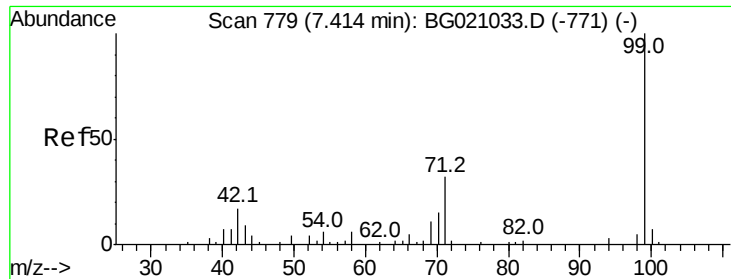

#7

Phenol-d6

Concen: 144.13 ng

RT: 7.41 min Scan# 778

Delta R.T. -0.00 min

Lab File: BG021063.D

Acq: 24 Feb 2016 22:31

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 63139

Ion Ratio Lower Upper




99 100

42 18.3 13.2 19.8

71 32.8 25.2 37.8

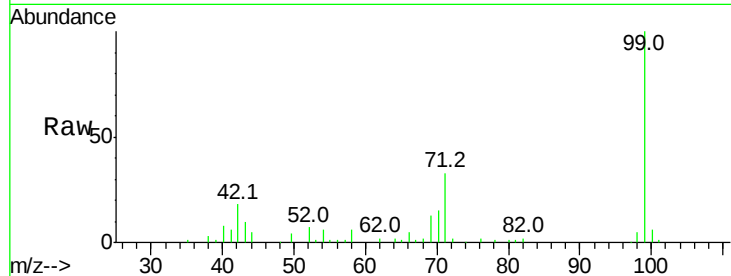

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

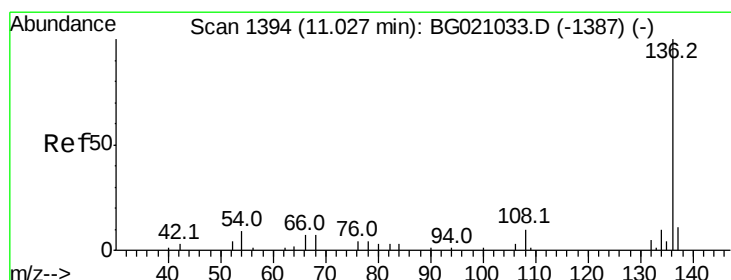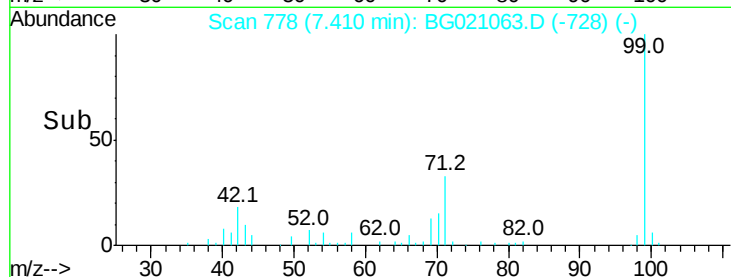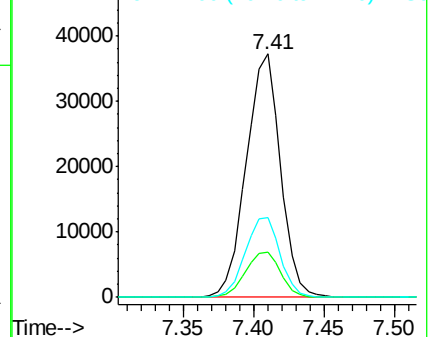

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 11.02 min Scan# 1393

Delta R.T. -0.00 min

Lab File: BG021063.D

Acq: 24 Feb 2016 22:31

Tgt Ion: 136 Resp: 25898


Ion Ratio Lower Upper

136 100



137 11.2 8.8 13.2


54 8.1 6.9 10.3

68 6.0 5.8 8.6

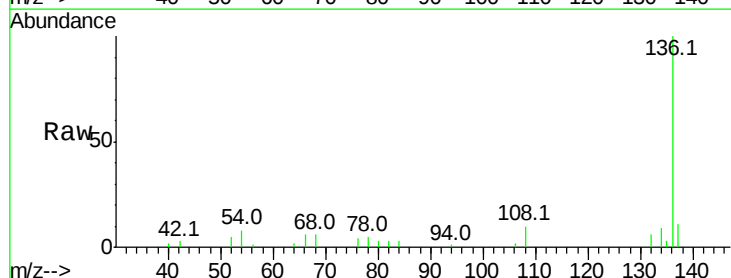

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



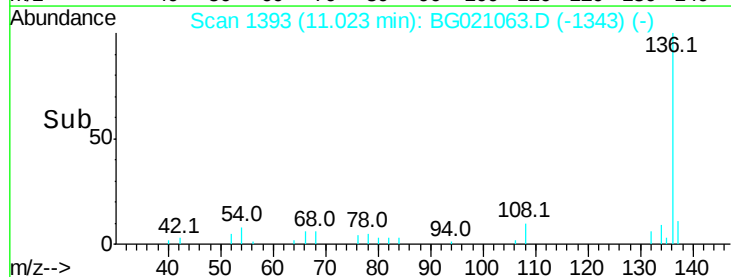
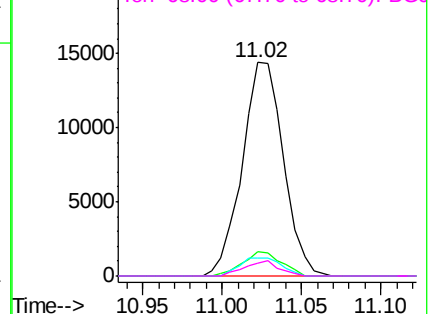


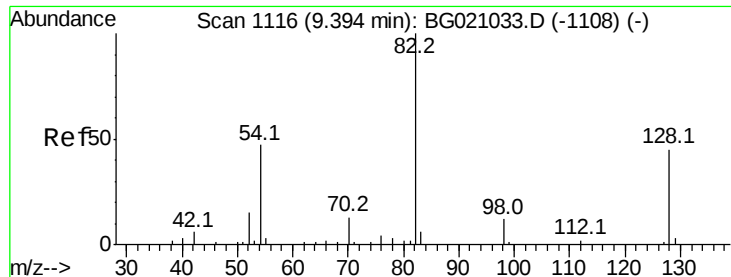

#23
Nitrobenzene-d5
Concen: 97.34 ng
RT: 9.39 min Scan# 1115
Delta R.T. -0.00 min
Lab File: BG021063.D
Acq: 24 Feb 2016 22:31




Instrument :
BNA_G
ClientSampleId :


Tot Ion	82	Resp	42935
Ion Ratio	100	Lower	Upper
128	41.6	36.3	54.5
54	46.6	37.6	56.4

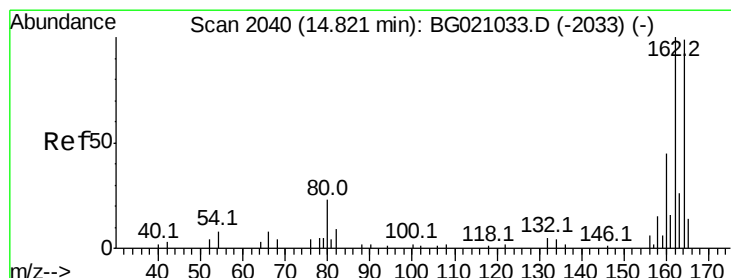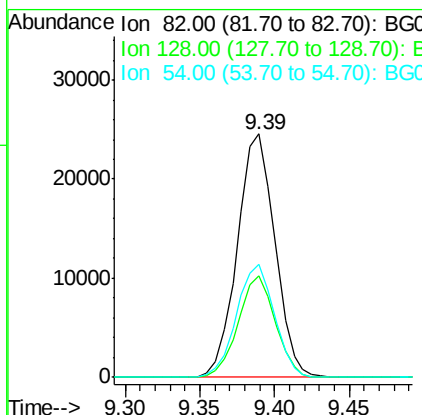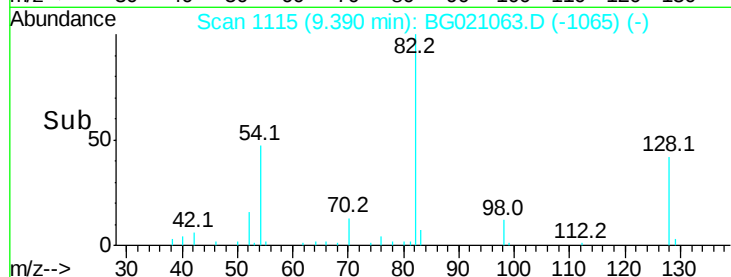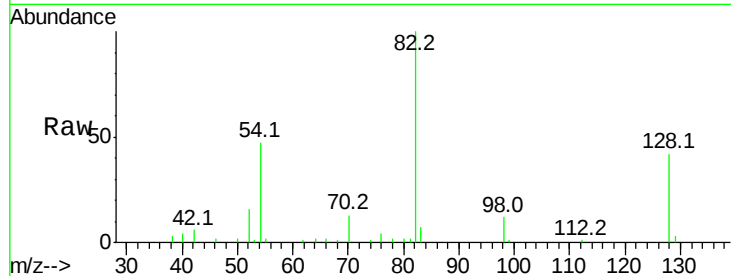

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.82 min Scan# 2039
Delta R.T. -0.00 min
Lab File: BG021063.D
Acq: 24 Feb 2016 22:31

Tgt Ion	164	Resp	12558
Ion Ratio	100	Lower	Upper
162	102.2	80.6	120.8
160	46.0	36.5	54.7

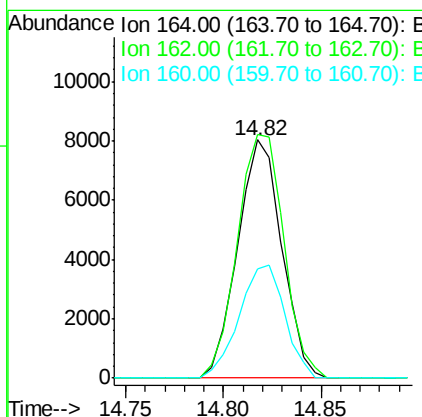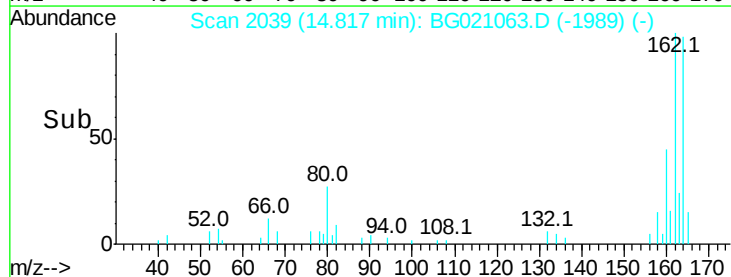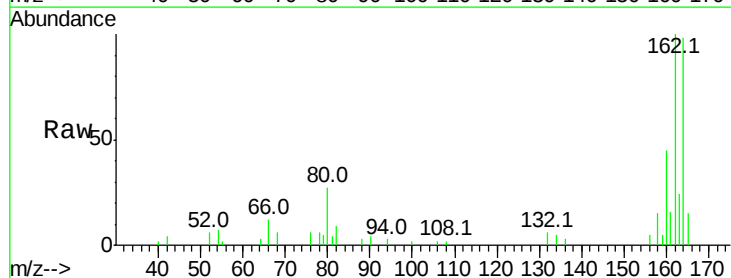


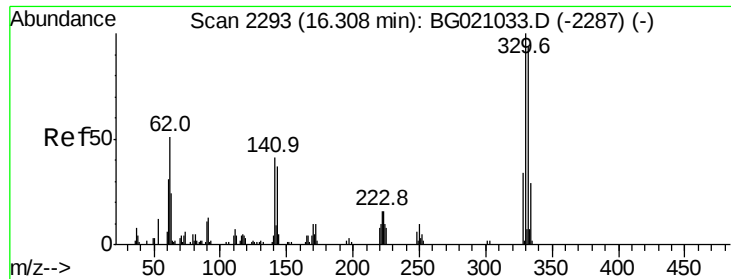




#41
 2,4,6-Tribromophenol
 Concen: 132.18 ng
 RT: 16.31 min Scan# 2293
 Delta R.T. 0.00 min
 Lab File: BG021063.D
 Acq: 24 Feb 2016 22:31

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:330 Resp: 19886
 Ion Ratio Lower Upper
 330 100
 332 97.0 77.4 116.0
 141 43.6 35.3 52.9

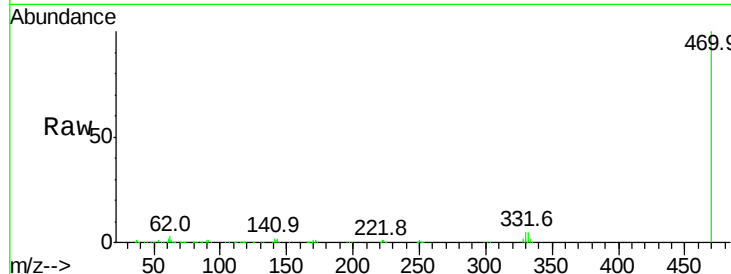


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

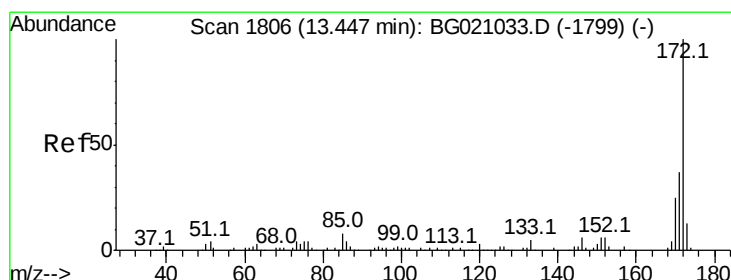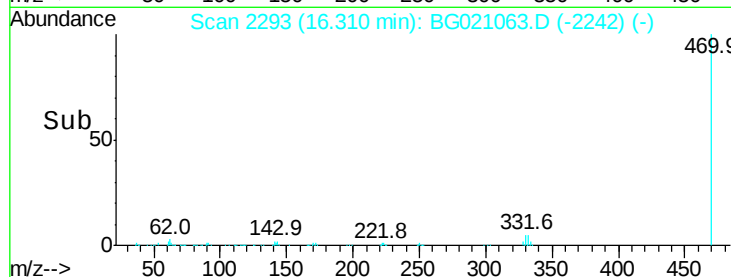
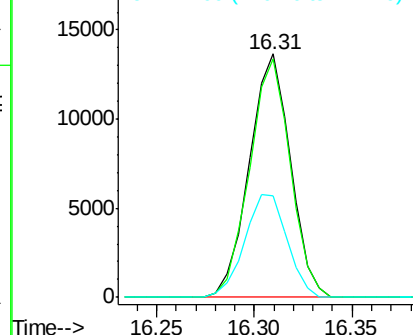



#44
 2-Fluorobiphenyl
 Concen: 89.89 ng
 RT: 13.45 min Scan# 1806
 Delta R.T. 0.00 min
 Lab File: BG021063.D
 Acq: 24 Feb 2016 22:31

Tgt Ion:172 Resp: 81087
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.4 44.0
 170 24.7 19.8 29.8

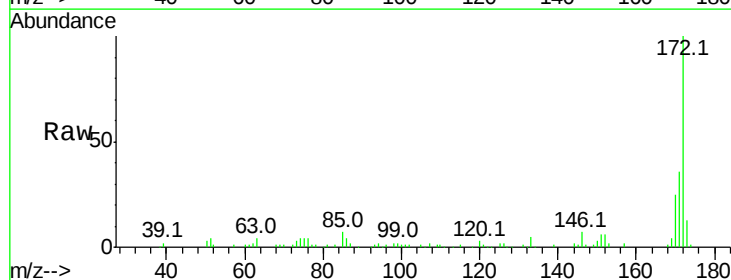

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



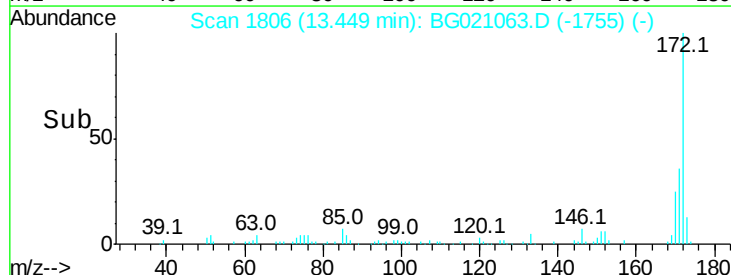
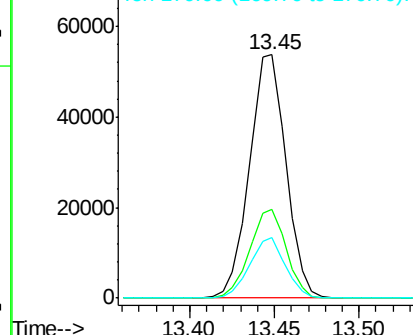


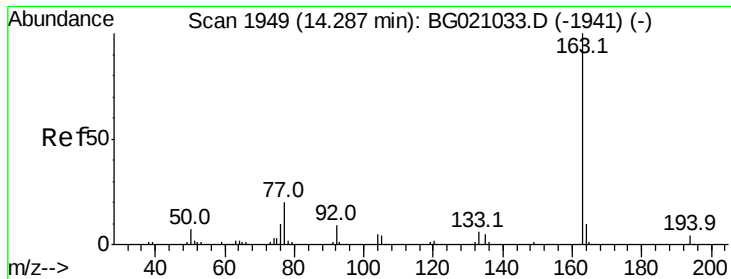

#49
Dimethylphthalate
Concen: 18.14 ng
RT: 14.27 min Scan# 1946
Delta R.T. -0.02 min
Lab File: BG021063.D
Acq: 24 Feb 2016 22:31




Instrument :
BNA_G
ClientSampleId :


Tot Ion:163 Resp: 18580
Ion Ratio Lower Upper
163 100
194 4.7 2.8 4.2#
164 9.7 7.9 11.9

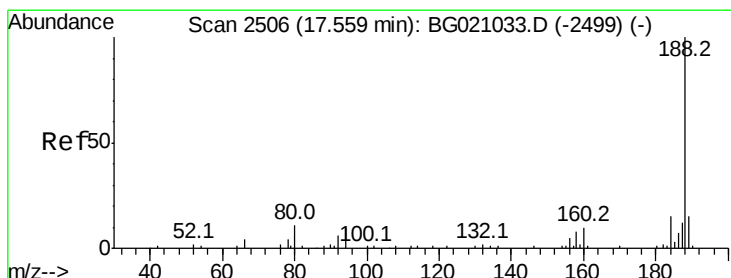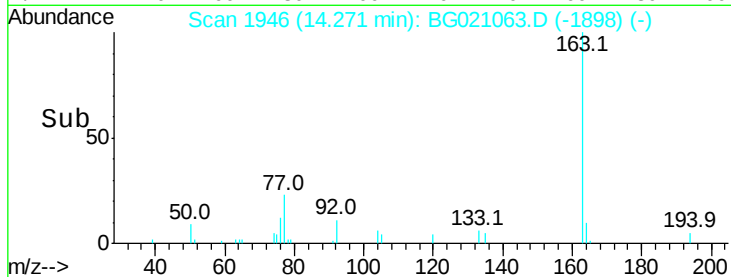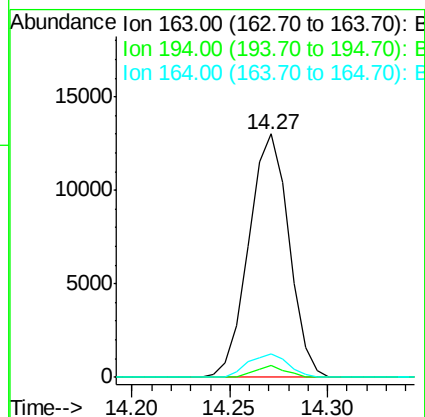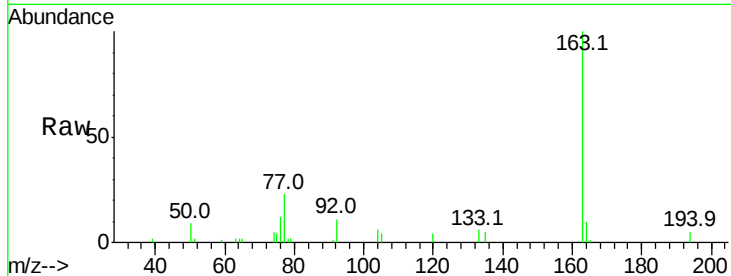

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.55 min Scan# 2505
Delta R.T. -0.00 min
Lab File: BG021063.D
Acq: 24 Feb 2016 22:31

Tgt Ion:188 Resp: 22140
Ion Ratio Lower Upper
188 100
94 10.4 8.2 12.4
80 11.9 9.2 13.8

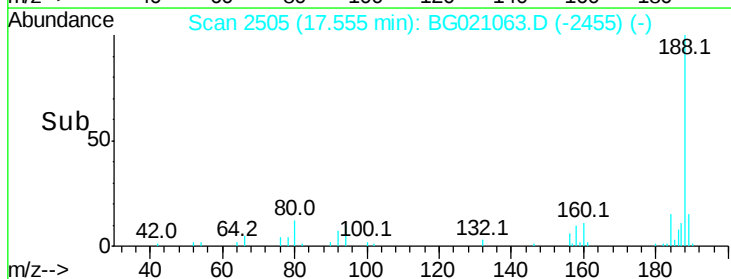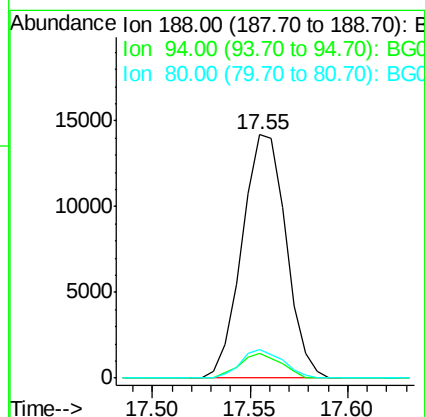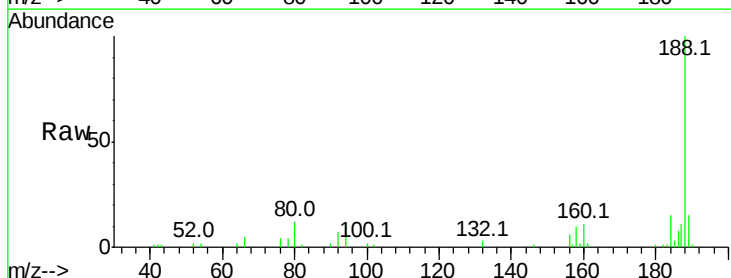

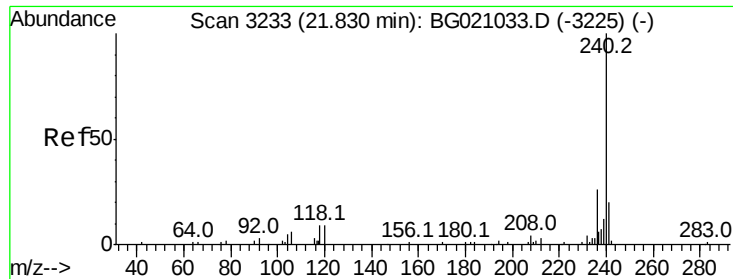

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.83 min Scan# 3232

Delta R.T. -0.00 min

Lab File: BG021063.D

Acq: 24 Feb 2016 22:31

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 16144

Ion Ratio Lower Upper

240 100

120 7.0 7.5 11.3#




236 25.5 20.5 30.7

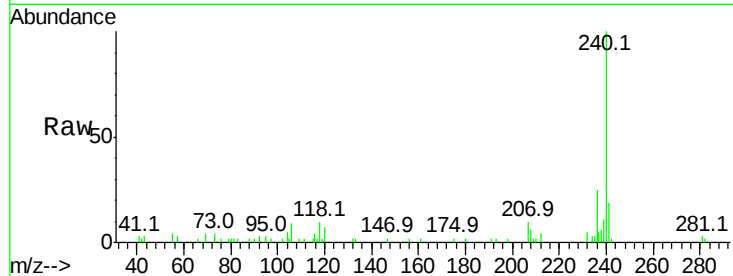

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

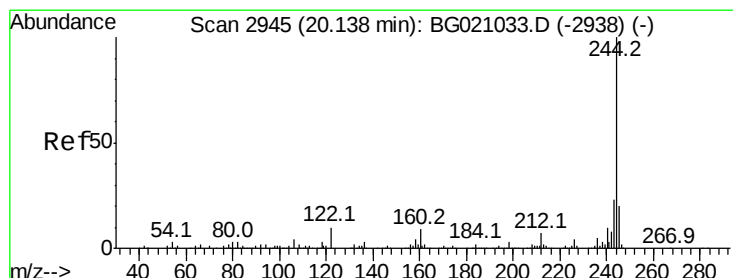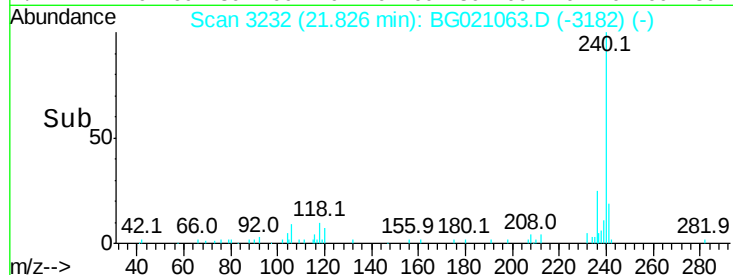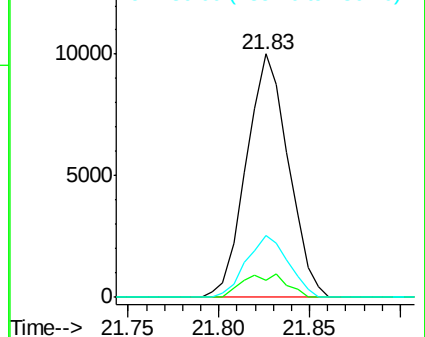

#78

Terphenyl-d14

Concen: 48.48 ng

RT: 20.14 min Scan# 2945

Delta R.T. 0.00 min

Lab File: BG021063.D

Acq: 24 Feb 2016 22:31


Tgt Ion:244 Resp: 60318

Ion Ratio Lower Upper

244 100

212 7.2 5.8 8.6



122 9.5 8.3 12.5

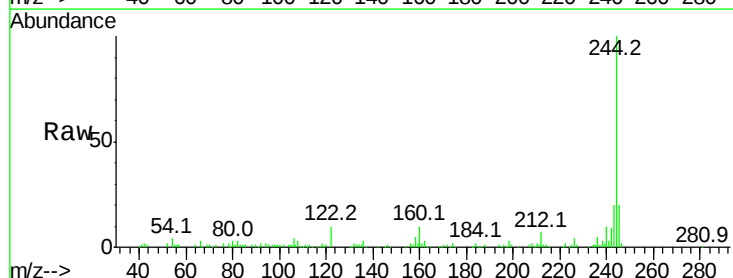


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

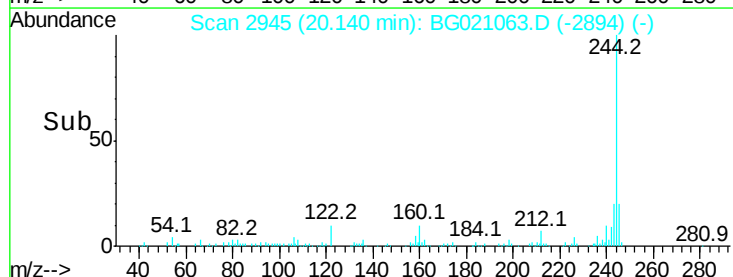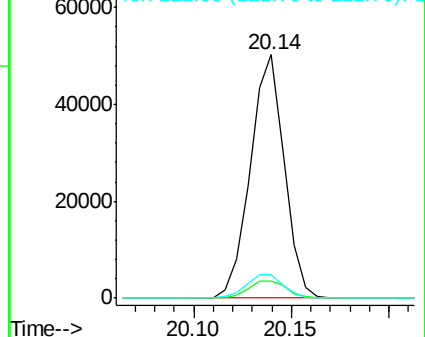


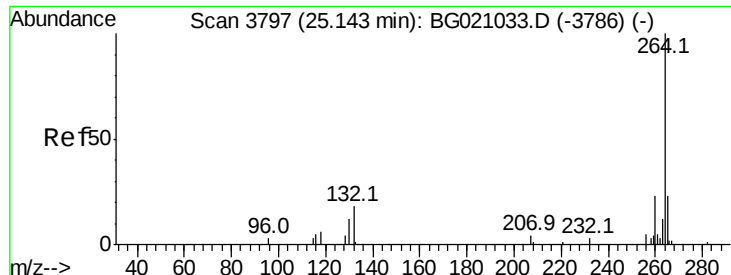

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 25.16 min Scan# 3799
 Delta R.T. 0.01 min
 Lab File: BG021063.D
 Acq: 24 Feb 2016 22:31

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:264 Resp: 14651
 Ion Ratio Lower Upper
 264 100
 260 25.0 18.5 27.7
 265 23.4 18.6 28.0

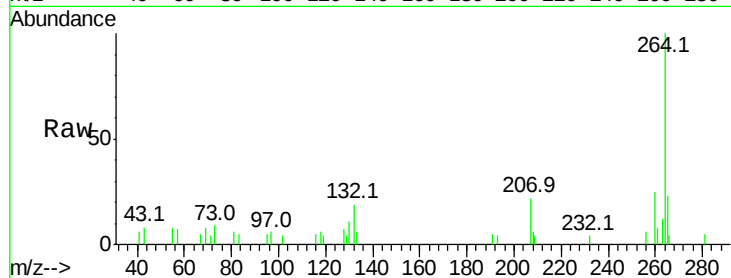

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

