
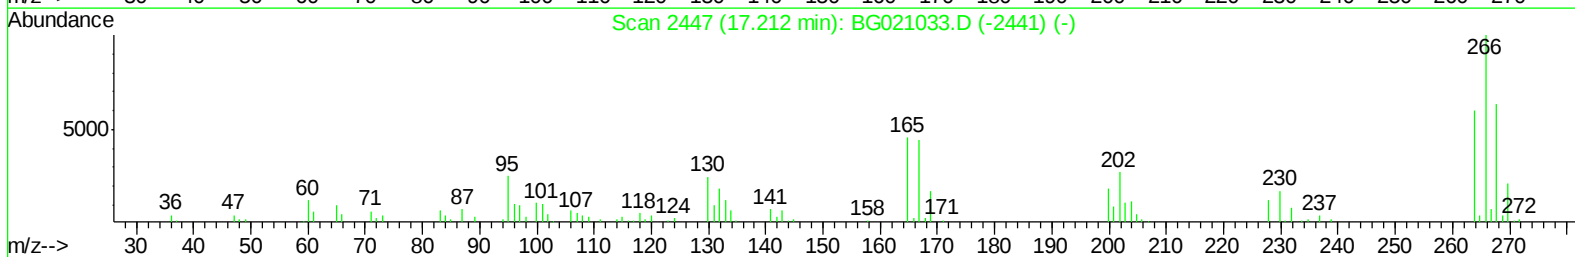
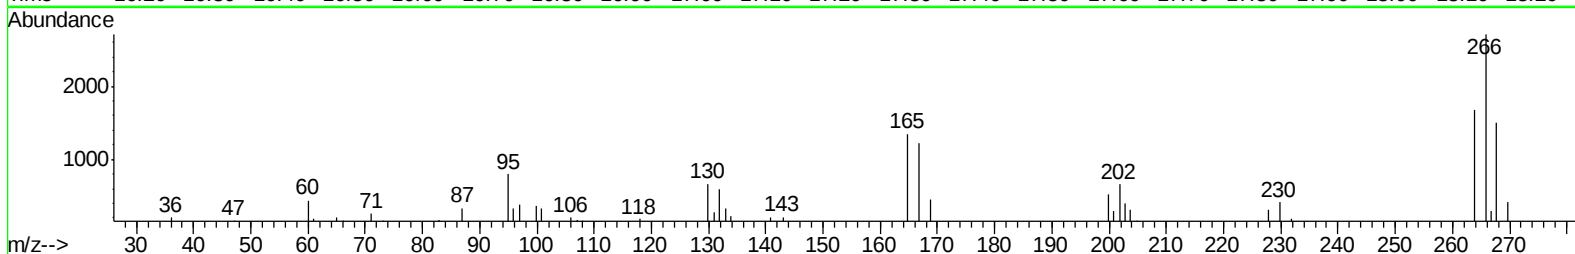


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022416\
Data File : BG021054.D
Acq On : 24 Feb 2016 16:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 17:12:40 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

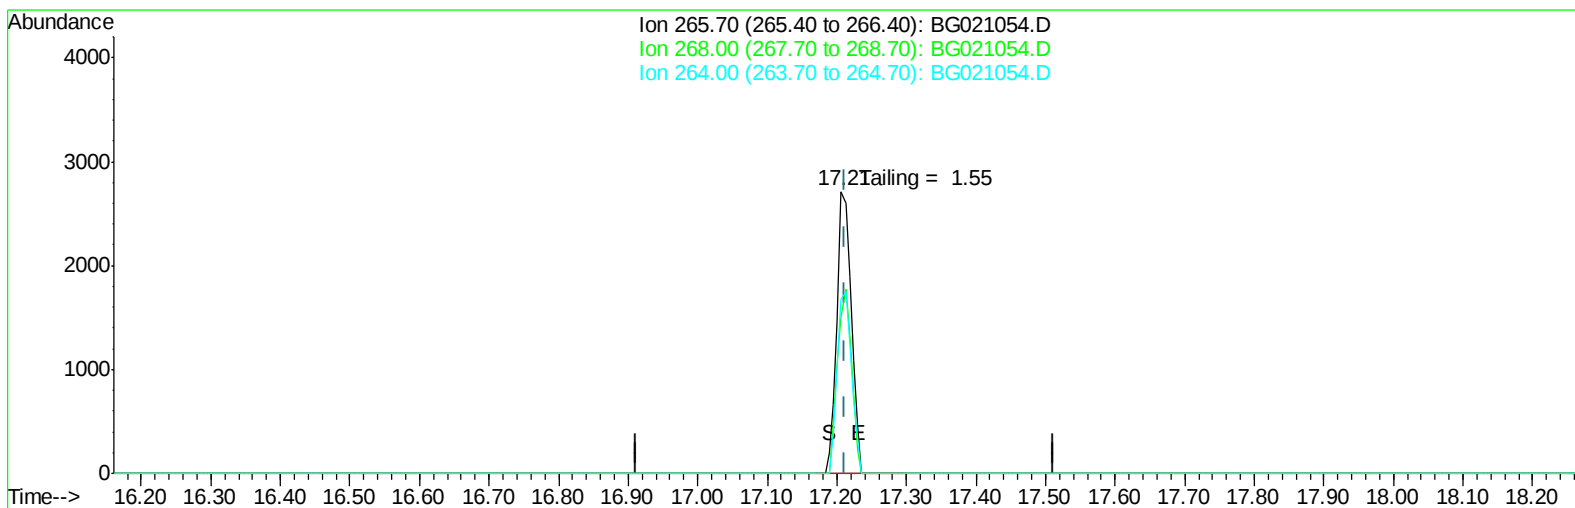

TIC: BG021054.D

(69) Pentachlorophenol (C)




17.206min (-0.006) 0.00ng

response 3912

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	55.40
264.00	59.80	61.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022416\
Data File : BG021054.D
Acq On : 24 Feb 2016 16:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 24 17:12:40 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022316.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 24 00:35:06 2016
Response via : Initial Calibration

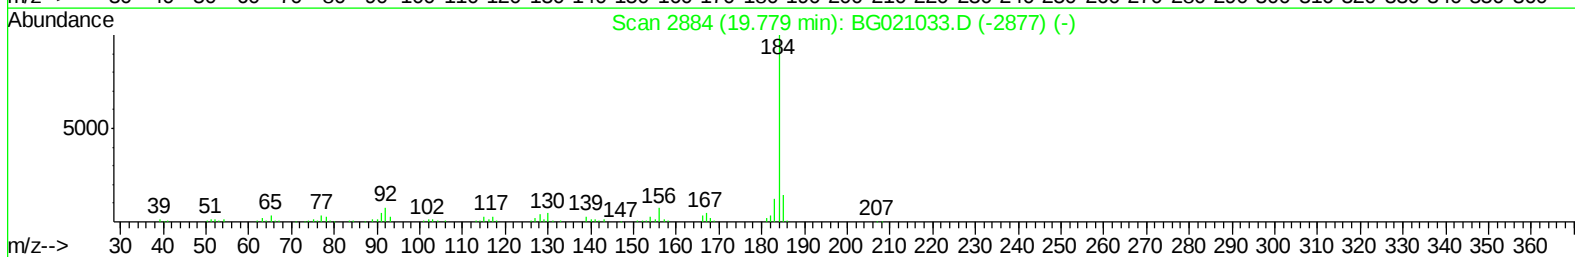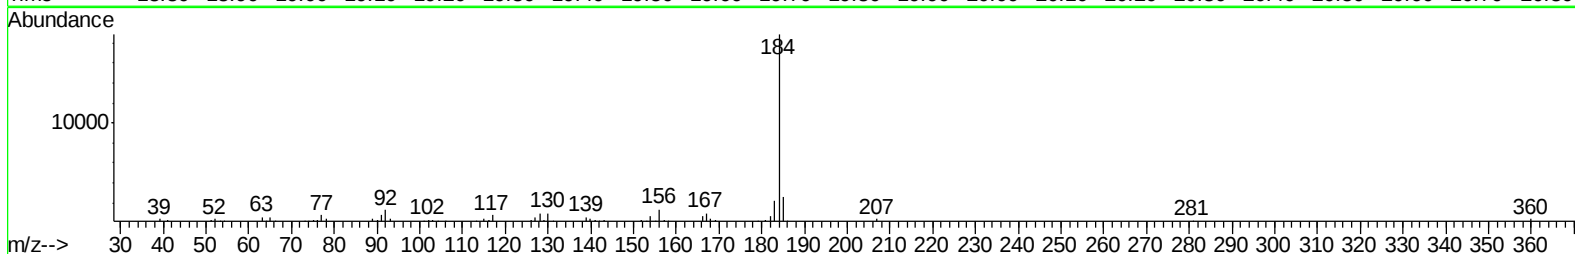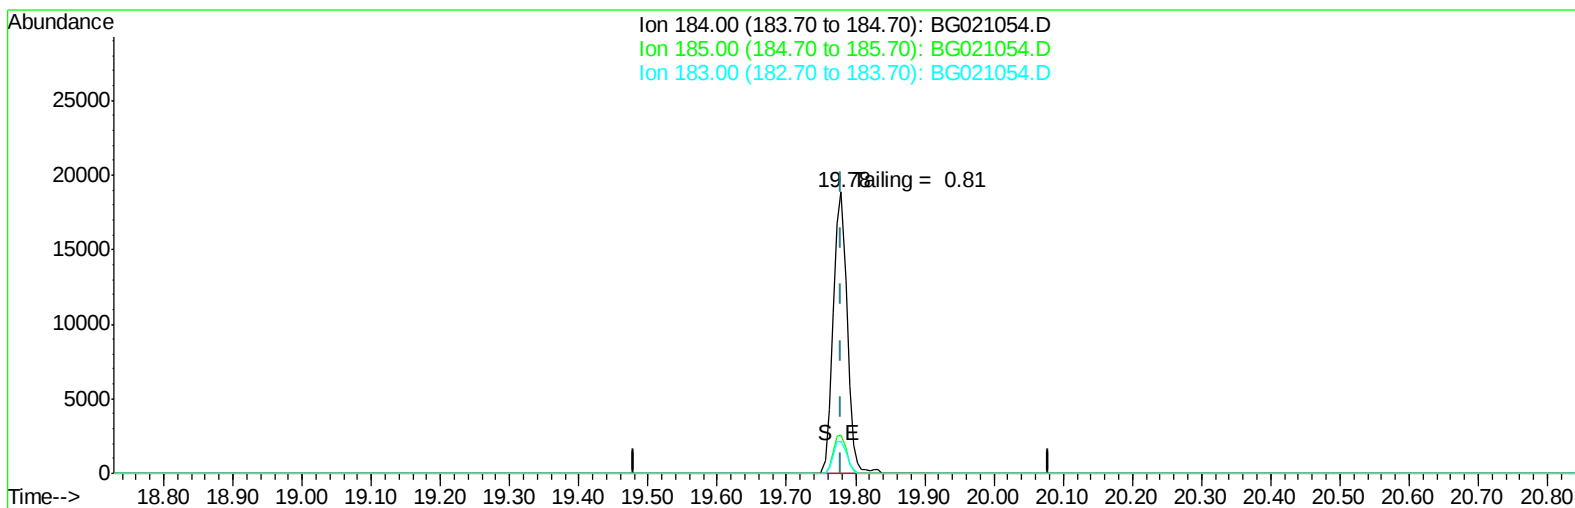

TIC: BG021054.D

(76) Benzidine

19.779min (-0.000) 0.00ng

response 26182

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	13.60
183.00	12.60	11.59
0.00	0.00	0.00