


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022416\
Data File : BG021054.D
Acq On : 24 Feb 2016 16:31
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022316.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 24 00:35:06 2016

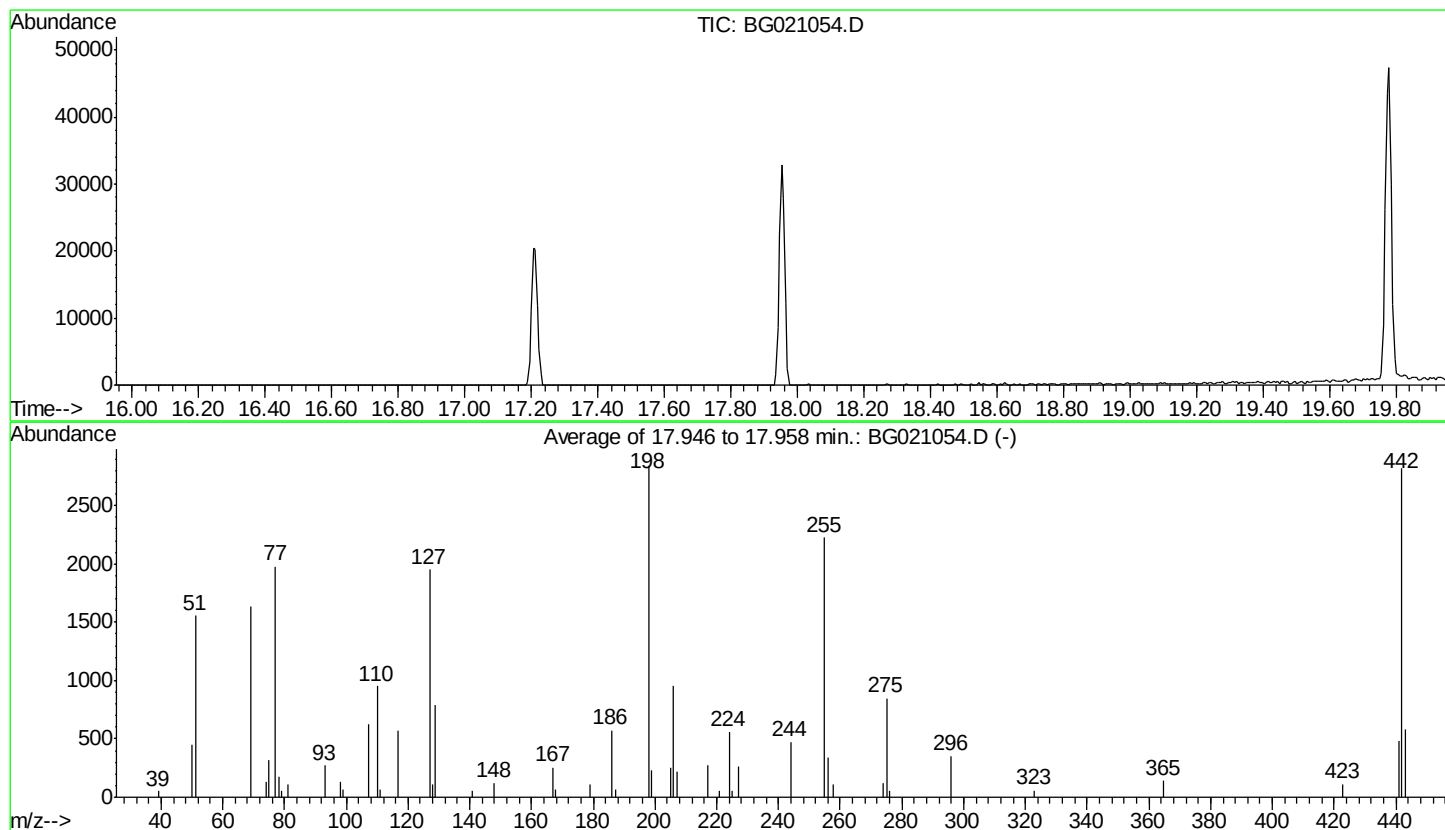

AutoFind: Scans 2572, 2573, 2574; Background Corrected with Scan 2567

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	1554	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	57.4	1631	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	68.7	1953	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	2843	PASS
199	198	5	9	8.0	228	PASS
275	198	10	60	29.8	848	PASS
365	198	1	100	4.9	140	PASS
441	442	0.01	24	16.9	478	PASS
442	198	50	100	99.3	2824	PASS
443	442	15	24	20.5	578	PASS