

Data File : BG025940.D
Acq On : 24 Feb 2017 20:19
Operator : SJ/MA
Sample : I1957-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
FB20170222

Quant Time: Feb 24 22:41:34 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	87942	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	394623	20.00	ng	-0.01
38) Acenaphthene-d10	14.68	164	265676	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	747388	20.00	ng	0.00
75) Chrysene-d12	21.66	240	817814	20.00	ng	-0.02
86) Perylene-d12	24.87	264	795513	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	343151	67.93	ng	0.00
7) Phenol-d6	7.23	99	290508	38.87	ng	0.00
23) Nitrobenzene-d5	9.23	82	628117	100.45	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	548970	223.65	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1726678	113.56	ng	-0.01
78) Terphenyl-d14	20.01	244	2888478	85.90	ng	-0.01

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BG025940.D

Acq On : 24 Feb 2017 20:19

Operator : SJ/MA

Sample : I1957-13

Misc :

ALS Vial : 8 Sample Multiplier: 1

Instrument :

BNA_G

ClientSampleId :

FB20170222


Quant Time: Feb 24 22:41:34 2017


Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Fri Feb 17 15:48:21 2017

Response via : Initial Calibration

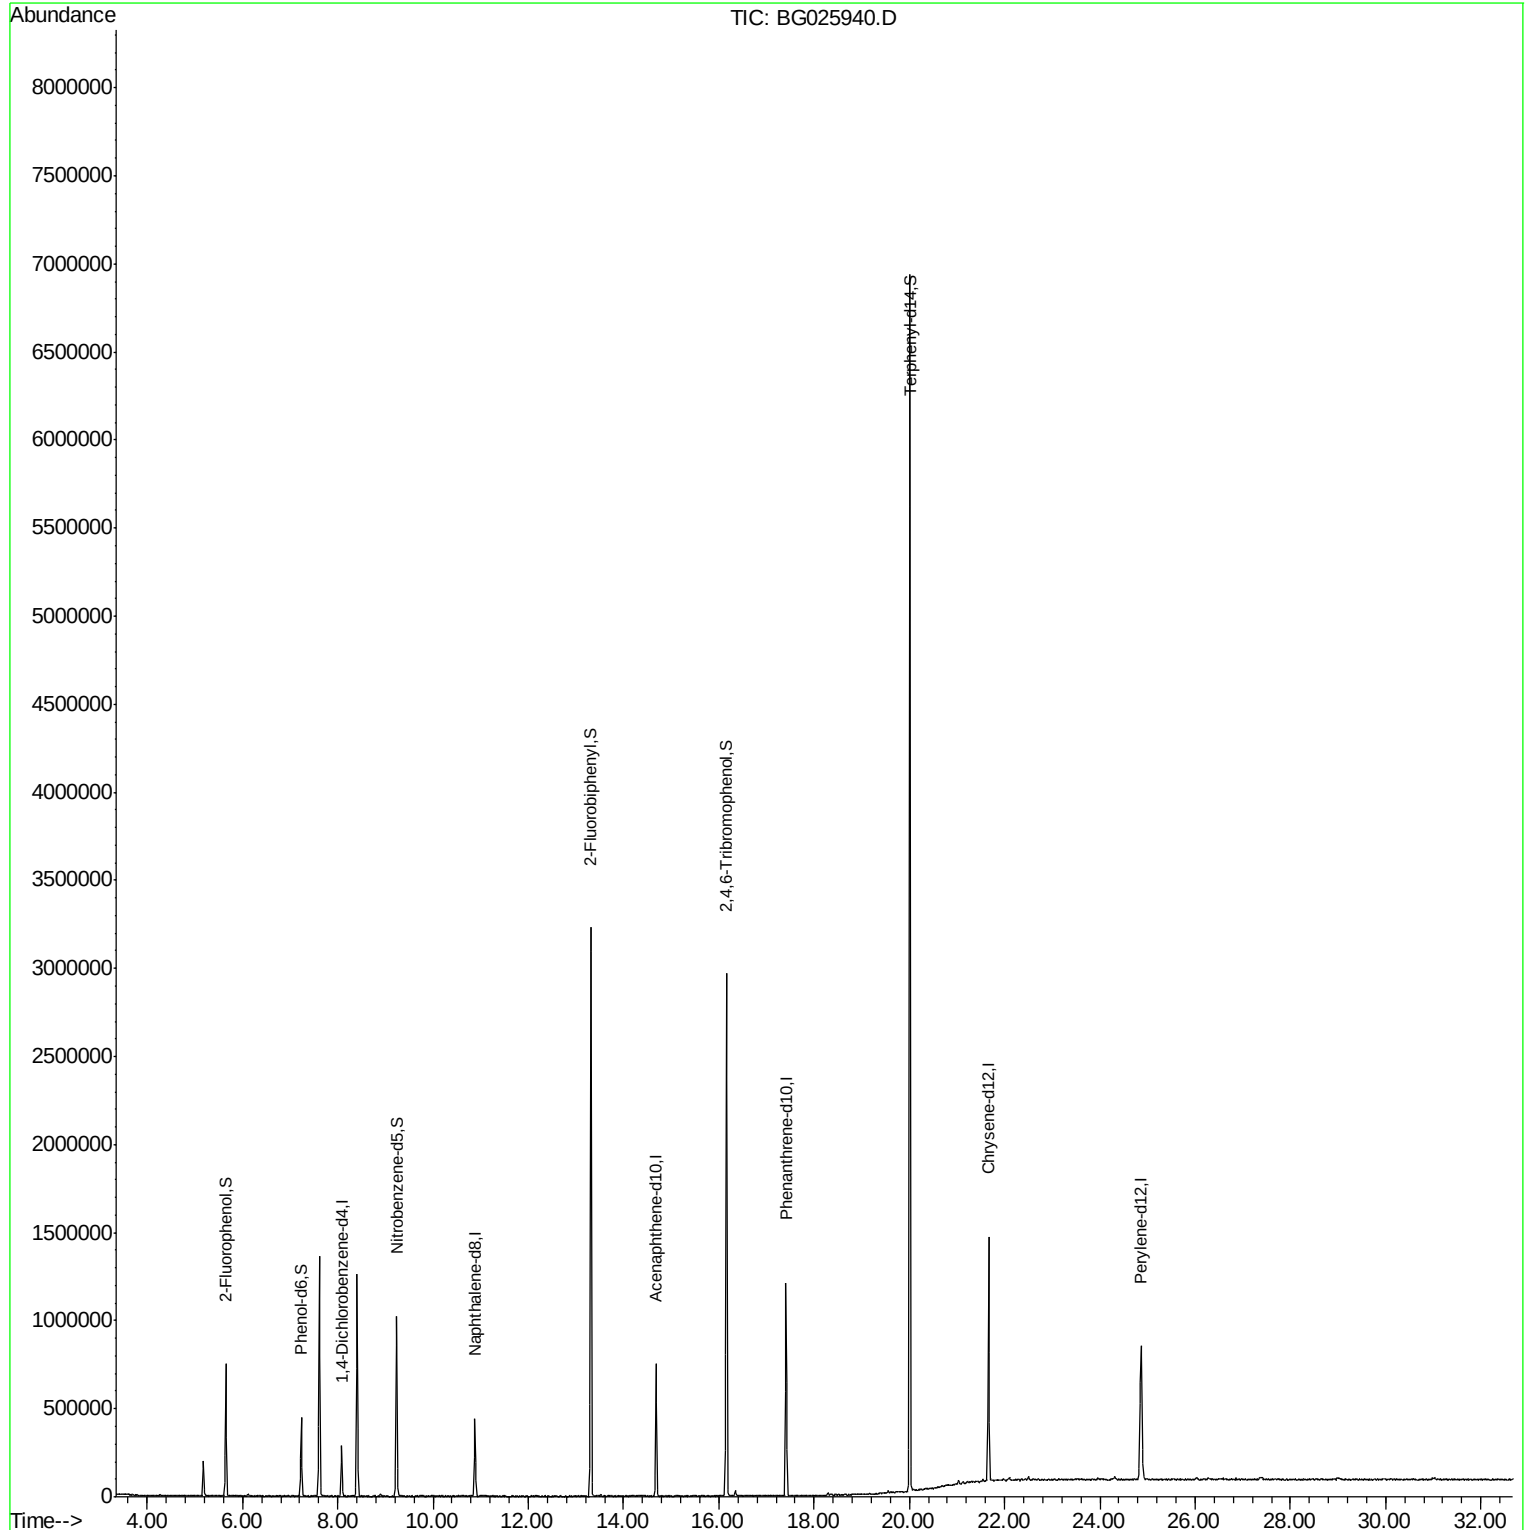

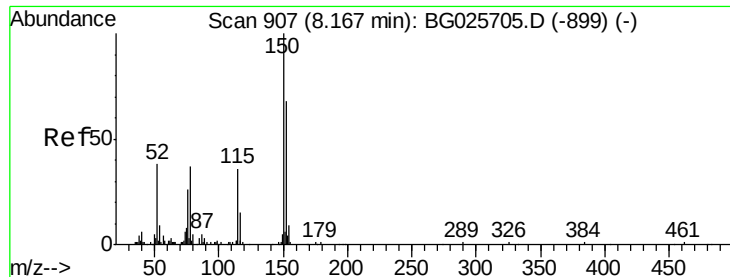

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 8.08 min Scan# 807

Delta R.T. -0.01 min

Lab File: BG025940.D

Acq: 24 Feb 2017 20:19

Instrument :

BNA_G

ClientSampleId :

FB20170222


Tgt Ion:152 Resp: 87942

Ion Ratio Lower Upper

152 100

150 155.3 114.0 171.0




115 54.8 48.1 72.1

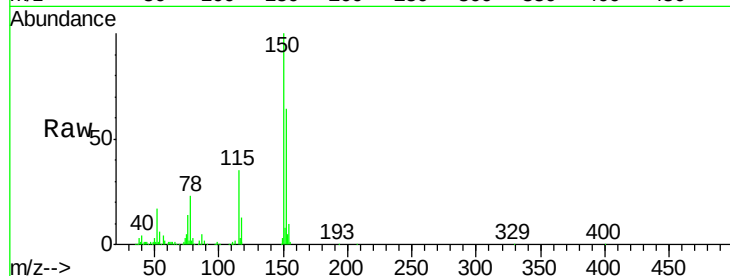

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

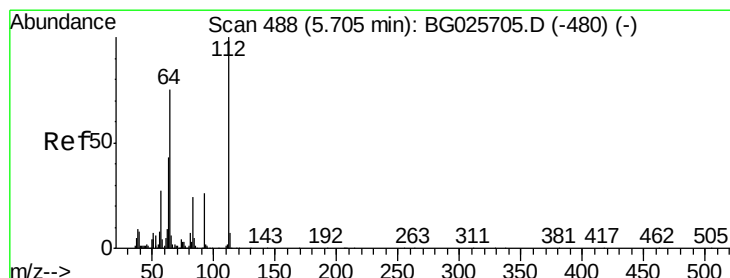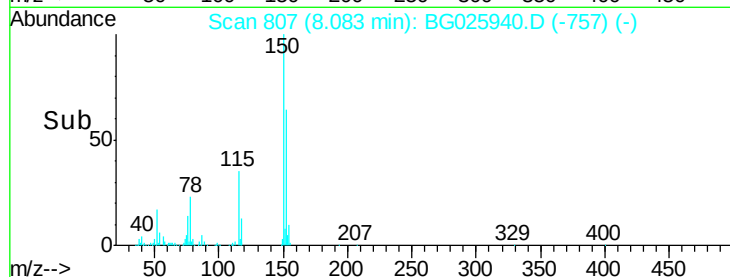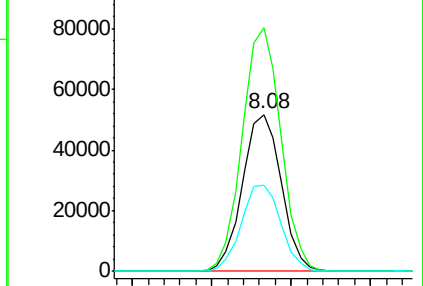

#5

2-Fluorophenol

Concen: 67.93 ng

RT: 5.65 min Scan# 393

Delta R.T. -0.00 min

Lab File: BG025940.D

Acq: 24 Feb 2017 20:19


Tgt Ion:112 Resp: 343151

Ion Ratio Lower Upper

112 100

64 67.8 61.8 92.6



63 33.5 37.2 55.8#

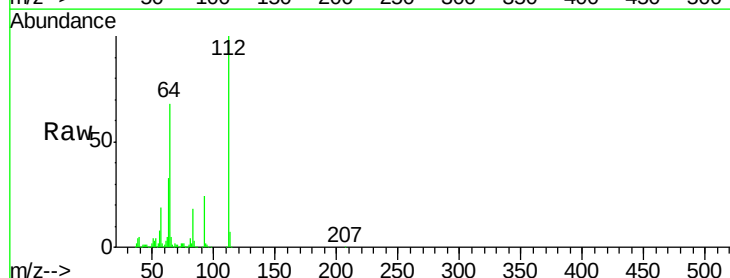


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG0

Ion 63.00 (62.70 to 63.70): BG0

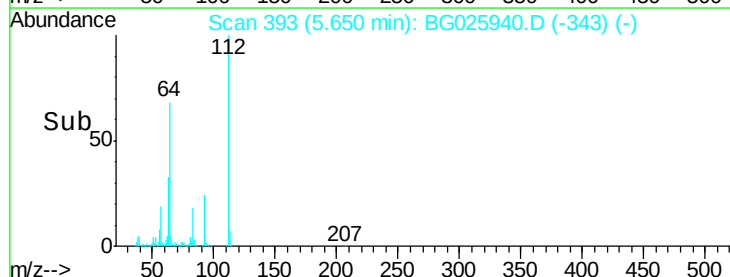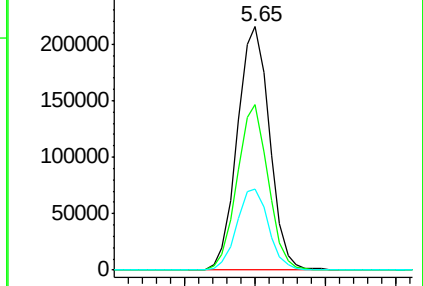

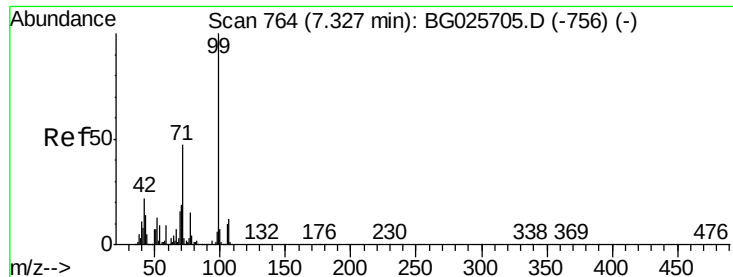

#7

Phenol-d6

Concen: 38.87 ng

RT: 7.23 min Scan# 662

Delta R.T. -0.01 min

Lab File: BG025940.D

Acq: 24 Feb 2017 20:19

Instrument :

BNA_G

ClientSampleId :

FB20170222


Tgt Ion: 99 Resp: 290508

Ion Ratio Lower Upper




99 100

42 14.0 20.5 30.7#

71 26.7 37.6 56.4#

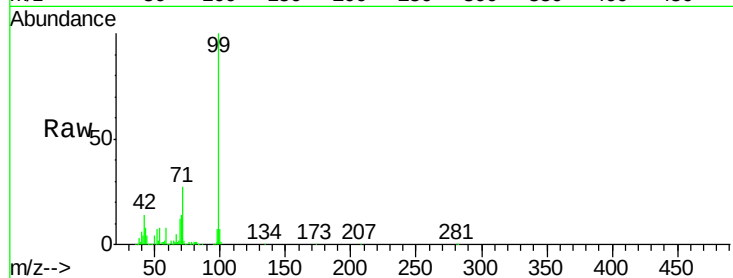

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

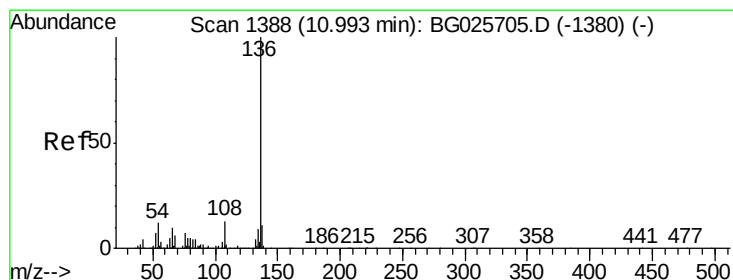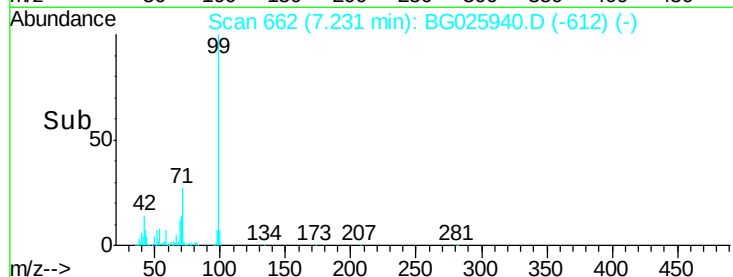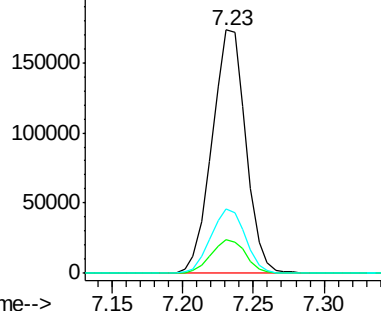

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 10.88 min Scan# 1283

Delta R.T. -0.01 min

Lab File: BG025940.D

Acq: 24 Feb 2017 20:19

Tgt Ion: 136 Resp: 394623


Ion Ratio Lower Upper

136 100



137 11.5 8.9 13.3


54 8.7 9.3 13.9#

68 7.2 5.1 7.7

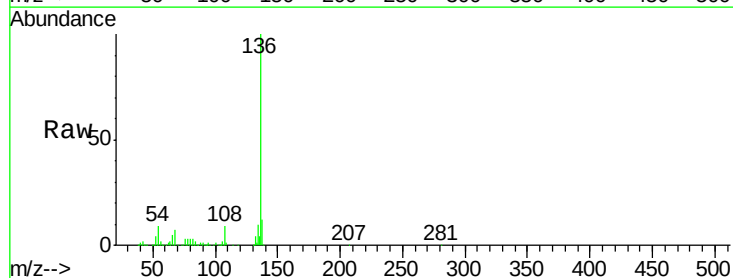

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



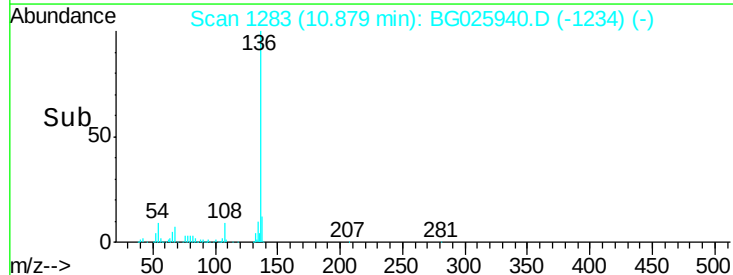
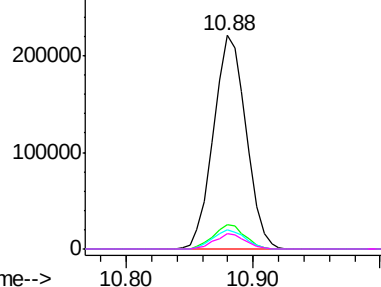


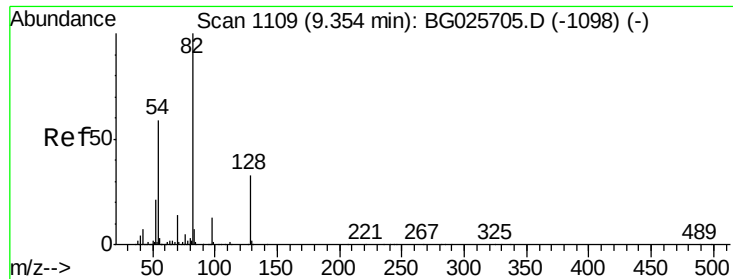

#23
 Nitrobenzene-d5
 Concen: 100.45 ng
 RT: 9.23 min Scan# 1003
 Delta R.T. -0.01 min
 Lab File: BG025940.D
 Acq: 24 Feb 2017 20:19




Instrument :
 BNA_G
 ClientSampleId :
 FB20170222


Tgt Ion	Ratio	Lower	Upper
82	100		
128	47.1	26.4	39.6
54	51.1	49.4	74.2

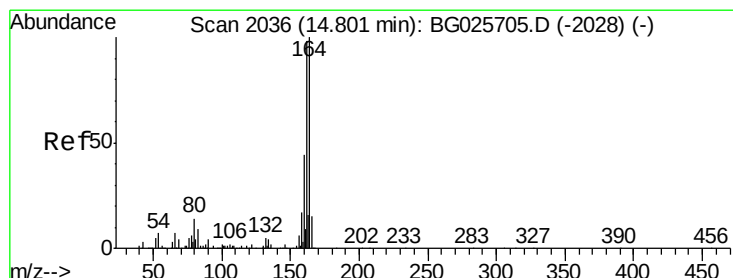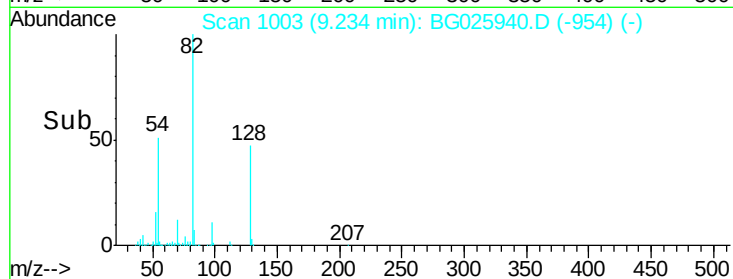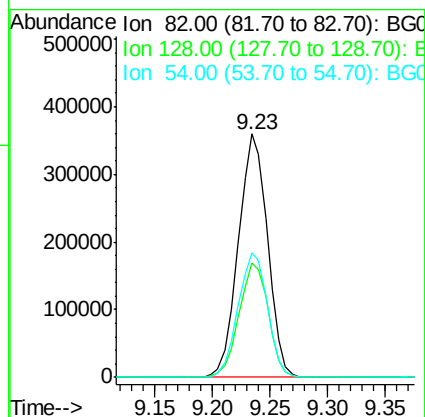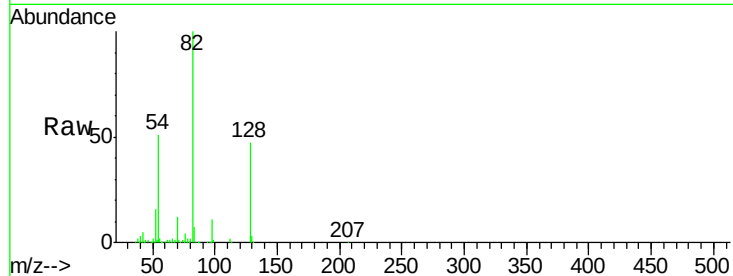

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 14.68 min Scan# 1930
 Delta R.T. -0.01 min
 Lab File: BG025940.D
 Acq: 24 Feb 2017 20:19

Tgt Ion	Ratio	Lower	Upper
164	100		
162	105.0	85.1	127.7
160	45.3	34.7	52.1


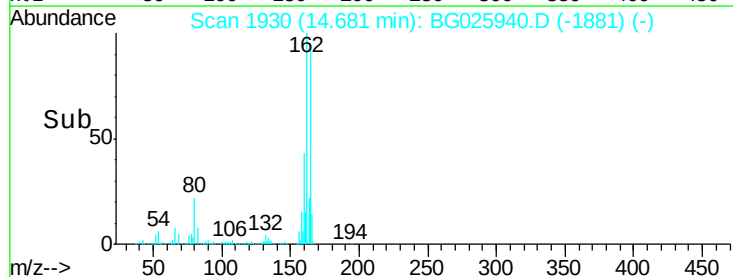
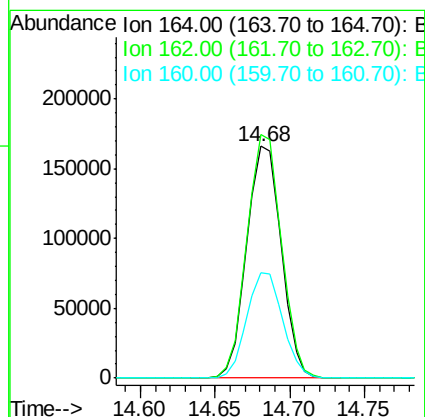
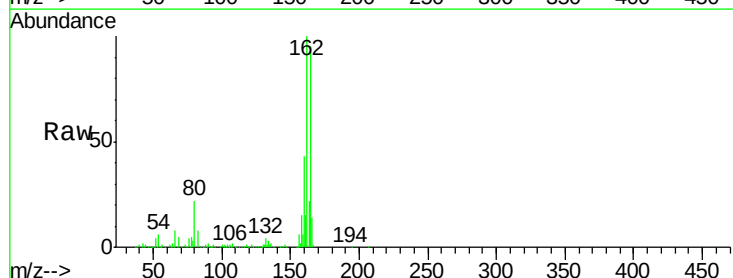


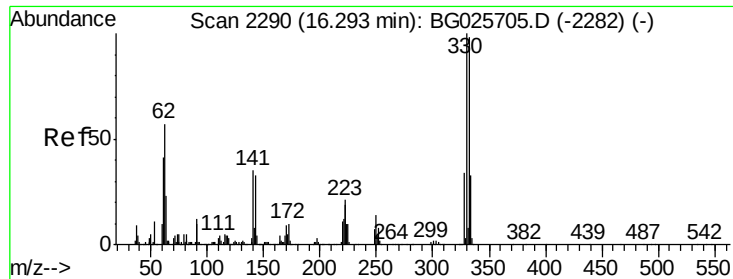

#41
 2,4,6-Tribromophenol
 Concen: 223.65 ng
 RT: 16.16 min Scan# 2182
 Delta R.T. -0.01 min
 Lab File: BG025940.D
 Acq: 24 Feb 2017 20:19




Instrument :
 BNA_G
 ClientSampleId :
 FB20170222


Tgt Ion:330 Resp: 548970
 Ion Ratio Lower Upper
 330 100
 332 97.3 77.3 115.9
 141 37.4 32.1 48.1

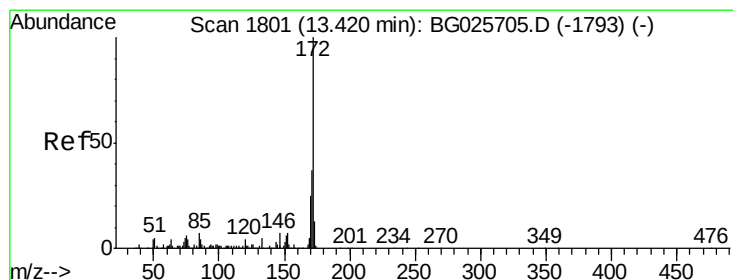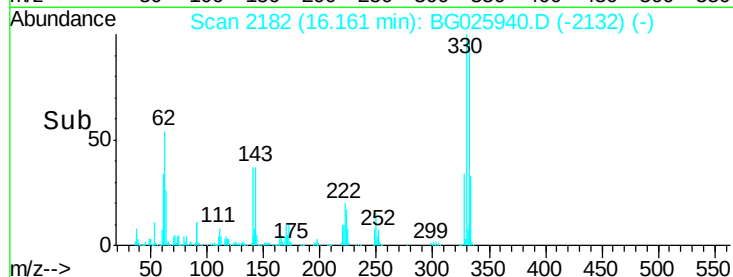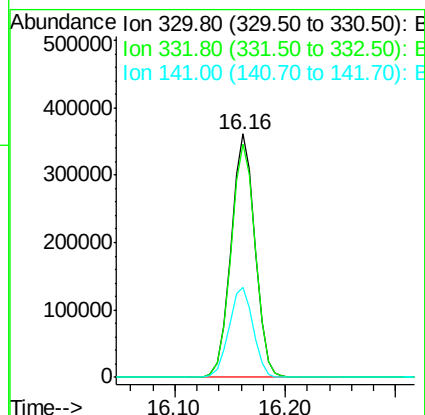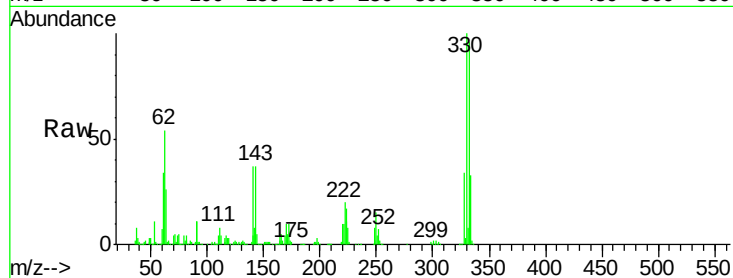

#44
 2-Fluorobiphenyl
 Concen: 113.56 ng
 RT: 13.31 min Scan# 1697
 Delta R.T. -0.01 min
 Lab File: BG025940.D
 Acq: 24 Feb 2017 20:19

Tgt Ion:172 Resp: 1726678
 Ion Ratio Lower Upper
 172 100
 171 38.5 32.2 48.2
 170 25.7 21.8 32.6


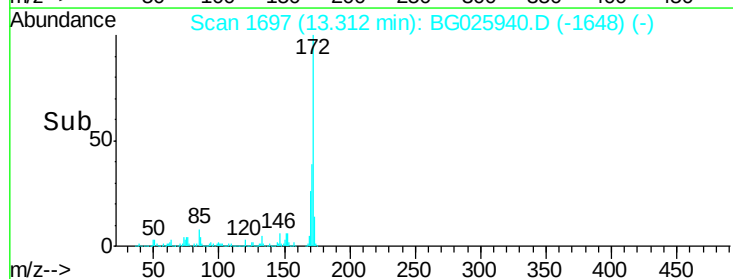
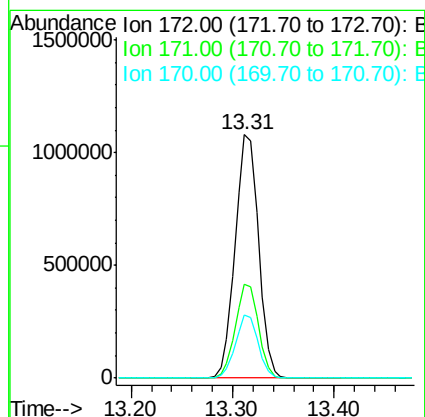
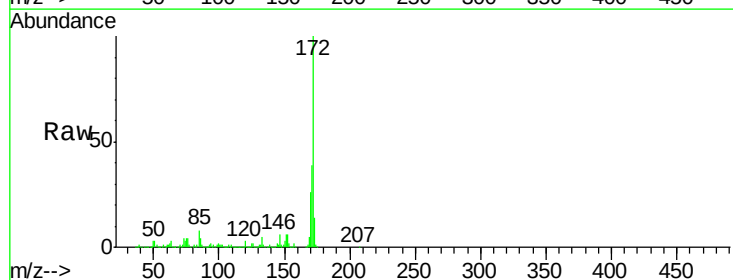


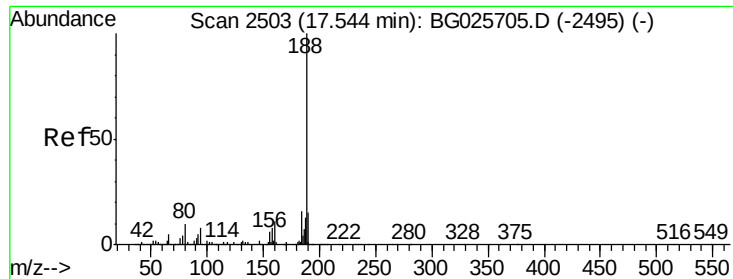

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 17.41 min Scan# 2395
Delta R.T. -0.01 min
Lab File: BG025940.D
Acq: 24 Feb 2017 20:19




Instrument :
BNA_G
ClientSampleId :
FB20170222


Tgt Ion:188 Resp: 747388
Ion Ratio Lower Upper
188 100
94 9.5 5.8 8.8#
80 10.8 7.5 11.3

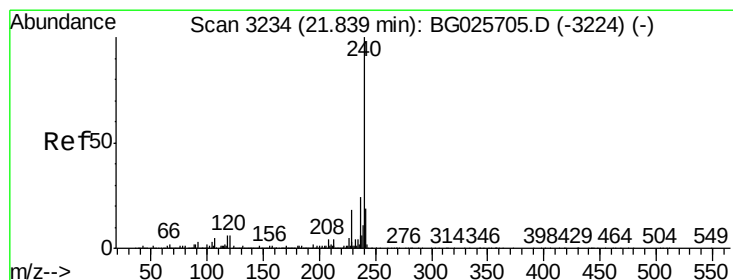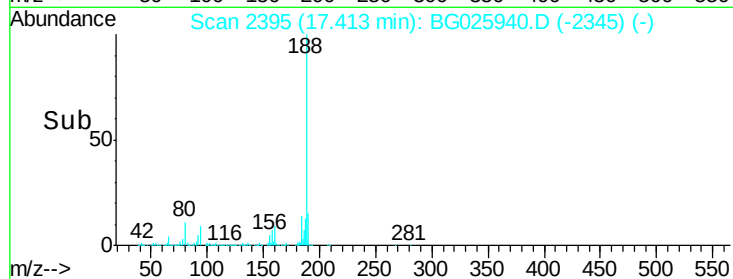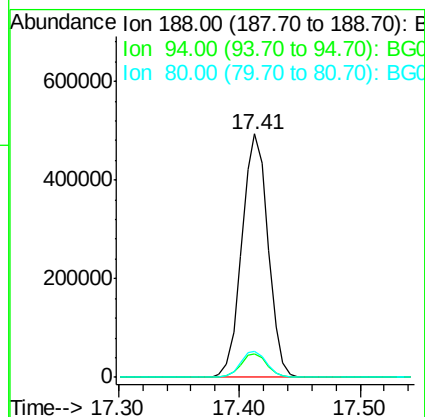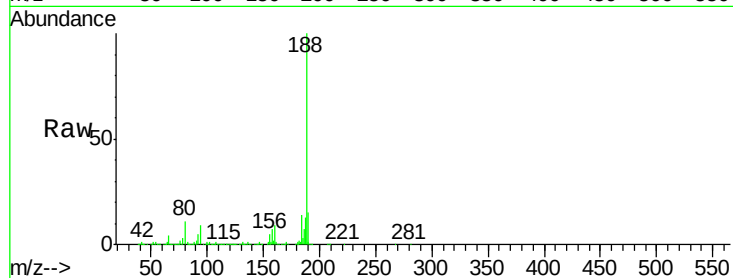

#75
Chrysene-d12
Concen: 20.00 ng
RT: 21.66 min Scan# 3118
Delta R.T. -0.02 min
Lab File: BG025940.D
Acq: 24 Feb 2017 20:19

Tgt Ion:240 Resp: 817814
Ion Ratio Lower Upper
240 100
120 11.2 5.7 8.5#
236 26.2 22.2 33.4

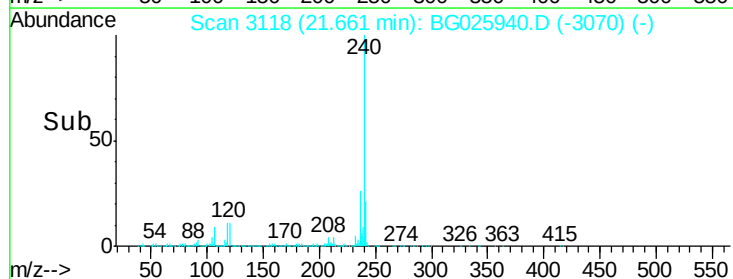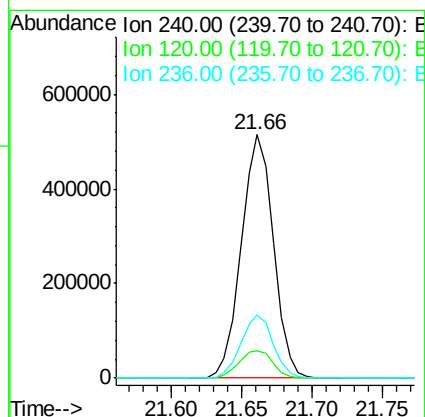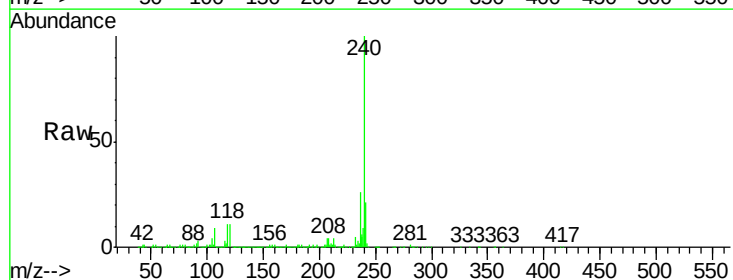

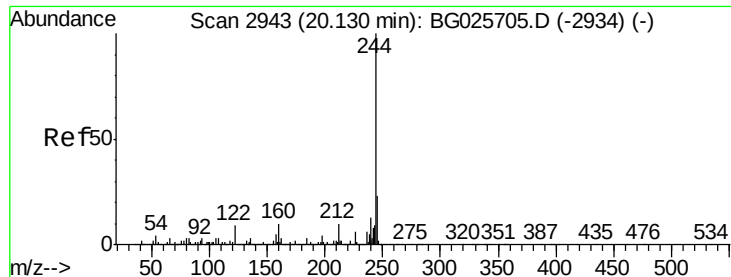

#78

Terphenyl-d14

Concen: 85.90 ng

RT: 20.01 min Scan# 2837

Delta R.T. -0.01 min

Lab File: BG025940.D

Acq: 24 Feb 2017 20:19

Instrument :

BNA_G

ClientSampleId :

FB20170222


Tgt Ion:244 Resp: 2888478

Ion Ratio Lower Upper

244 100

212 9.0 10.0 15.0#




122 14.4 8.6 12.8#

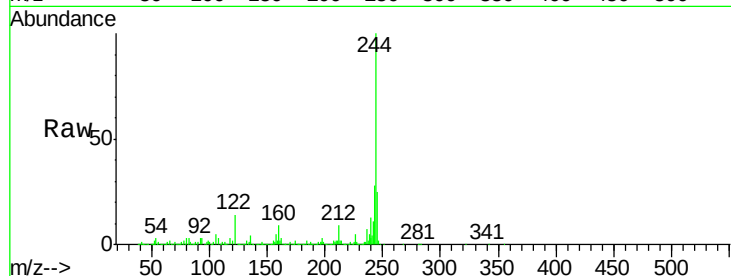

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

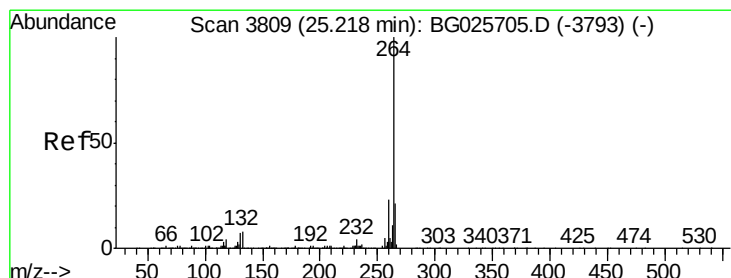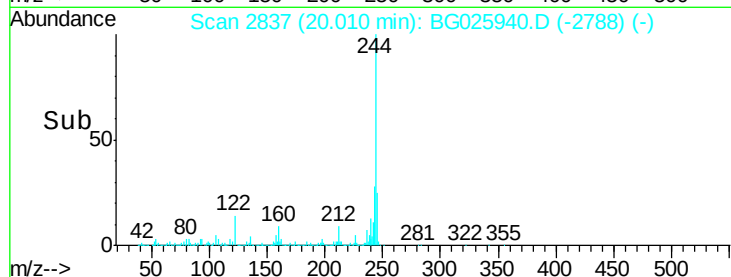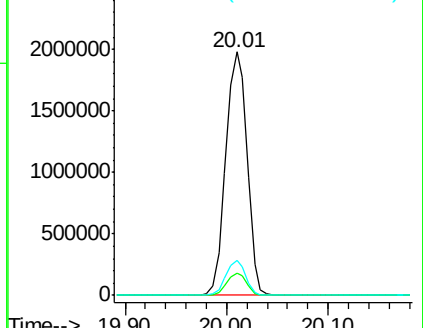

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.87 min Scan# 3664

Delta R.T. -0.02 min

Lab File: BG025940.D

Acq: 24 Feb 2017 20:19


Tgt Ion:264 Resp: 795513

Ion Ratio Lower Upper

264 100

260 23.2 21.8 32.8

265 21.4 18.2 27.4

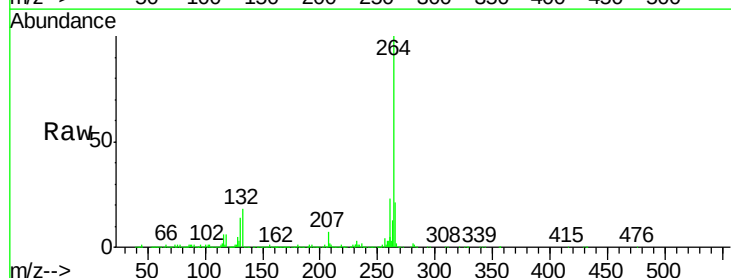

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

