
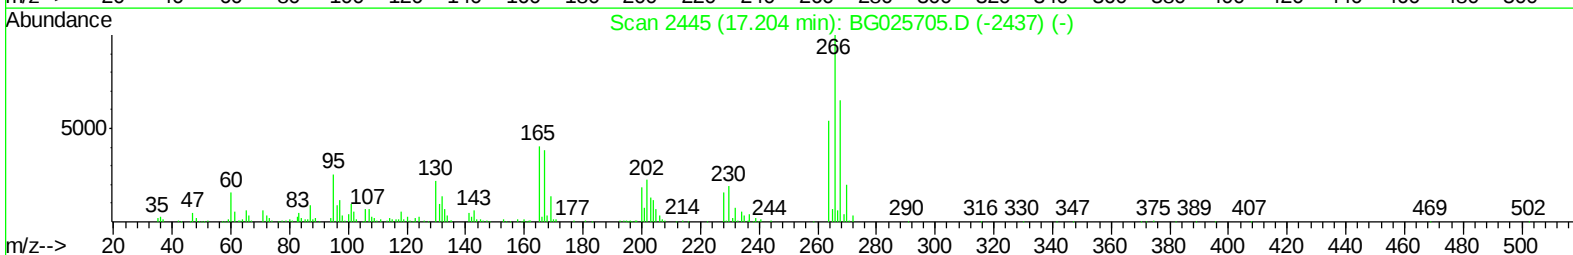
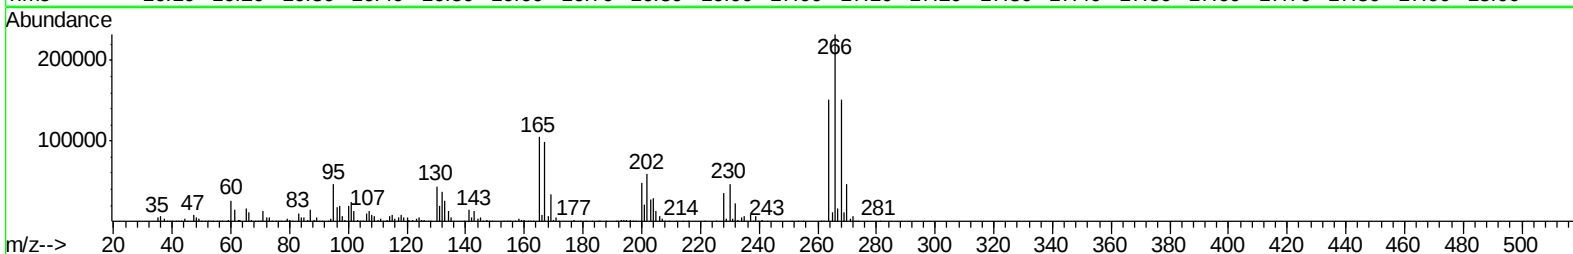


Data File : BG025933.D
Acq On : 24 Feb 2017 15:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 02:56:52 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

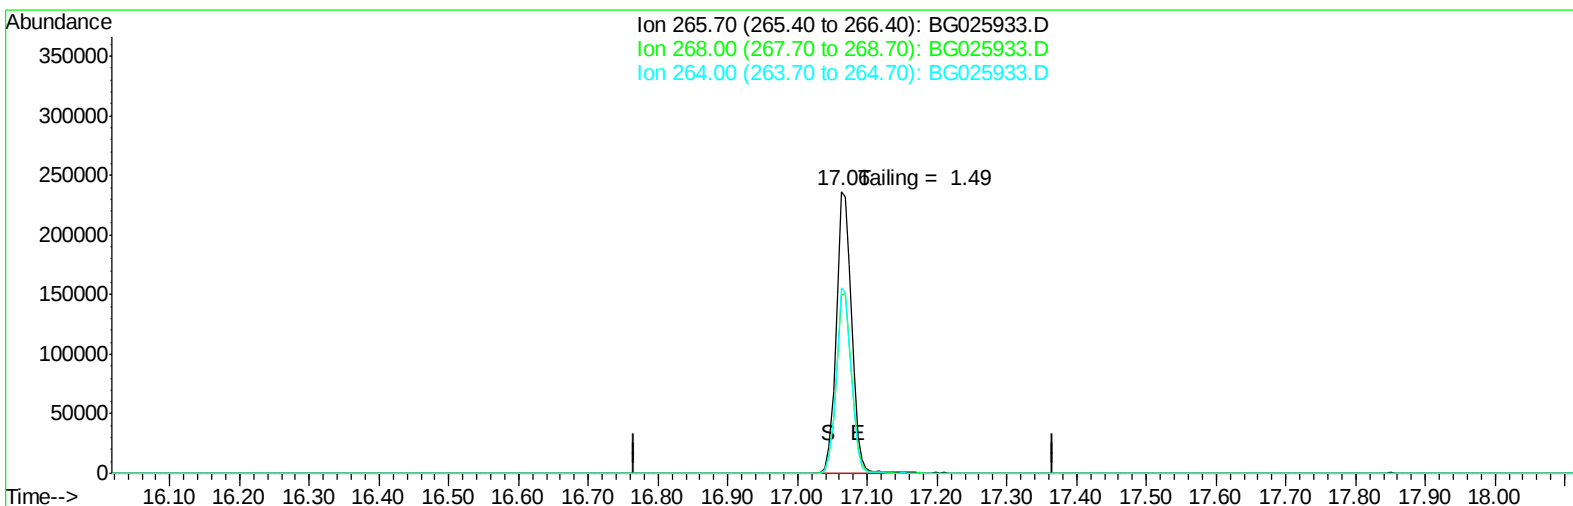

TIC: BG025933.D

(69) Pentachlorophenol (C)




17.066min (-17.066) 0.00ng

response 0

Ion	Exp%	Act%
265.70	100	0.00
268.00	60.70	0.00#
264.00	62.60	0.00#
0.00	0.00	0.00

Data File : BG025933.D
Acq On : 24 Feb 2017 15:35
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 02:56:52 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

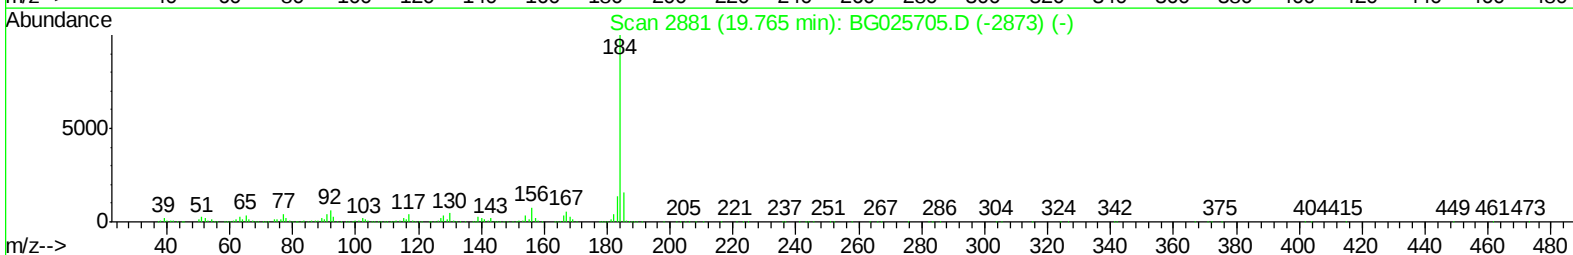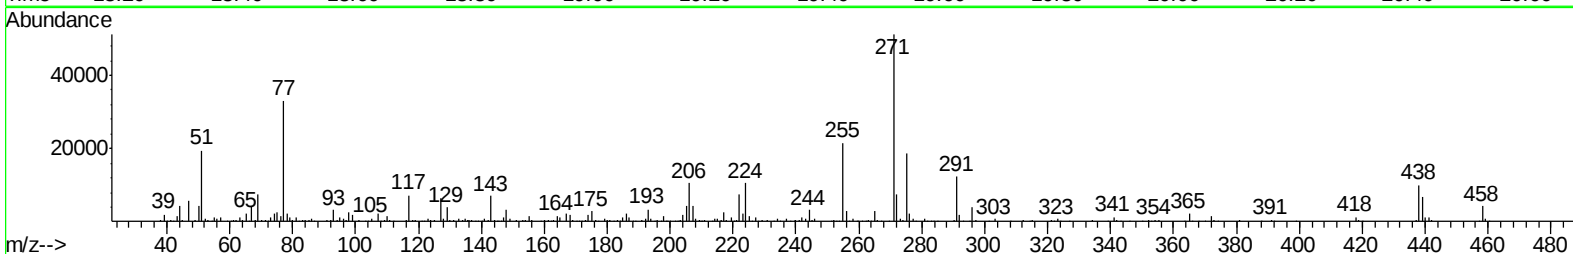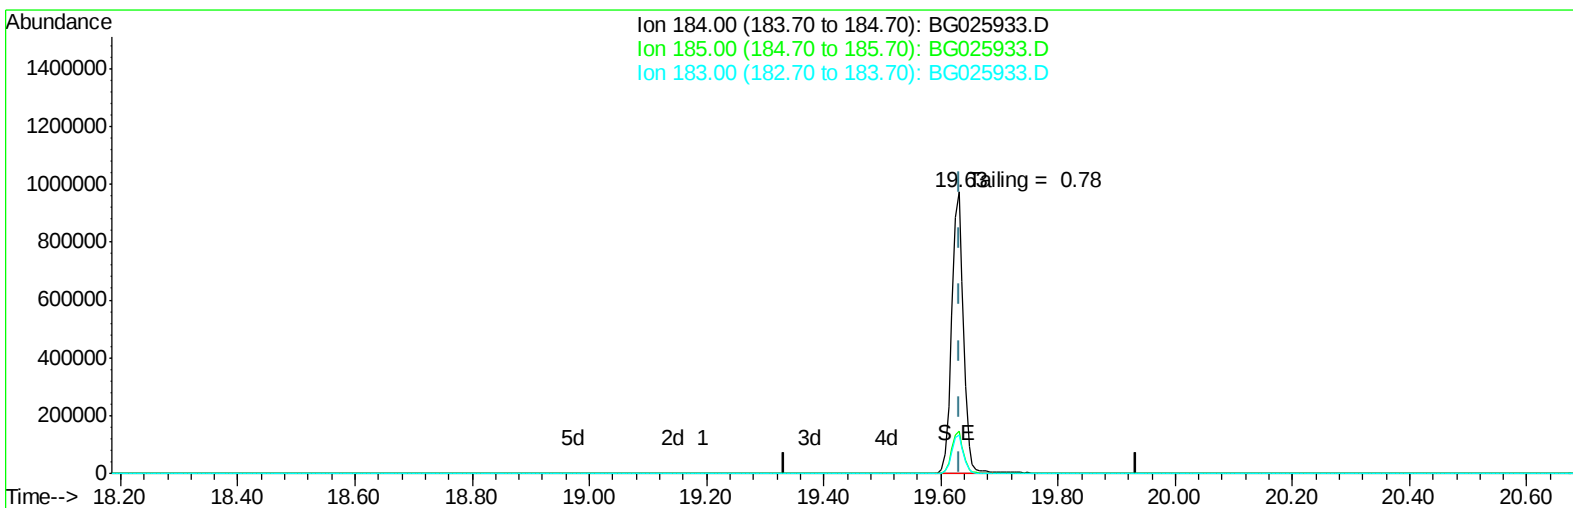

TIC: BG025933.D

(76) Benzidine

19.196min (-0.438) 18.90ng

response 210

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	389.52#
183.00	13.80	130.79#
0.00	0.00	0.00