

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022417\
 Data File : BG025946.D
 Acq On : 25 Feb 2017 00:20
 Operator : SJ/MA
 Sample : I1973-07
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E2-Y6N-SW

Quant Time: Feb 25 01:33:06 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 15:48:21 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.08	152	81431	20.00	ng	0.00
21) Naphthalene-d8	10.88	136	388200	20.00	ng	-0.01
38) Acenaphthene-d10	14.68	164	261222	20.00	ng	-0.01
63) Phenanthrene-d10	17.41	188	714161	20.00	ng	0.00
75) Chrysene-d12	21.66	240	767594	20.00	ng	-0.02
86) Perylene-d12	24.86	264	745867	20.00	ng	-0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	820261	175.37	ng	0.00
7) Phenol-d6	7.24	99	1164500	168.25	ng	0.00
23) Nitrobenzene-d5	9.23	82	625195	101.63	ng	-0.01
41) 2,4,6-Tribromophenol	16.16	330	567787	235.26	ng	0.00
44) 2-Fluorobiphenyl	13.31	172	1588836	106.28	ng	-0.01
78) Terphenyl-d14	20.01	244	2436066	77.19	ng	-0.01
Target Compounds						
10) Phenol	7.26	94	50613	6.73	ng	79
49) Dimethylphthalate	14.13	163	97540	5.44	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022417\
Data File : BG025946.D
Acq On : 25 Feb 2017 00:20
Operator : SJ/MA
Sample : I1973-07
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E2-Y6N-SW

Quant Time: Feb 25 01:33:06 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 15:48:21 2017
Response via : Initial Calibration

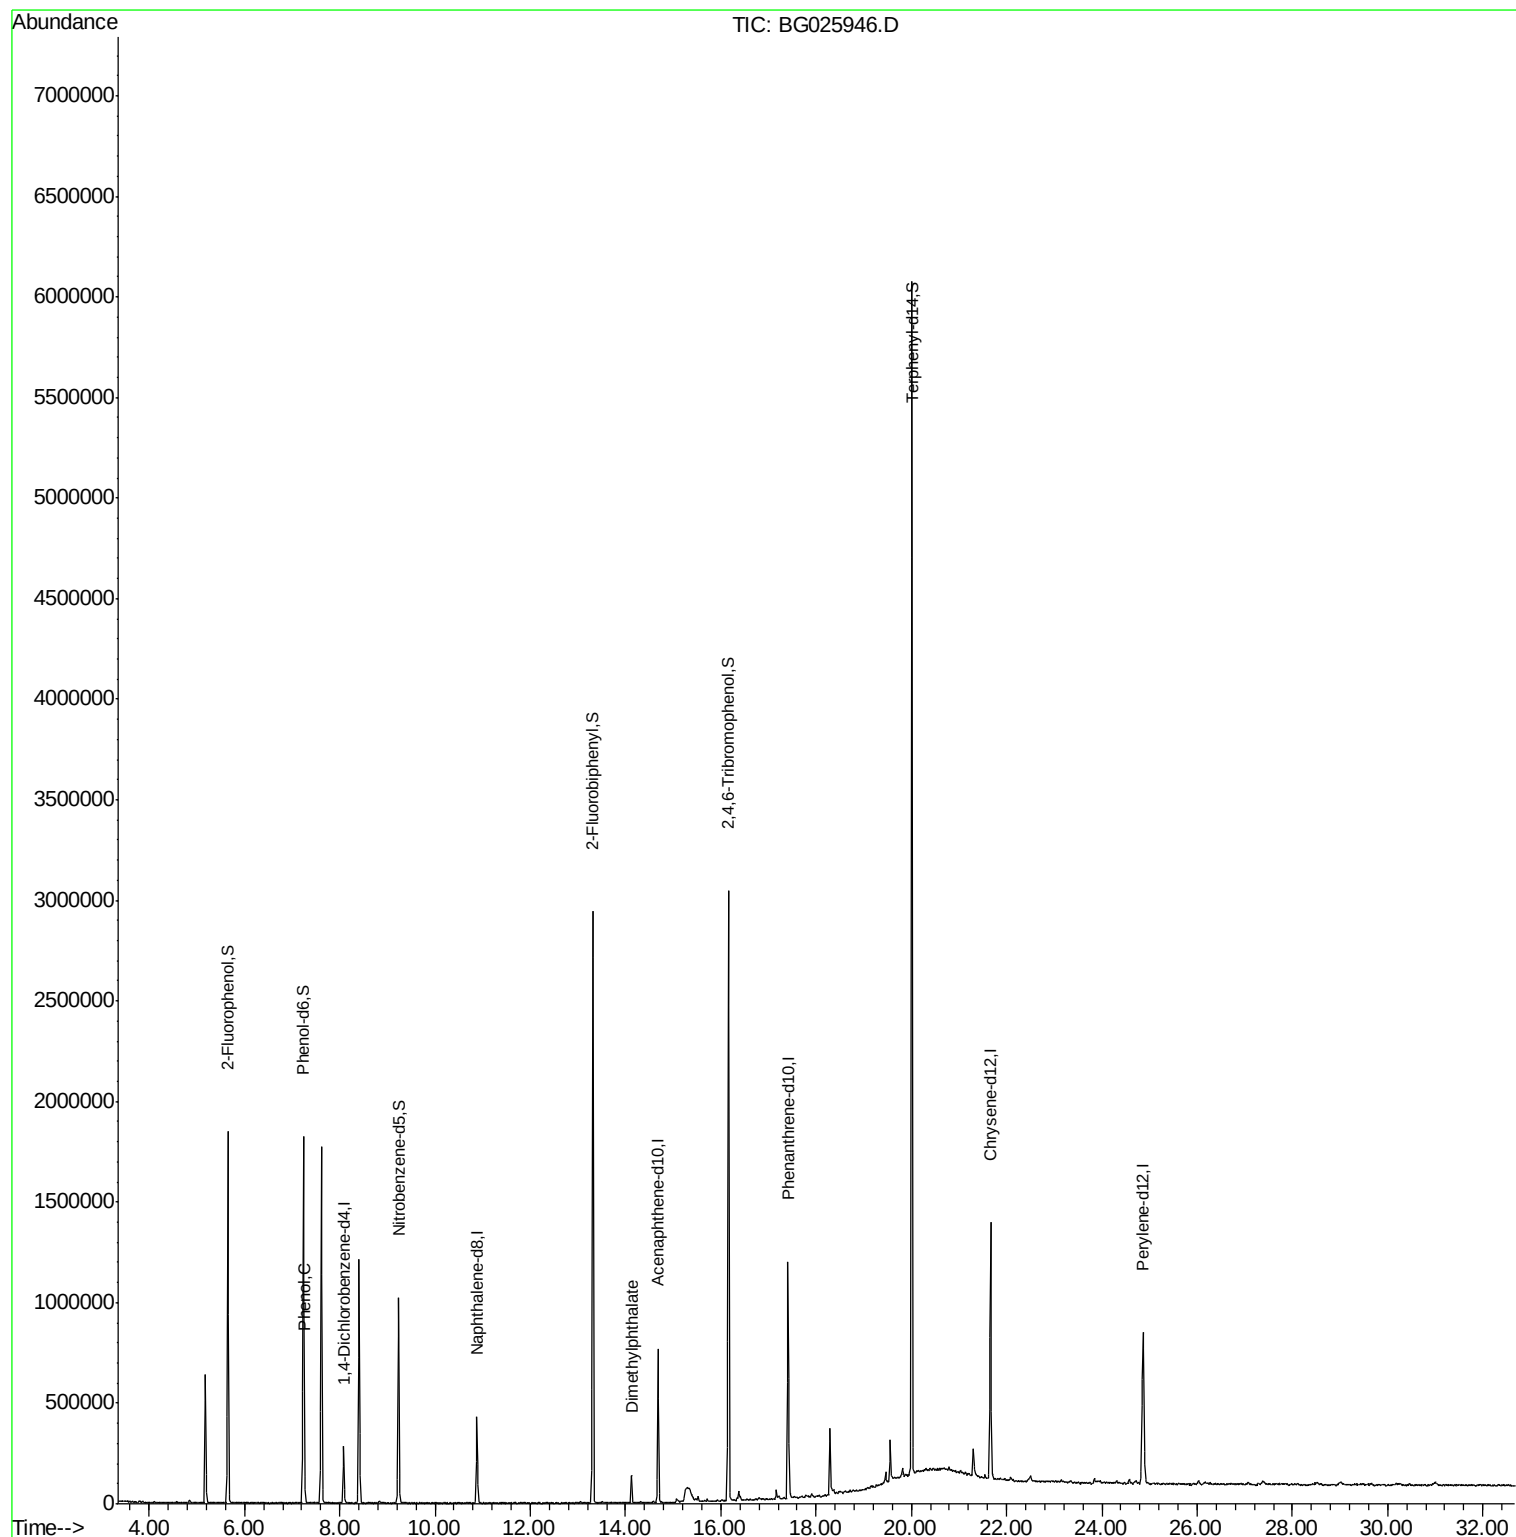

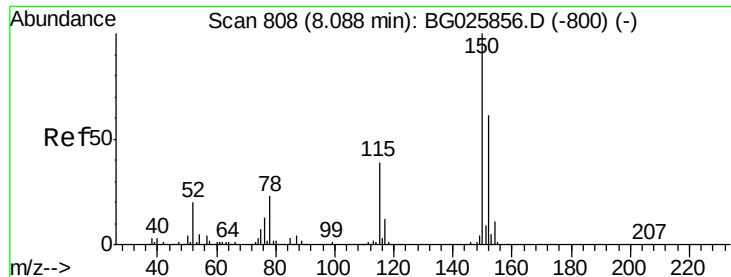


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 8.08 min Scan# 807
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20

Instrument :
BNA_G
ClientSampleId :
E2-Y6N-SW

Tgt Ion:152 Resp: 81431
Ion Ratio Lower Upper
152 100
150 161.4 114.0 171.0
115 56.5 48.1 72.1

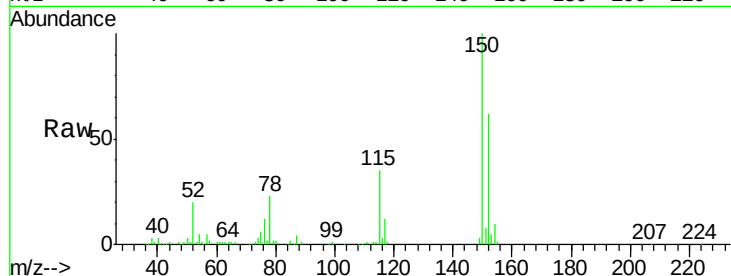


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

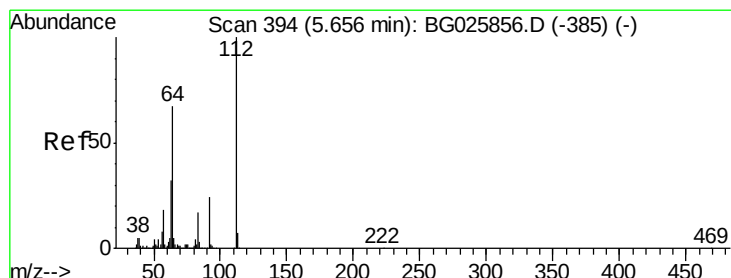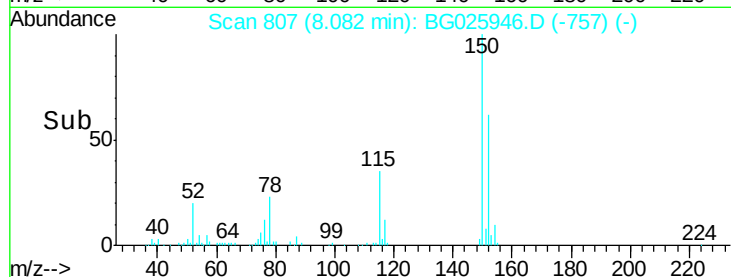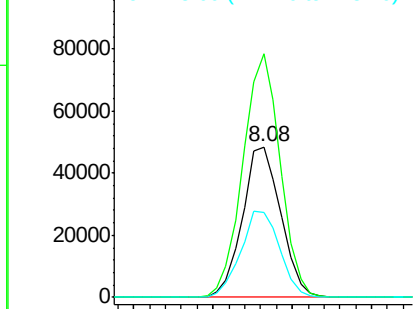



#5




2-Fluorophenol
Concen: 175.37 ng
RT: 5.65 min Scan# 393
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20

Tgt Ion:112 Resp: 820261
Ion Ratio Lower Upper
112 100
64 66.1 61.8 92.6
63 33.3 37.2 55.8#

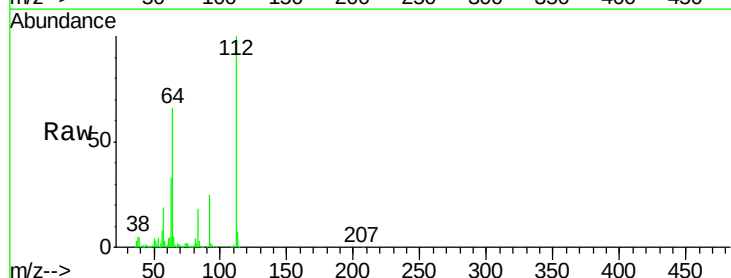

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BG0
Ion 63.00 (62.70 to 63.70): BG0

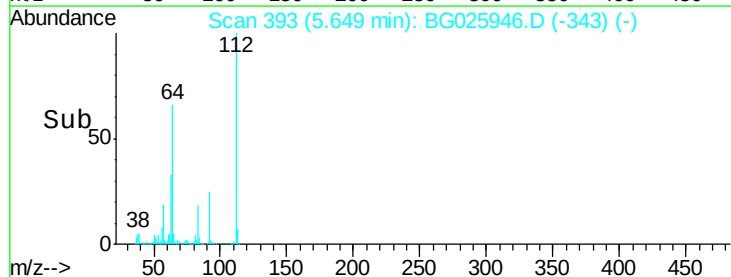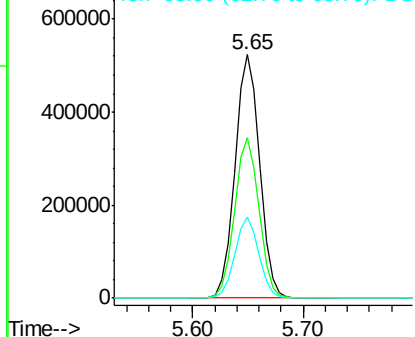

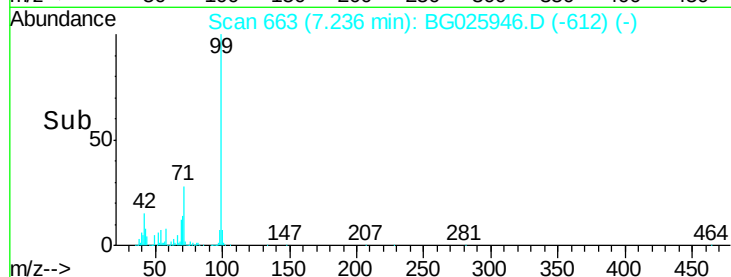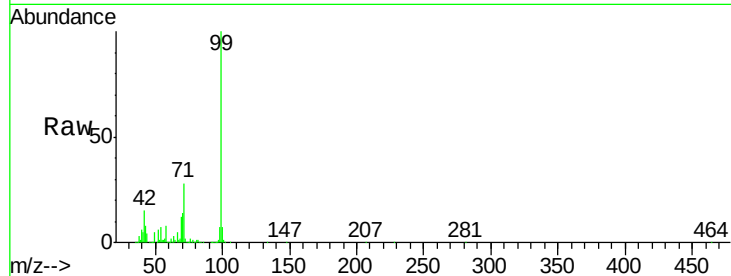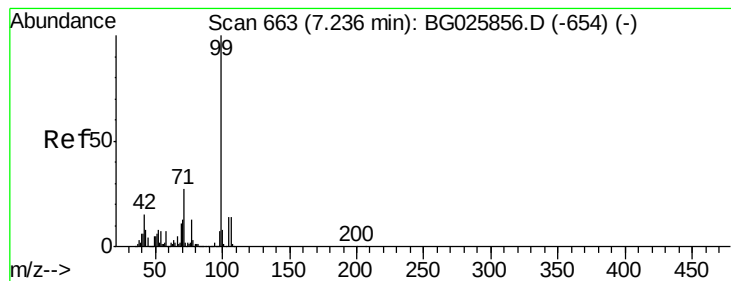

#7

Phenol-d6

Concen: 168.25 ng

RT: 7.24 min Scan# 663

Delta R.T. -0.00 min

Lab File: BG025946.D

Acq: 25 Feb 2017 00:20

Instrument :

BNA_G

ClientSampleId :

E2-Y6N-SW





Tgt Ion: 99 Resp: 1164500

Ion Ratio Lower Upper

99 100

42 14.6 20.5 30.7#

71 28.4 37.6 56.4#

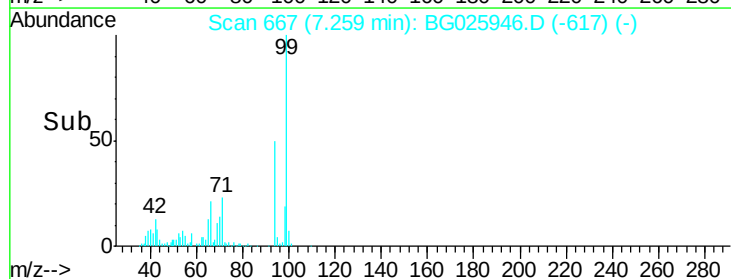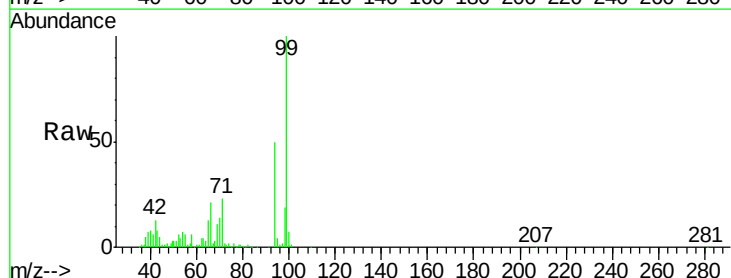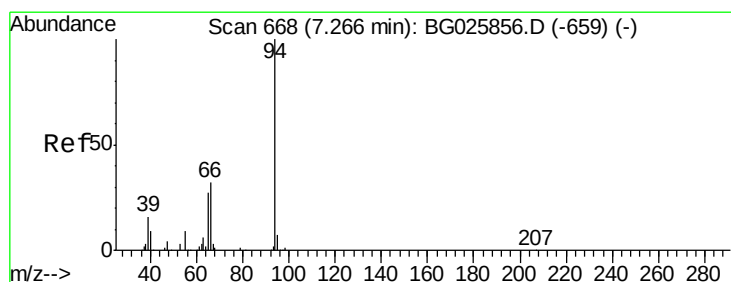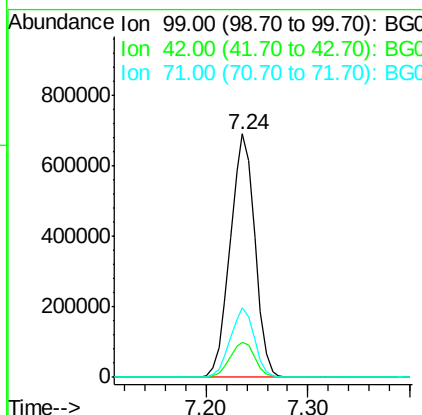

#10

Phenol

Concen: 6.73 ng

RT: 7.26 min Scan# 667

Delta R.T. -0.01 min

Lab File: BG025946.D

Acq: 25 Feb 2017 00:20


Tgt Ion: 94 Resp: 50613


Ion Ratio Lower Upper

94 100

65 26.4 20.6 60.6

66 41.8 35.5 75.5

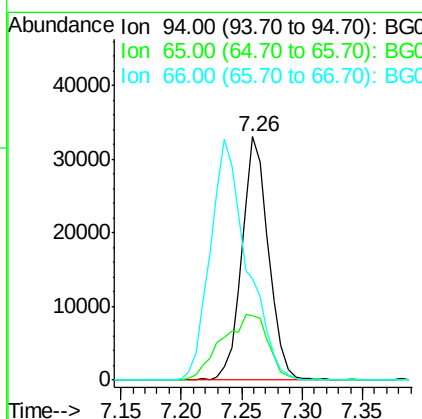


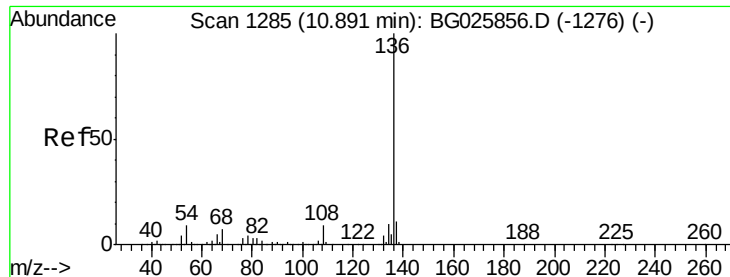




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 10.88 min Scan# 1283
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20

Instrument :
BNA_G
ClientSampleId :
E2-Y6N-SW

Tgt Ion:	136	Resp:	388200
Ion	Ratio	Lower	Upper
136	100		
137	11.2	8.9	13.3
54	9.3	9.3	13.9#
68	7.3	5.1	7.7

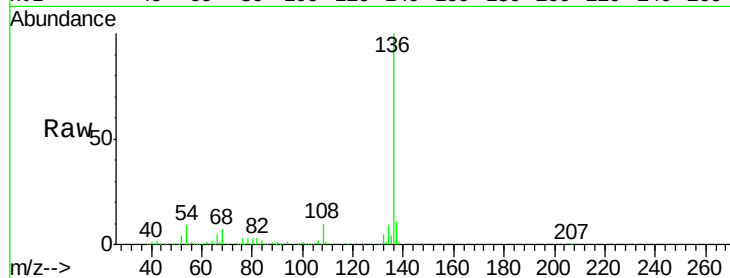


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BG
Ion 68.00 (67.70 to 68.70): BG

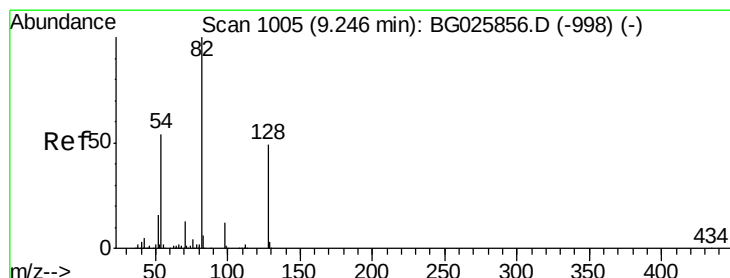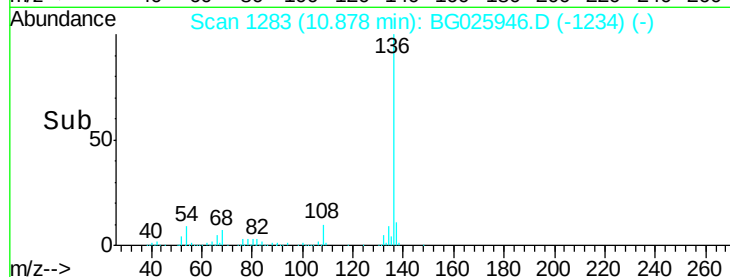
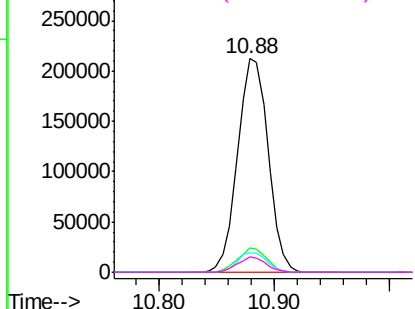



#23
Nitrobenzene-d5
Concen: 101.63 ng
RT: 9.23 min Scan# 1003
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20

Tgt Ion:	82	Resp:	625195
Ion	Ratio	Lower	Upper
82	100		
128	46.0	26.4	39.6#
54	50.2	49.4	74.2

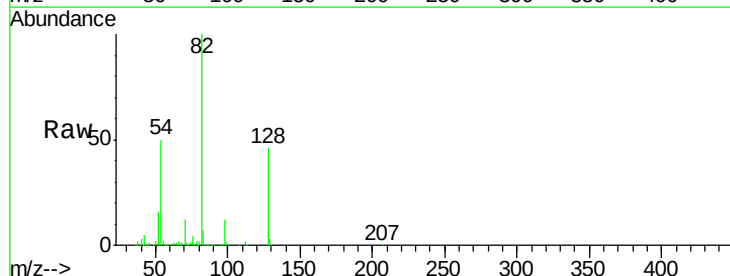

Abundance Ion 82.00 (81.70 to 82.70): BG
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BG



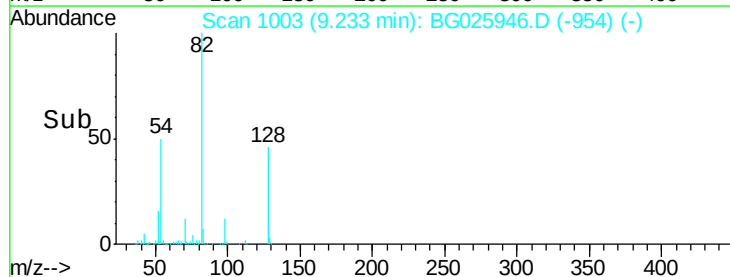
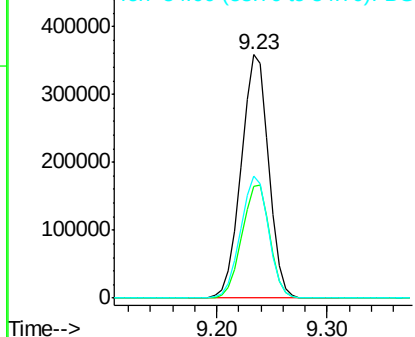


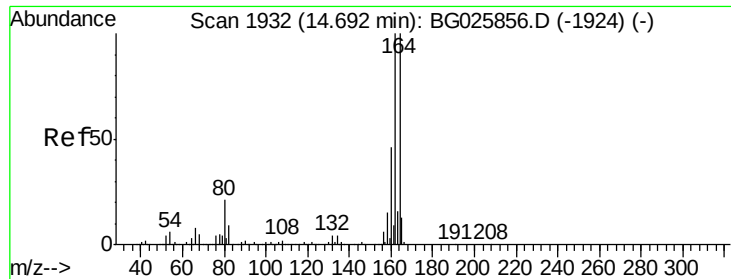

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 14.68 min Scan# 1930
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20




Instrument :
BNA_G
ClientSampleId :
E2-Y6N-SW


Tgt Ion:164 Resp: 261222
Ion Ratio Lower Upper
164 100
162 103.9 85.1 127.7
160 46.7 34.7 52.1

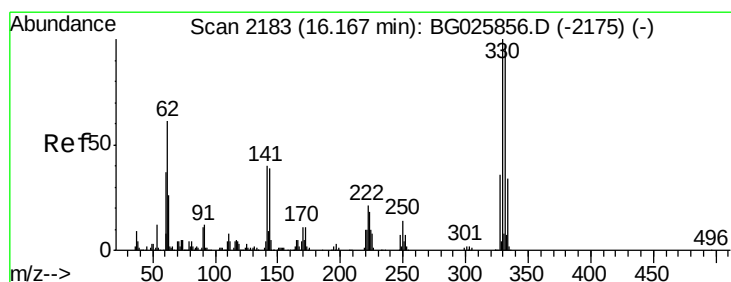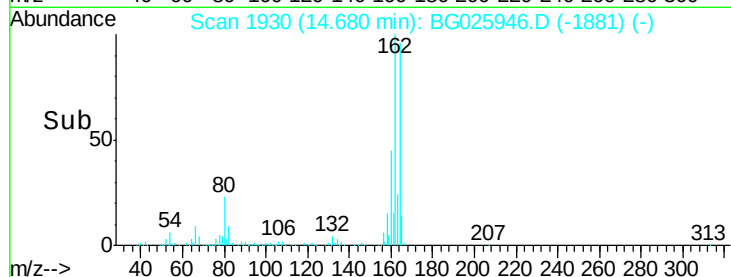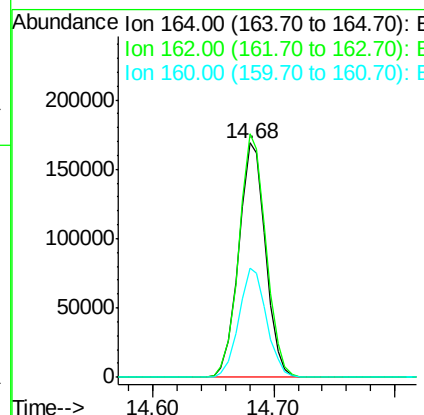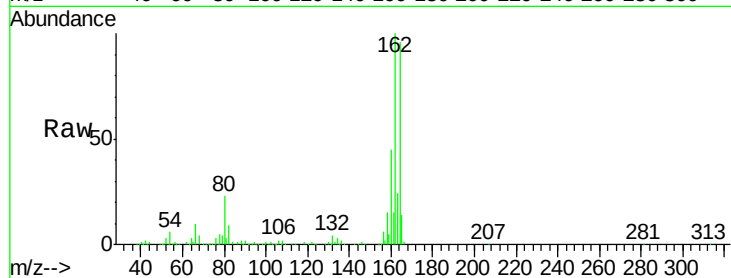

#41
2,4,6-Tribromophenol
Concen: 235.26 ng
RT: 16.16 min Scan# 2182
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20

Tgt Ion:330 Resp: 567787
Ion Ratio Lower Upper
330 100
332 96.3 77.3 115.9
141 37.1 32.1 48.1


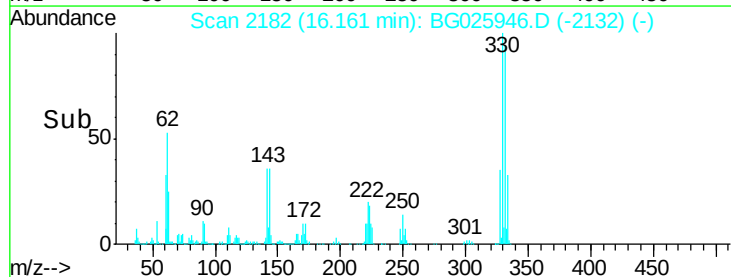
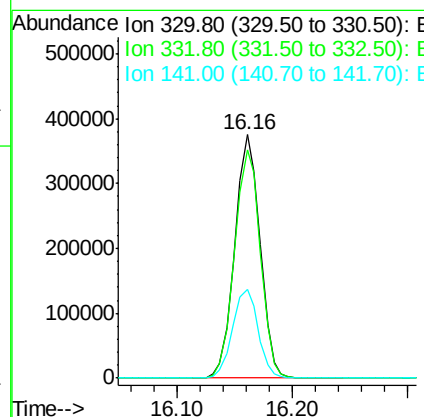
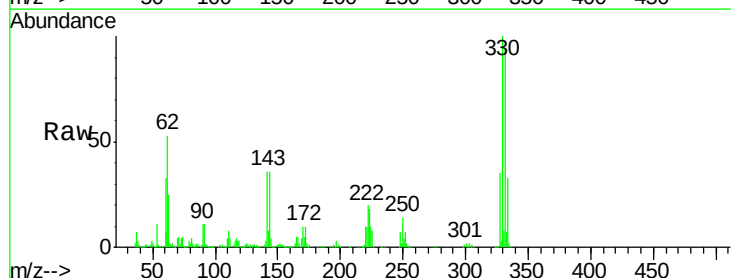


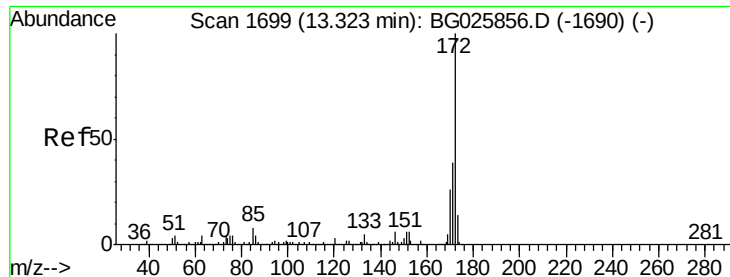

#44
2-Fluorobiphenyl
Concen: 106.28 ng
RT: 13.31 min Scan# 1697
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20




Instrument :
BNA_G
ClientSampleId :
E2-Y6N-SW


Tgt Ion:172 Resp: 1588836
Ion Ratio Lower Upper
172 100
171 38.0 32.2 48.2
170 25.4 21.8 32.6

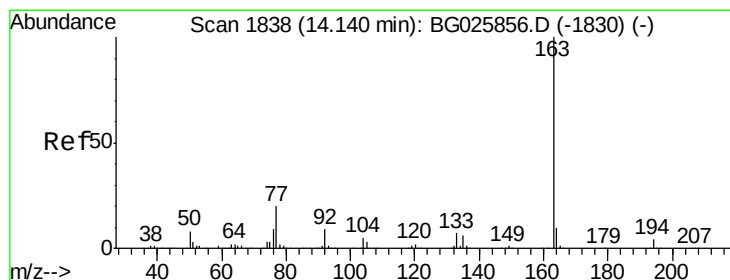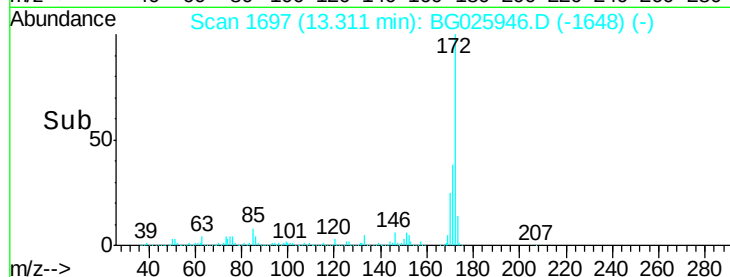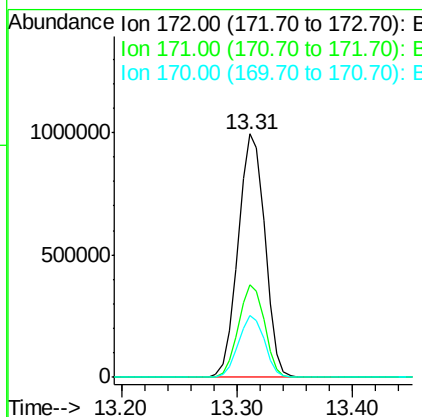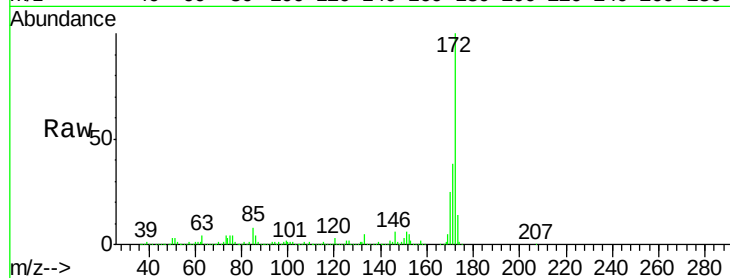

#49
Dimethylphthalate
Concen: 5.44 ng
RT: 14.13 min Scan# 1836
Delta R.T. -0.01 min
Lab File: BG025946.D
Acq: 25 Feb 2017 00:20

Tgt Ion:163 Resp: 97540
Ion Ratio Lower Upper
163 100
194 4.1 3.8 5.6
164 10.0 9.3 13.9

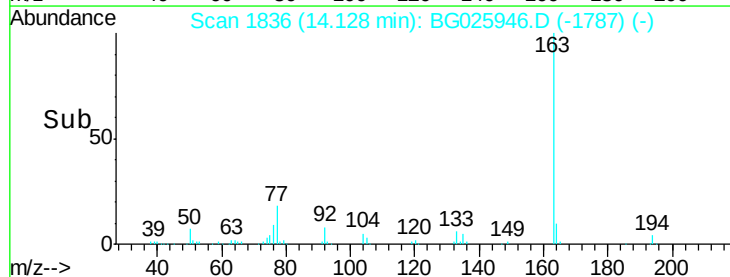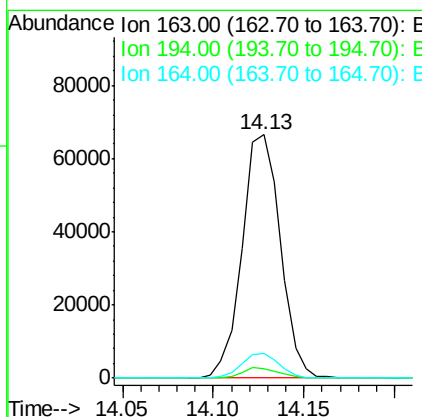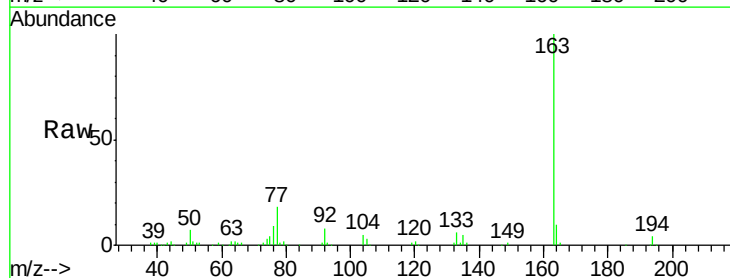

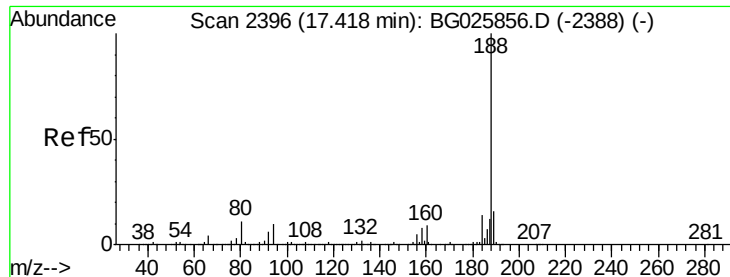

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 17.41 min Scan# 2395

Delta R.T. -0.01 min

Lab File: BG025946.D

Acq: 25 Feb 2017 00:20

Instrument :

BNA_G

ClientSampleId :

E2-Y6N-SW


Tgt Ion:188 Resp: 714161

Ion Ratio Lower Upper

188 100

94 9.7 5.8 8.8#

80 10.7 7.5 11.3

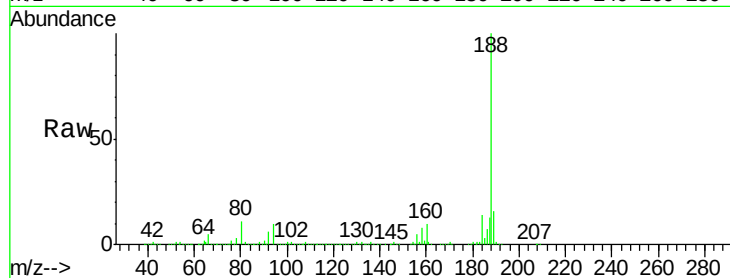

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): B

Ion 80.00 (79.70 to 80.70): B

600000

500000

400000

300000

200000

100000



0

17.41

17.40

17.50

Time-->

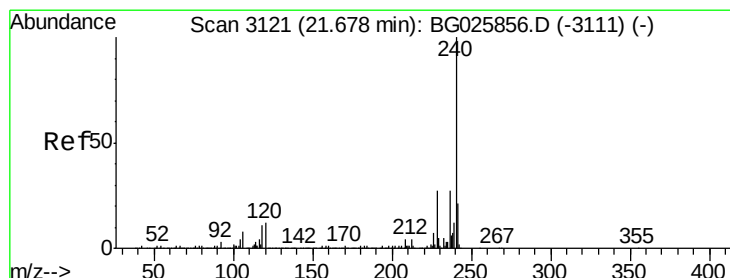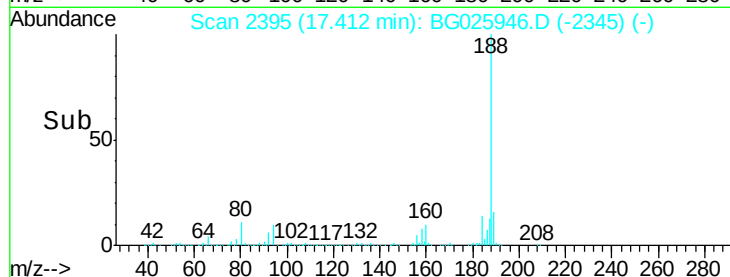

#75

Chrysene-d12

Concen: 20.00 ng

RT: 21.66 min Scan# 3118

Delta R.T. -0.02 min

Lab File: BG025946.D

Acq: 25 Feb 2017 00:20


Tgt Ion:240 Resp: 767594

Ion Ratio Lower Upper

240 100

120 12.0 5.7 8.5#

236 25.2 22.2 33.4

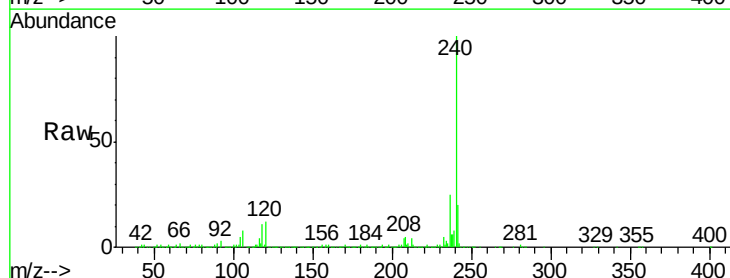

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

600000

500000

400000

300000

200000

100000

0


21.66


21.60

21.70

21.80

Time-->

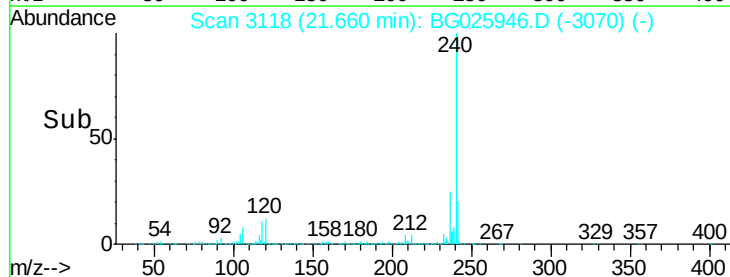

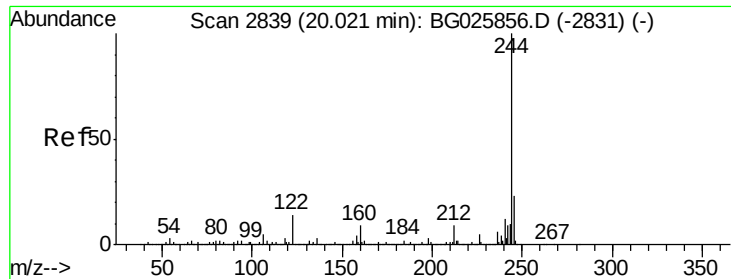

#78

Terphenyl-d14

Concen: 77.19 ng

RT: 20.01 min Scan# 2837

Delta R.T. -0.01 min

Lab File: BG025946.D

Acq: 25 Feb 2017 00:20

Instrument :

BNA_G

ClientSampleId :

E2-Y6N-SW


Tgt Ion:244 Resp: 2436066

Ion Ratio Lower Upper

244 100

212 8.8 10.0 15.0#




122 14.2 8.6 12.8#

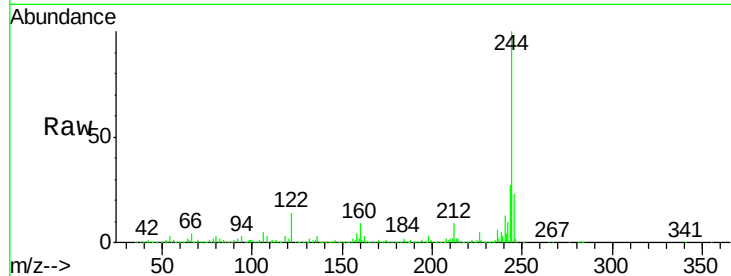

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

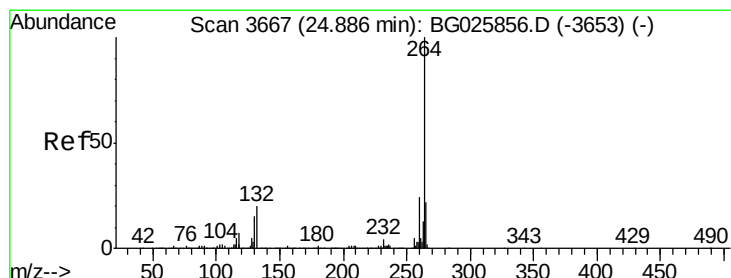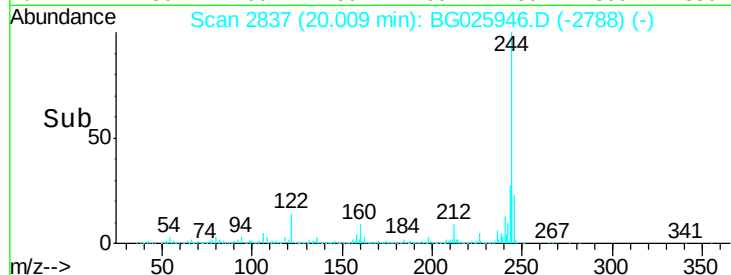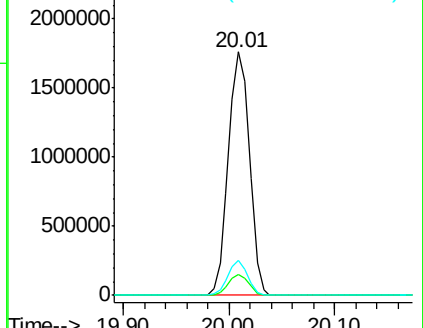

#86

Perylene-d12

Concen: 20.00 ng

RT: 24.86 min Scan# 3663

Delta R.T. -0.02 min

Lab File: BG025946.D

Acq: 25 Feb 2017 00:20


Tgt Ion:264 Resp: 745867

Ion Ratio Lower Upper

264 100

260 23.6 21.8 32.8

265 21.5 18.2 27.4

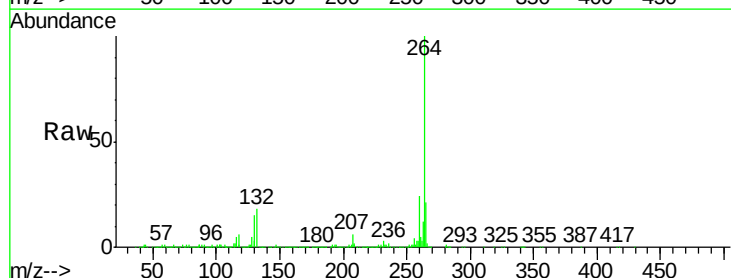

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

