


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022417\
 Data File : BG025933.D
 Acq On : 24 Feb 2017 15:35
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 15:48:21 2017

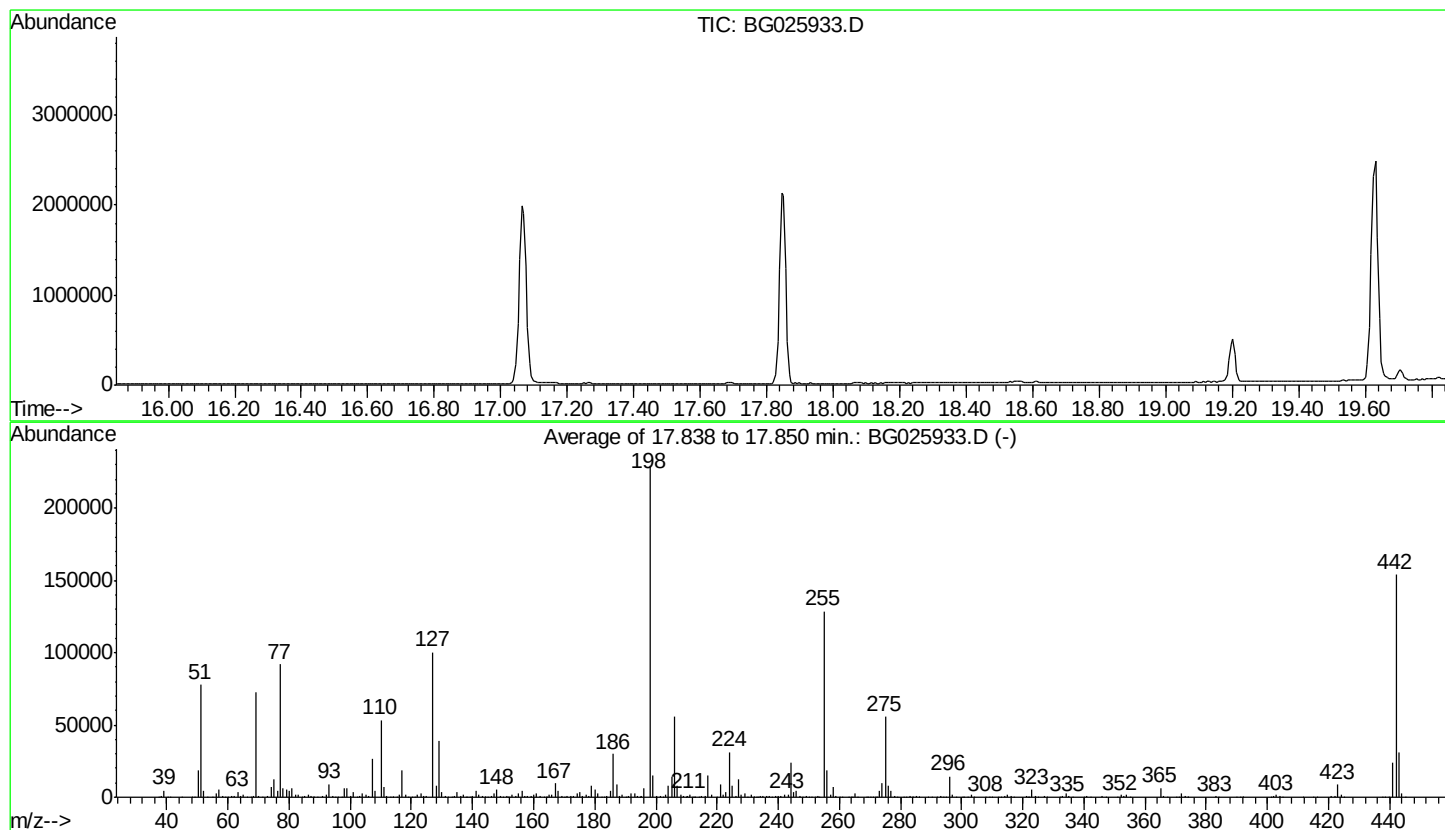

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	77674	PASS
68	69	0.00	2	1.9	1343	PASS
69	198	0.00	100	31.5	72335	PASS
70	69	0.00	2	0.7	533	PASS
127	198	10	80	43.7	100373	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	229546	PASS
199	198	5	9	6.7	15342	PASS
275	198	10	60	24.2	55586	PASS
365	198	1	100	2.8	6330	PASS
441	442	0.01	24	15.8	24309	PASS
442	198	50	100	67.2	154168	PASS
443	442	15	24	20.1	30984	PASS