


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022417\
 Data File : BG025950.D
 Acq On : 25 Feb 2017 2:59
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG021717.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 15:48:21 2017

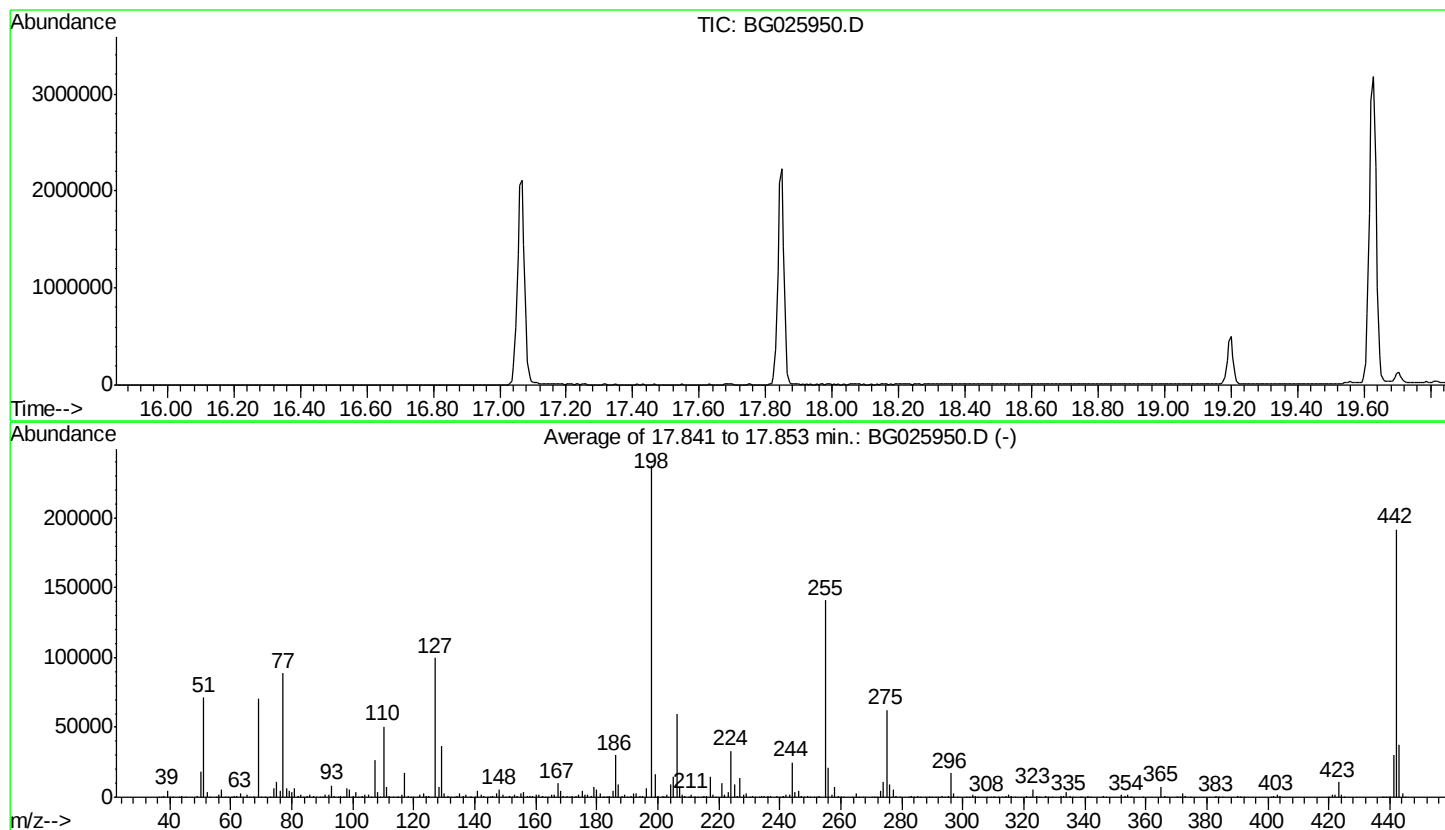

AutoFind: Scans 2468, 2469, 2470; Background Corrected with Scan 2460

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.1	71493	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	29.5	70170	PASS
70	69	0.00	2	0.6	446	PASS
127	198	10	80	42.0	99850	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	237504	PASS
199	198	5	9	6.9	16386	PASS
275	198	10	60	26.3	62413	PASS
365	198	1	100	3.3	7798	PASS
441	442	0.01	24	16.0	30706	PASS
442	198	50	100	80.8	191850	PASS
443	442	15	24	19.7	37757	PASS