

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022423\
 Data File : BG056721.D
 Acq On : 24 Feb 2023 14:27
 Operator : CG/JU
 Sample : PB150959BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.696	23	27	32	rVV4	4247	6106	1.02%	0.105%
2	4.131	97	101	109	rVV	51073	84240	14.09%	1.445%
3	4.484	159	161	162	rBV2	1196	1075	0.18%	0.018%
4	4.496	162	163	166	rVB3	1992	1244	0.21%	0.021%
5	6.205	452	454	458	rVB3	915	1055	0.18%	0.018%
6	6.241	458	460	463	rBV	696	959	0.16%	0.016%
7	6.370	481	482	487	rVB2	737	957	0.16%	0.016%
8	6.740	540	545	547	rVV2	670	974	0.16%	0.017%
9	7.010	589	591	595	rVB2	870	1004	0.17%	0.017%
10	7.057	595	599	601	rBV2	711	1002	0.17%	0.017%
11	7.192	621	622	626	rBV2	908	1053	0.18%	0.018%
12	7.539	674	681	688	rBV	72172	122824	20.55%	2.107%
13	7.721	705	712	718	rVB	49231	83471	13.96%	1.432%
14	7.939	742	749	756	rVB2	63014	109687	18.35%	1.882%
15	8.420	824	831	837	rVV	59591	102370	17.12%	1.756%
16	9.102	941	947	956	rVV	88061	149202	24.96%	2.560%
17	9.590	1022	1030	1038	rVB	72650	127382	21.31%	2.186%
18	10.318	1146	1154	1163	rBV2	62607	107923	18.05%	1.852%
19	10.859	1238	1246	1254	rBV	93176	155163	25.96%	2.662%
20	11.258	1305	1314	1322	rBV	90860	158565	26.52%	2.721%
21	11.376	1327	1334	1344	rVB	91080	160252	26.81%	2.750%
22	12.809	1571	1578	1581	rBV3	1483	2369	0.40%	0.041%
23	14.407	1844	1850	1858	rVB	202403	295277	49.39%	5.066%
24	14.725	1897	1904	1911	rVB	204165	315514	52.78%	5.414%
25	15.024	1949	1955	1961	rBV	166902	256422	42.89%	4.400%
26	15.177	1974	1981	1993	rBV2	102128	161717	27.05%	2.775%
27	16.006	2116	2122	2129	rVB	284908	421320	70.48%	7.229%
28	16.105	2133	2139	2144	rBV	96815	137729	23.04%	2.363%
29	17.762	2413	2421	2427	rVV	235205	358274	59.93%	6.147%
30	17.856	2429	2437	2443	rVV2	325696	489885	81.95%	8.406%
31	19.237	2669	2672	2675	rVB2	1266	1051	0.18%	0.018%
32	19.684	2742	2748	2752	rBV4	4968	8028	1.34%	0.138%
33	19.754	2756	2760	2764	rBV2	4610	6028	1.01%	0.103%
34	20.007	2801	2803	2807	rBV2	773	1265	0.21%	0.022%
35	20.118	2815	2822	2829	rBV	425152	597813	100.00%	10.257%
36	20.306	2852	2854	2855	rBV2	1399	1064	0.18%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022423\
 Data File : BG056721.D
 Acq On : 24 Feb 2023 14:27
 Operator : CG/JU
 Sample : PB150959BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	20.389	2865	2868	2870	rBV2	1231	1020	0.17%	0.018%
38	20.418	2870	2873	2874	rVV2	1470	1340	0.22%	0.023%
39	20.453	2878	2879	2882	rBV2	1765	1703	0.28%	0.029%
40	20.547	2893	2895	2896	rBV2	2068	1071	0.18%	0.018%
41	20.571	2896	2899	2901	rBV4	1908	2349	0.39%	0.040%
42	20.635	2908	2910	2913	rVV4	1616	1579	0.26%	0.027%
43	20.776	2932	2934	2935	rBV2	2148	1698	0.28%	0.029%
44	20.841	2944	2945	2947	rBV2	2113	1214	0.20%	0.021%
45	20.923	2957	2959	2961	rBV3	1823	2260	0.38%	0.039%
46	21.070	2982	2984	2986	rBV2	1967	1465	0.25%	0.025%
47	21.147	2995	2997	2998	rBV2	2253	1508	0.25%	0.026%
48	21.405	3039	3041	3042	rVB2	3096	1580	0.26%	0.027%
49	22.069	3147	3154	3161	rBV2	225485	373634	62.50%	6.411%
50	22.234	3180	3182	3184	rBV3	2426	1866	0.31%	0.032%
51	22.386	3206	3208	3209	rBV2	2429	1453	0.24%	0.025%
52	23.127	3333	3334	3337	rVB3	3774	2528	0.42%	0.043%
53	23.156	3337	3339	3340	rBV2	1966	1511	0.25%	0.026%
54	23.603	3413	3415	3417	rBV3	2012	1239	0.21%	0.021%
55	23.655	3420	3424	3427	rBV6	5211	8521	1.43%	0.146%
56	23.996	3480	3482	3483	rBV2	2176	1603	0.27%	0.028%
57	24.537	3570	3574	3581	rVB10	6499	14635	2.45%	0.251%
58	24.748	3608	3610	3615	rBV5	2972	4078	0.68%	0.070%
59	25.353	3703	3713	3725	rVB2	177240	520353	87.04%	8.928%
60	25.494	3736	3737	3738	rVB	3288	1159	0.19%	0.020%
61	25.600	3744	3755	3766	rVB2	120381	361889	60.54%	6.209%
62	25.729	3775	3777	3779	rBV3	1728	1670	0.28%	0.029%
63	25.923	3809	3810	3811	rVB	3202	1129	0.19%	0.019%
64	26.070	3833	3835	3836	rBV2	2547	1474	0.25%	0.025%
65	26.164	3850	3851	3852	rBV	2932	1475	0.25%	0.025%
66	26.211	3858	3859	3862	rBV3	2255	1625	0.27%	0.028%
67	26.529	3911	3913	3915	rBV3	1665	1057	0.18%	0.018%
68	26.834	3961	3965	3966	rBV4	3370	4520	0.76%	0.078%
69	26.852	3966	3968	3971	rVV4	3032	3868	0.65%	0.066%
70	27.222	4029	4031	4033	rBV3	2405	1646	0.28%	0.028%
71	27.292	4041	4043	4044	rBV2	1883	932	0.16%	0.016%
72	27.492	4075	4077	4080	rBV3	2349	2969	0.50%	0.051%
73	27.621	4097	4099	4101	rBV3	2530	2516	0.42%	0.043%
74	28.097	4178	4180	4181	rBV2	3403	2294	0.38%	0.039%
75	28.274	4208	4210	4212	rVB3	3791	2689	0.45%	0.046%
76	28.297	4212	4214	4215	rBV2	2562	1453	0.24%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022423\
 Data File : BG056721.D
 Acq On : 24 Feb 2023 14:27
 Operator : CG/JU
 Sample : PB150959BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK959

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

77	28.503	4248	4249	4250	rVB	2916	1028	0.17%	0.018%
78	28.520	4250	4252	4254	rBV3	2549	3087	0.52%	0.053%
79	28.761	4292	4293	4294	rVB	3586	1264	0.21%	0.022%
80	28.914	4317	4319	4323	rBV5	1779	2256	0.38%	0.039%
81	28.996	4331	4333	4335	rVB3	2283	1429	0.24%	0.025%
82	29.102	4349	4351	4355	rBV4	2202	2423	0.41%	0.042%
83	29.308	4384	4386	4387	rVB2	2700	1271	0.21%	0.022%
84	29.325	4387	4389	4390	rBV2	2289	1596	0.27%	0.027%
85	29.449	4408	4410	4412	rBV3	2019	1950	0.33%	0.033%
86	29.889	4483	4485	4487	rBV3	2447	1923	0.32%	0.033%
87	30.024	4506	4508	4511	rVB3	2863	2356	0.39%	0.040%
88	30.060	4512	4514	4516	rBV3	2094	1591	0.27%	0.027%
89	30.171	4531	4533	4535	rBV3	2983	2773	0.46%	0.048%
90	30.218	4538	4541	4546	rVV6	3195	5696	0.95%	0.098%
91	30.371	4565	4567	4569	rBV3	3173	3049	0.51%	0.052%
92	30.841	4646	4647	4648	rBV	2290	1063	0.18%	0.018%
93	31.041	4679	4681	4683	rBV3	2144	1663	0.28%	0.029%
94	31.587	4772	4774	4777	rBV4	2879	2451	0.41%	0.042%
95	31.822	4813	4814	4816	rVB2	3339	1973	0.33%	0.034%
96	31.846	4816	4818	4820	rBV3	2877	2643	0.44%	0.045%
97	32.057	4852	4854	4858	rBV5	2475	3450	0.58%	0.059%
98	32.151	4868	4870	4871	rBV2	2476	2014	0.34%	0.035%
99	32.286	4891	4893	4894	rBV2	1940	1090	0.18%	0.019%
100	32.375	4906	4908	4911	rBV4	2528	3250	0.54%	0.056%




Sum of corrected areas: 5828126

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022423\
Data File : BG056721.D
Acq On : 24 Feb 2023 14:27
Operator : CG/JU
Sample : PB150959BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

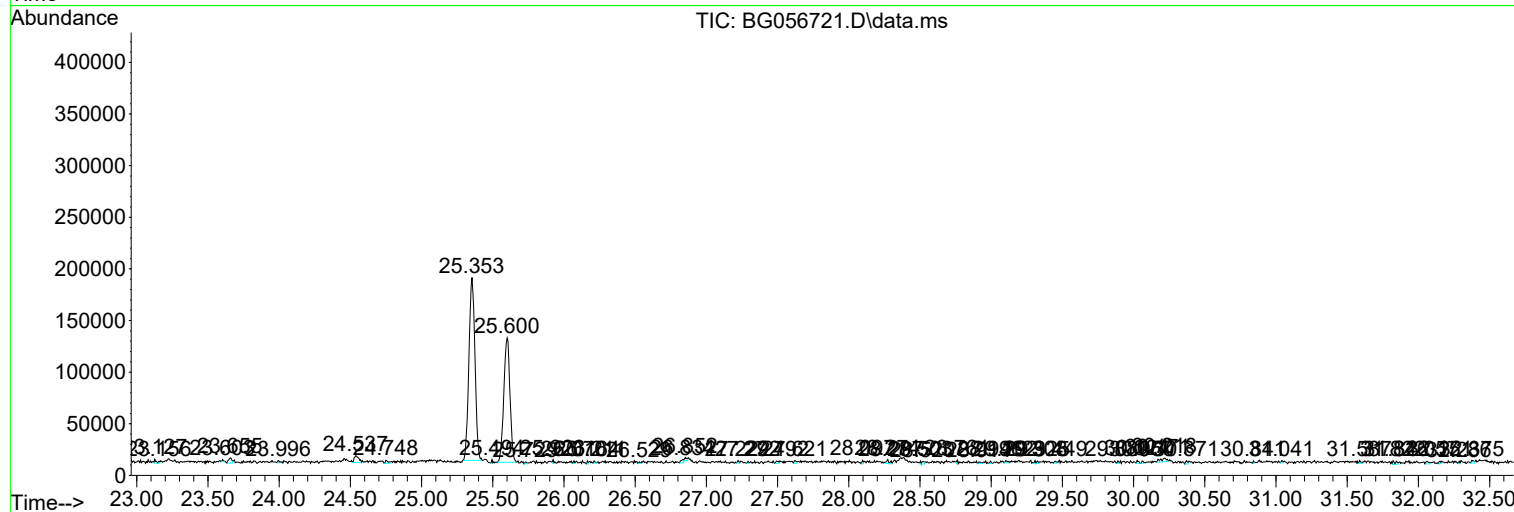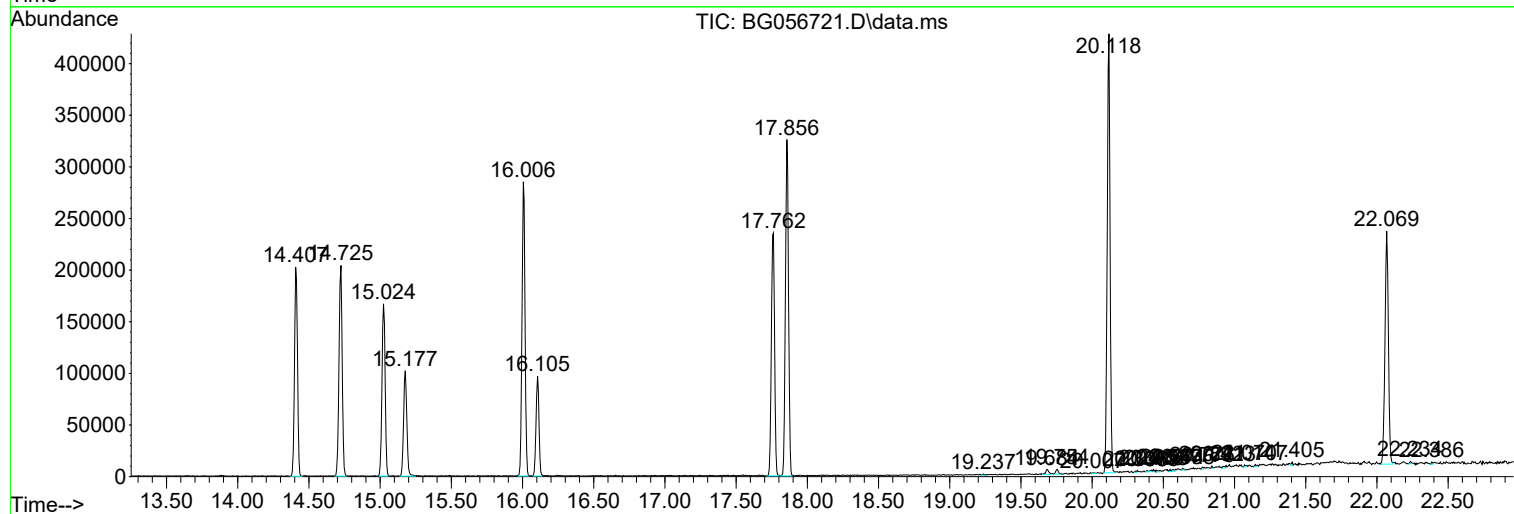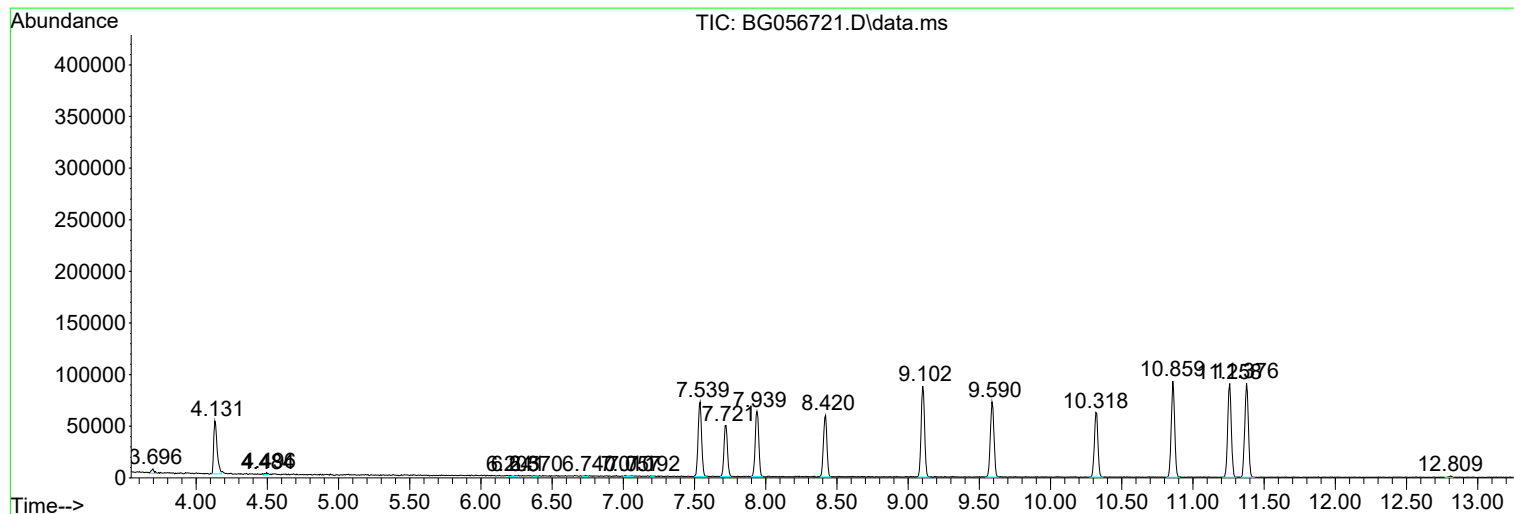

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022423\
Data File : BG056721.D
Acq On : 24 Feb 2023 14:27
Operator : CG/JU
Sample : PB150959BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022423\
Data File : BG056721.D
Acq On : 24 Feb 2023 14:27
Operator : CG/JU
Sample : PB150959BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK959

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc