

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022615\
 Data File : BF077468.D
 Acq On : 26 Feb 2015 16:40
 Operator : TP/IZ
 Sample : G1348-07
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 36A-EW-022515

Quant Time: Feb 26 17:32:54 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 26 17:14:46 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.26	152	58853	20.00	ng	0.00
21) Naphthalene-d8	8.84	136	233475	20.00	ng	0.00
38) Acenaphthene-d10	11.01	164	118665	20.00	ng	-0.01
63) Phenanthrene-d10	12.87	188	240875	20.00	ng	0.00
75) Chrysene-d12	16.17	240	275936	20.00	ng	-0.01
86) Perylene-d12	17.97	264	275770	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.56	112	363239	103.04	ng	0.00
7) Phenol-d6	6.82	99	442373	97.60	ng	-0.01
23) Nitrobenzene-d5	7.96	82	264580	70.47	ng	0.00
41) 2,4,6-Tribromophenol	12.00	330	130644	114.34	ng	-0.01
44) 2-Fluorobiphenyl	10.19	172	588982	77.39	ng	0.00
78) Terphenyl-d14	14.87	244	741717	62.84	ng	0.00
Target Compounds						
10) Phenol	6.84	94	10878	2.02	ng	94
49) Dimethylphthalate	10.69	163	43490	5.21	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF022615\
Data File : BF077468.D
Acq On : 26 Feb 2015 16:40
Operator : TP/IZ
Sample : G1348-07
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
36A-EW-022515

Quant Time: Feb 26 17:32:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 26 17:14:46 2015
Response via : Initial Calibration

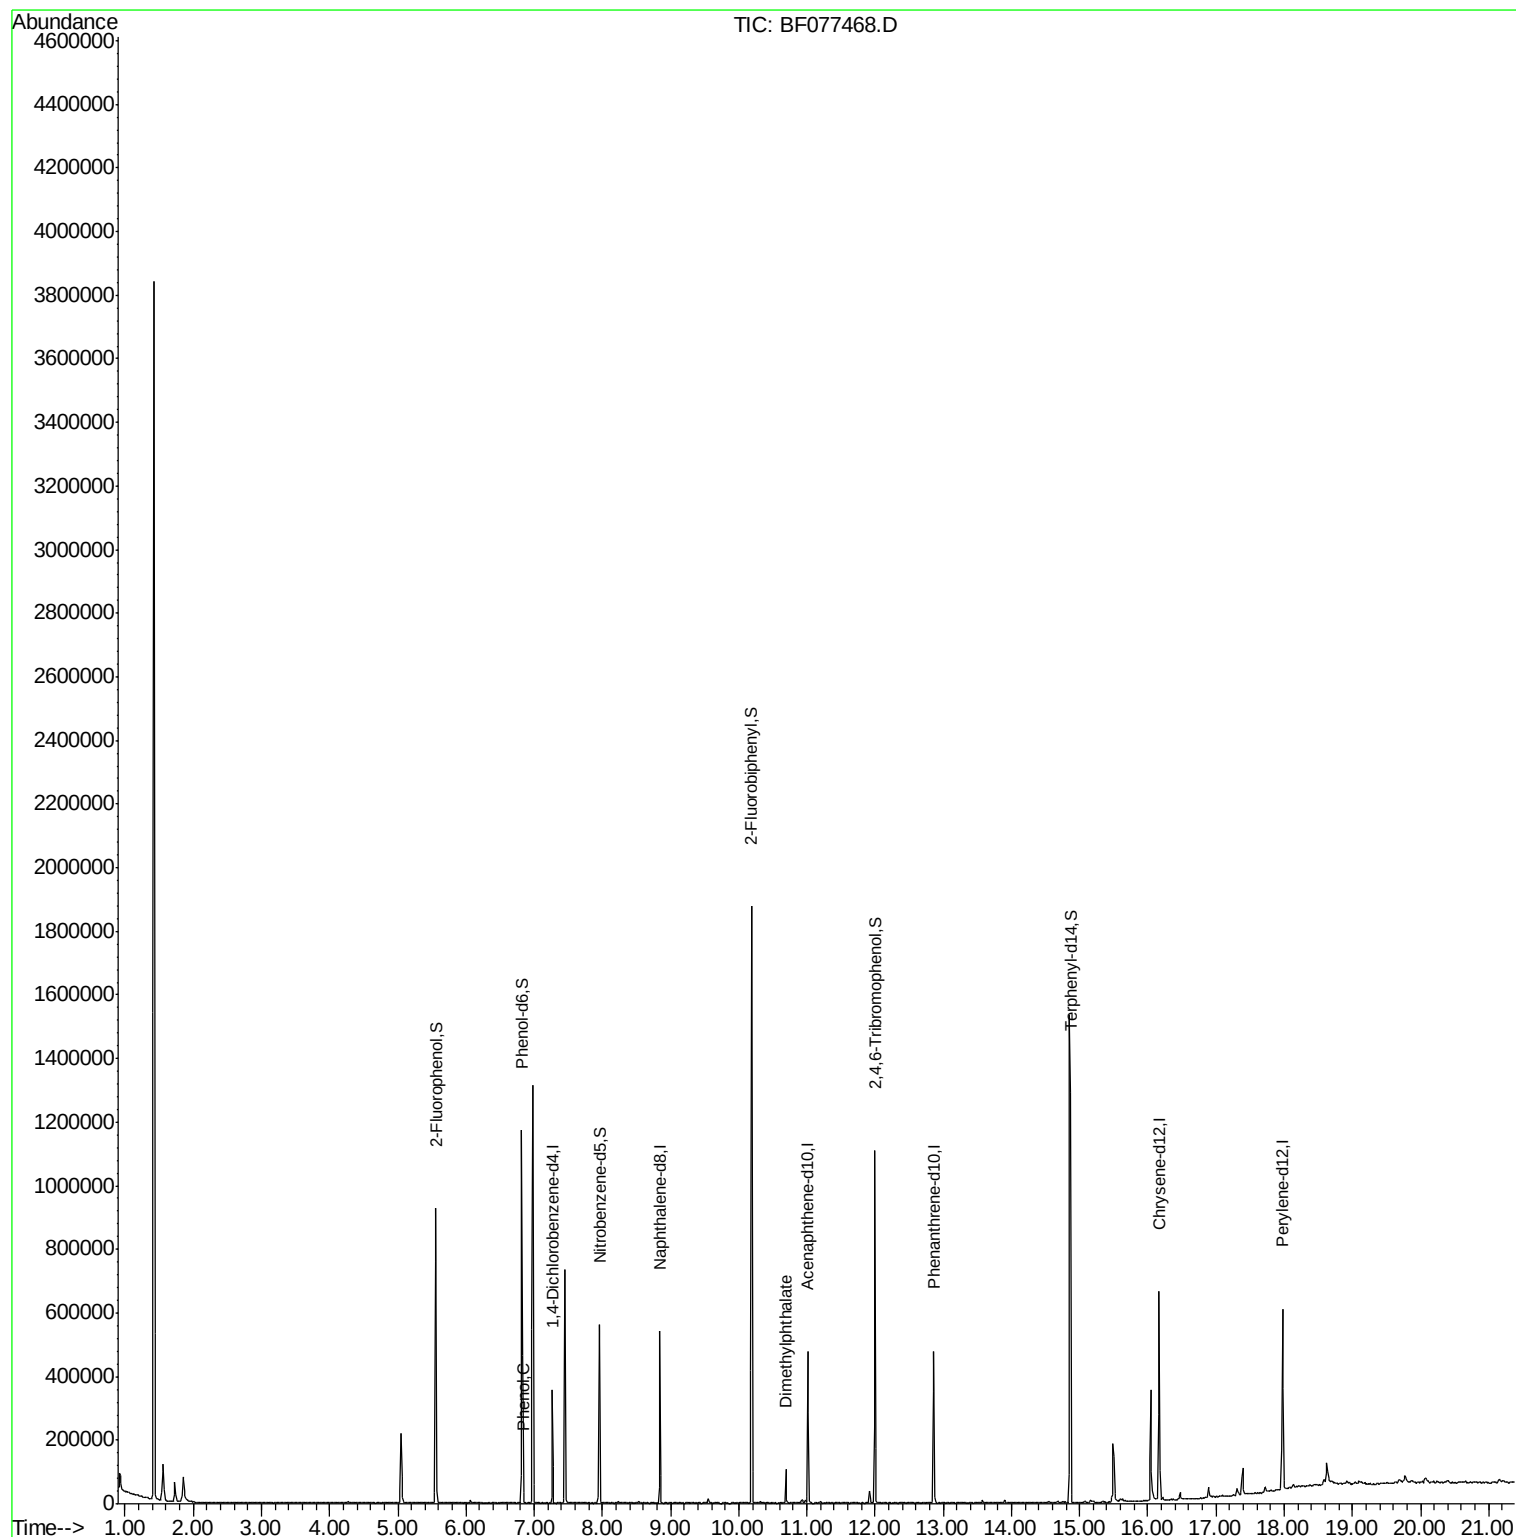

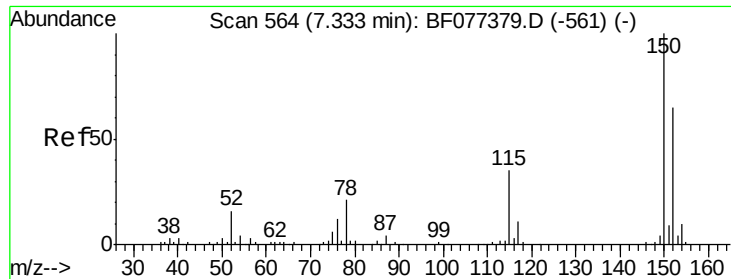


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.26 min Scan# 558
Delta R.T. 0.00 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Instrument :
BNA_G
ClientSampleId :
36A-EW-022515

Tgt Ion:152 Resp: 58853
Ion Ratio Lower Upper
152 100
150 154.2 124.0 186.0
115 62.8 49.4 74.2

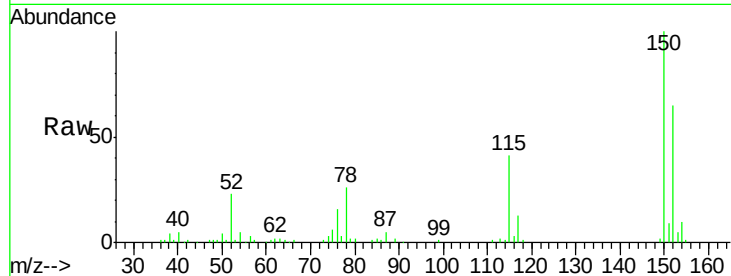


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

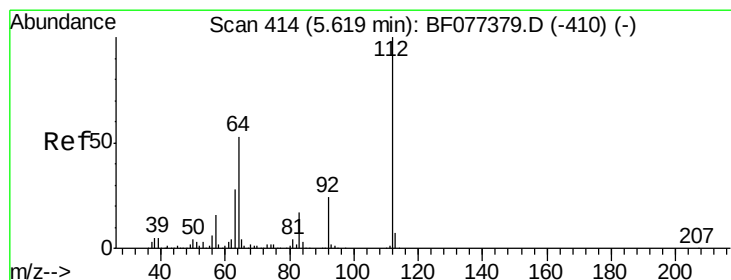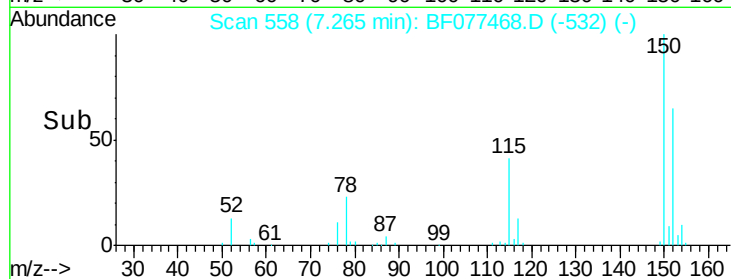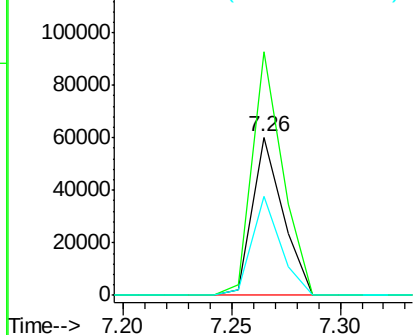



#5


2-Fluorophenol
Concen: 103.04 ng
RT: 5.56 min Scan# 409
Delta R.T. 0.00 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Tgt Ion:112 Resp: 363239
Ion Ratio Lower Upper
112 100
64 48.3 48.5 72.7#
63 25.2 25.0 37.4

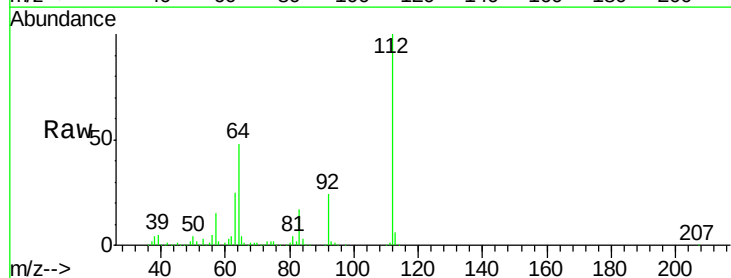

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

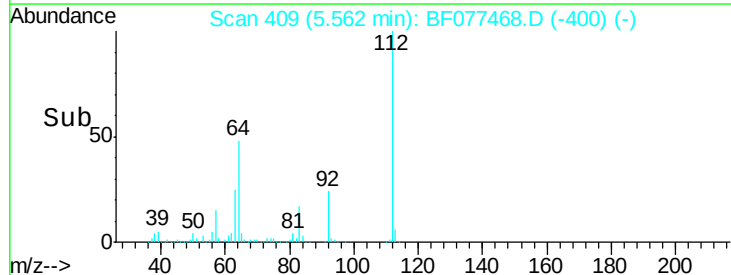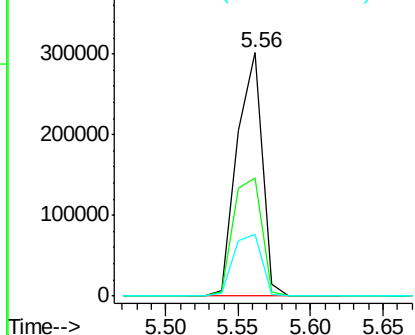

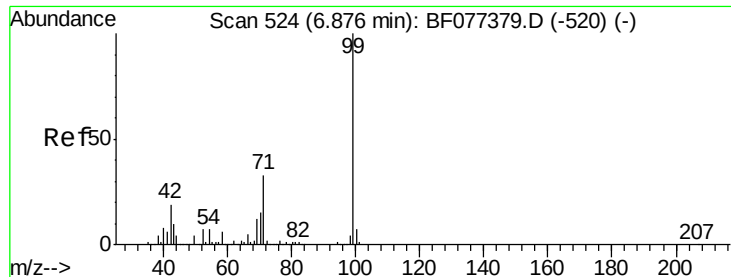

#7

Phenol-d6

Concen: 97.60 ng

RT: 6.82 min Scan# 519

Delta R.T. -0.01 min

Lab File: BF077468.D

Acq: 26 Feb 2015 16:40

Instrument :

BNA_G

ClientSampleId :

36A-EW-022515


Tgt Ion: 99 Resp: 442373

Ion Ratio Lower Upper

99 100

42 19.5 16.2 24.4

71 33.4 26.7 40.1

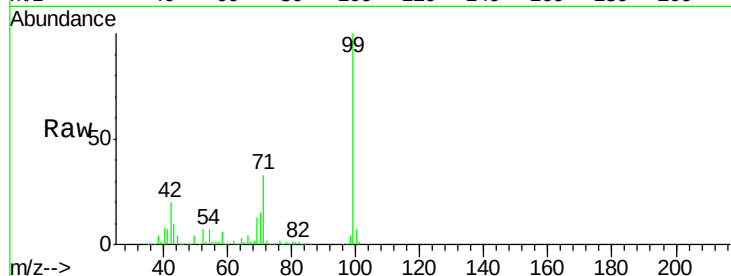

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

500000

400000

300000



200000

100000

0

6.82

Time-->

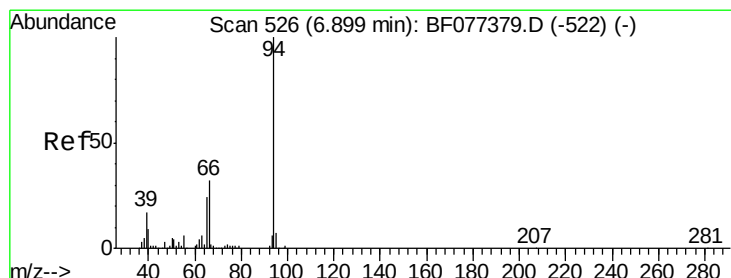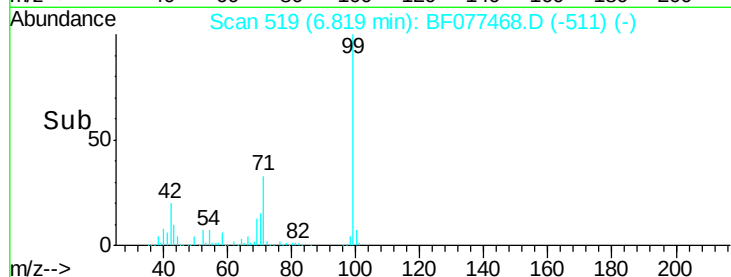

#10

Phenol

Concen: 2.02 ng

RT: 6.84 min Scan# 521

Delta R.T. 0.00 min

Lab File: BF077468.D

Acq: 26 Feb 2015 16:40


Tgt Ion: 94 Resp: 10878

Ion Ratio Lower Upper

94 100

65 27.5 5.7 45.7

66 37.7 13.6 53.6

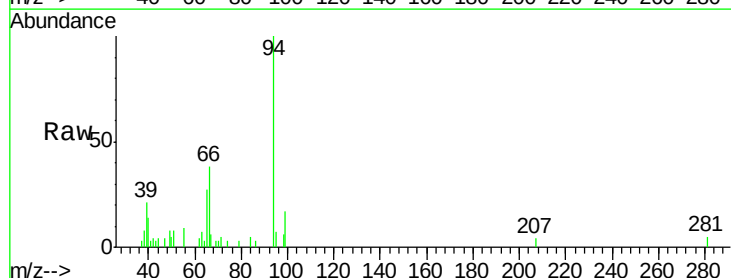

Abundance Ion 94.00 (93.70 to 94.70): BF0

Ion 65.00 (64.70 to 65.70): BF0

Ion 66.00 (65.70 to 66.70): BF0

25000

20000

15000


10000


5000

0

6.84

Time-->

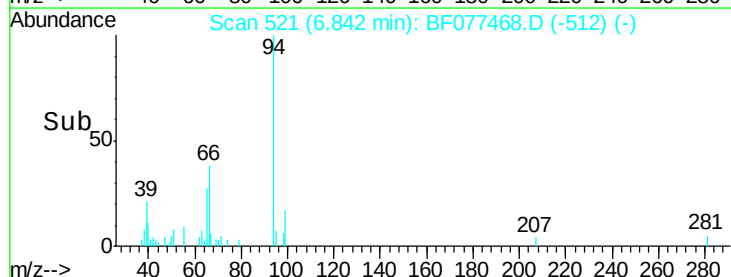


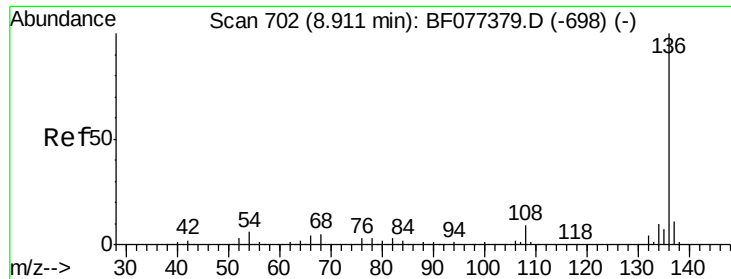




#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.84 min Scan# 696
Delta R.T. 0.00 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Instrument :
BNA_G
ClientSampleId :
36A-EW-022515

Tgt Ion:	136	Resp:	233475
Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.6	13.0
54	7.4	6.2	9.4
68	5.6	5.0	7.6

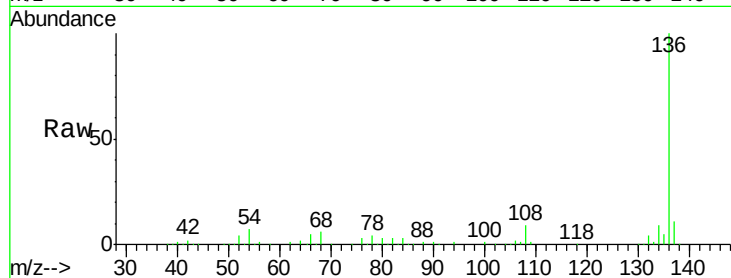


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

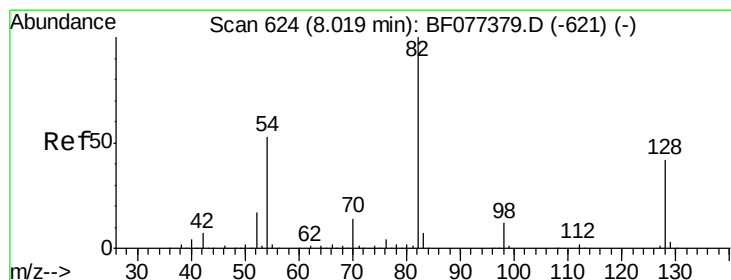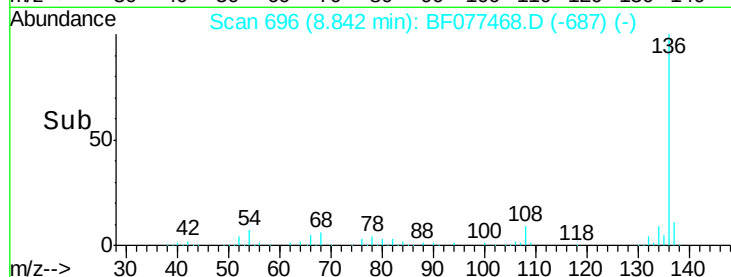
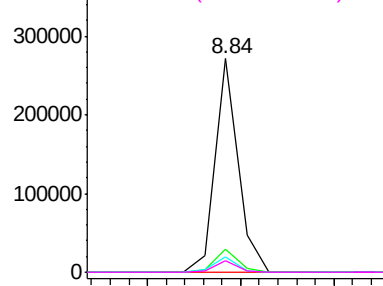



#23
Nitrobenzene-d5
Concen: 70.47 ng
RT: 7.96 min Scan# 619
Delta R.T. 0.00 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Tgt Ion:	82	Resp:	264580
Ion	Ratio	Lower	Upper
82	100		
128	54.3	43.8	65.8
54	44.3	36.7	55.1

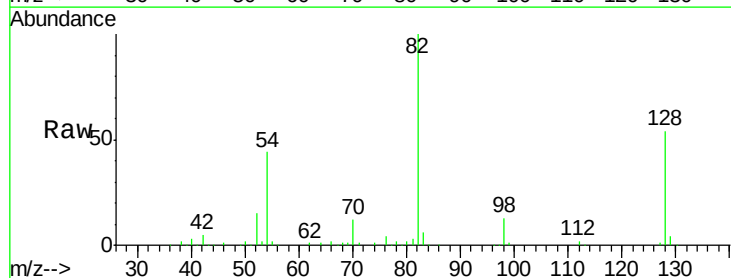

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF0



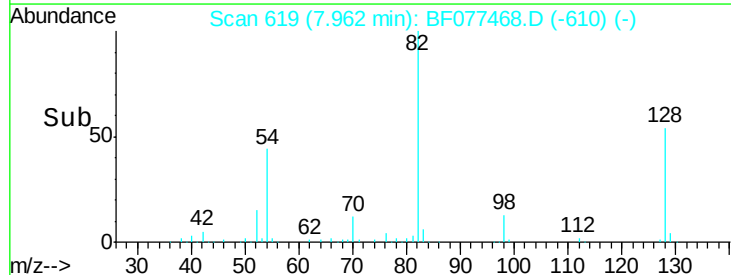
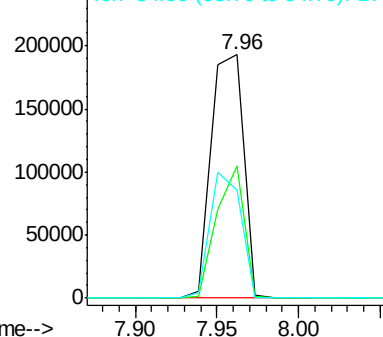


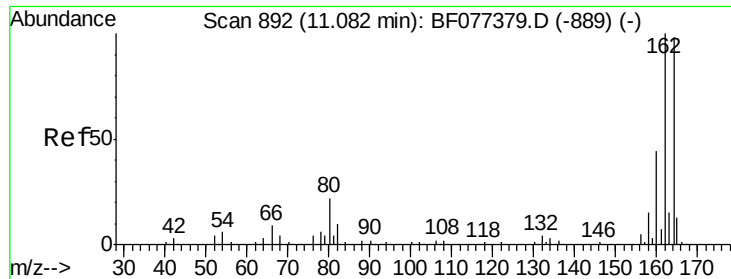

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 11.01 min Scan# 886
Delta R.T. -0.01 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40




Instrument :
BNA_G
ClientSampleId :
36A-EW-022515


Tgt Ion:164 Resp: 118665
Ion Ratio Lower Upper
164 100
162 102.6 83.2 124.8
160 45.0 34.6 52.0

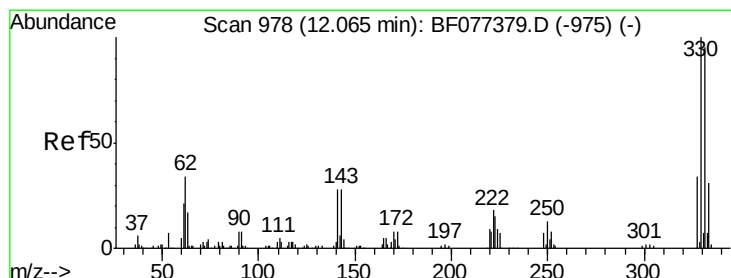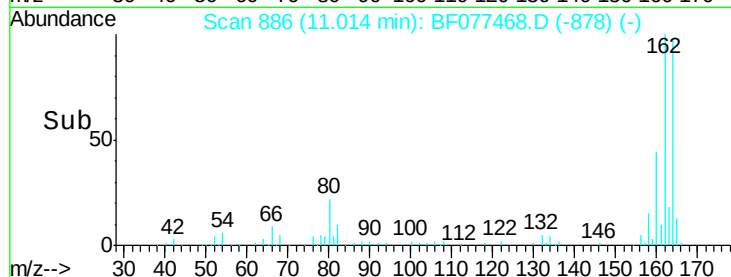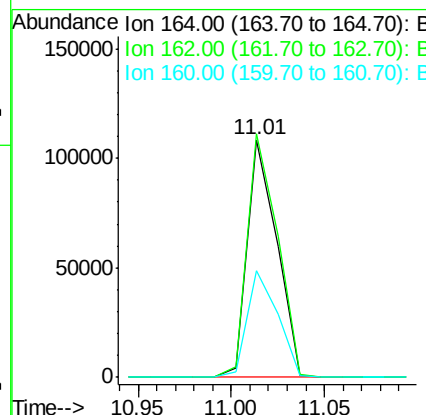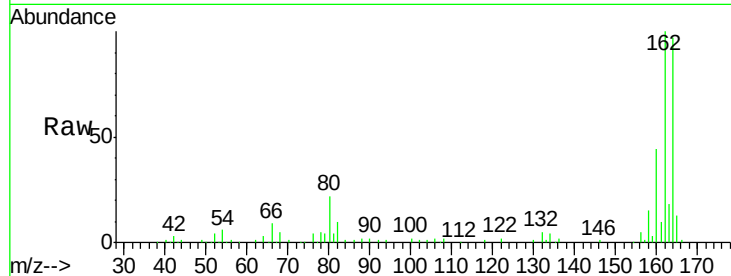

#41
2,4,6-Tribromophenol
Concen: 114.34 ng
RT: 12.00 min Scan# 972
Delta R.T. -0.01 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Tgt Ion:330 Resp: 130644
Ion Ratio Lower Upper
330 100
332 96.7 77.4 116.2
141 35.8 28.8 43.2


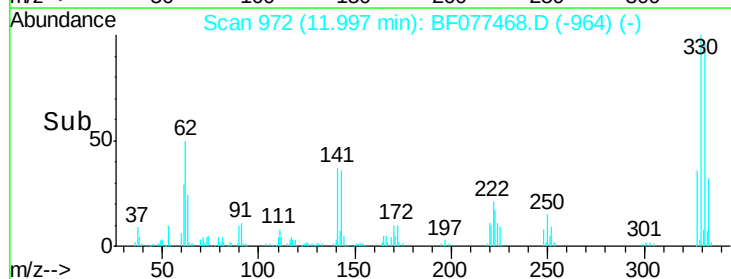
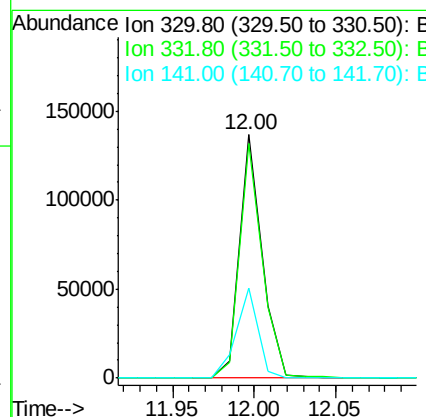
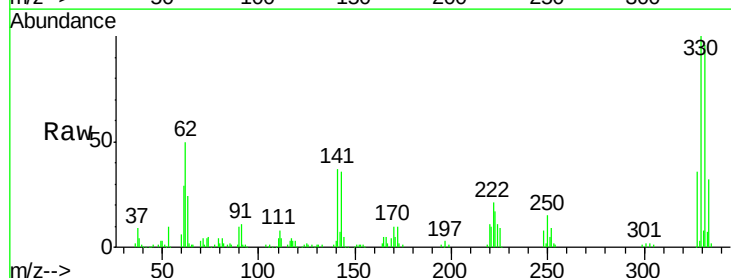


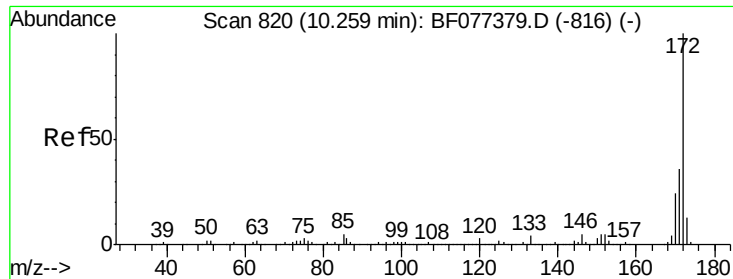

#44
2-Fluorobiphenyl
Concen: 77.39 ng
RT: 10.19 min Scan# 814
Delta R.T. 0.00 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40




Instrument :
BNA_G
ClientSampleId :
36A-EW-022515


Tgt Ion:172 Resp: 588982
Ion Ratio Lower Upper
172 100
171 35.4 28.9 43.3
170 23.6 19.4 29.2

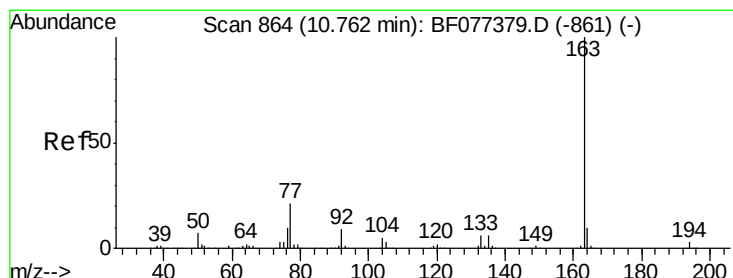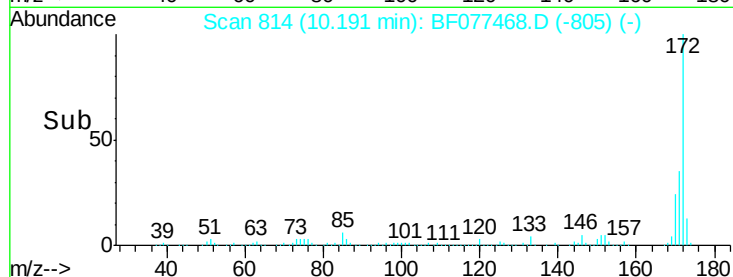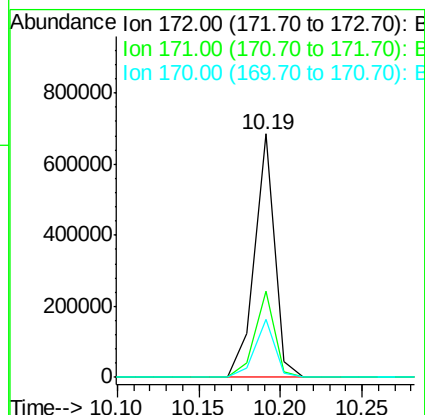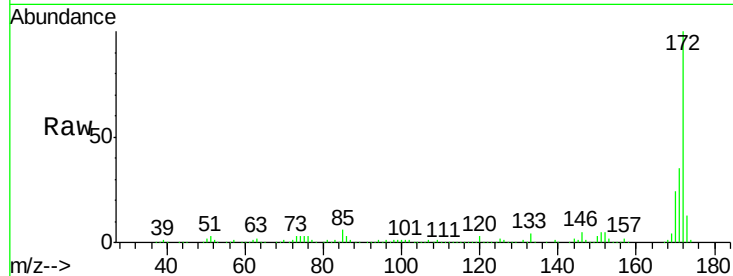

#49
Dimethylphthalate
Concen: 5.21 ng
RT: 10.69 min Scan# 858
Delta R.T. -0.01 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Tgt Ion:163 Resp: 43490
Ion Ratio Lower Upper
163 100
194 3.1 2.6 4.0
164 9.7 8.6 13.0


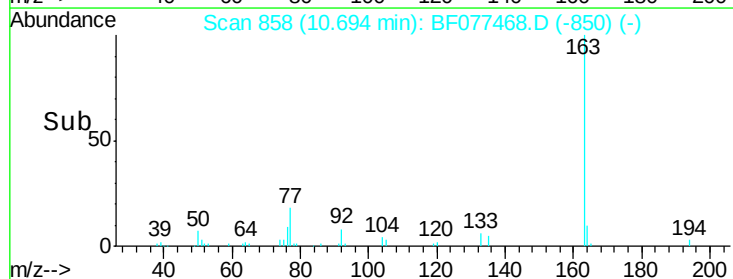
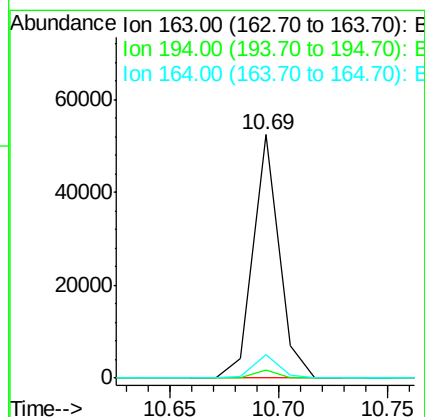
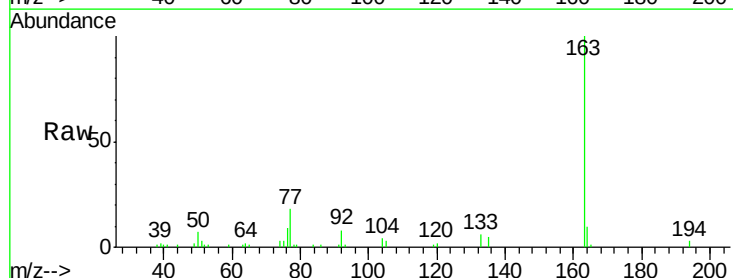


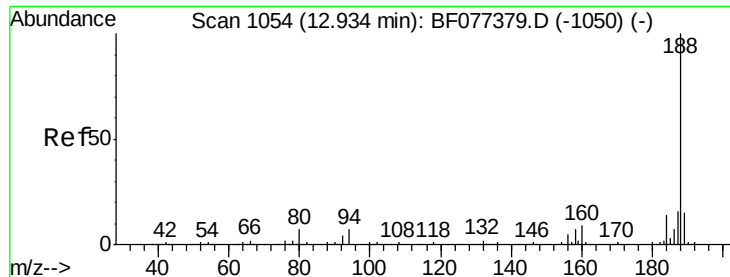

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.87 min Scan# 1048
Delta R.T. 0.00 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40




Instrument :
BNA_G
ClientSampleId :
36A-EW-022515


Tgt Ion:188 Resp: 240875
Ion Ratio Lower Upper
188 100
94 7.2 7.4 11.2#
80 7.3 8.0 12.0#

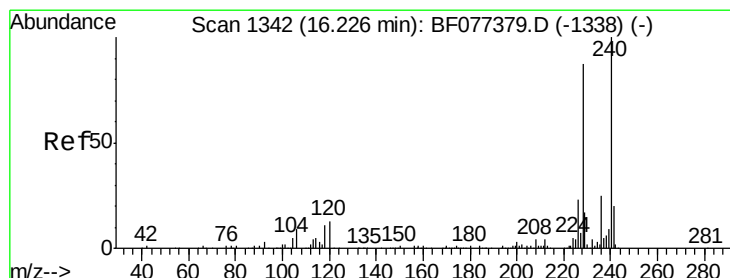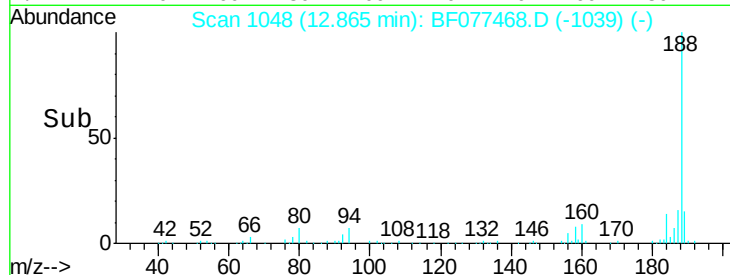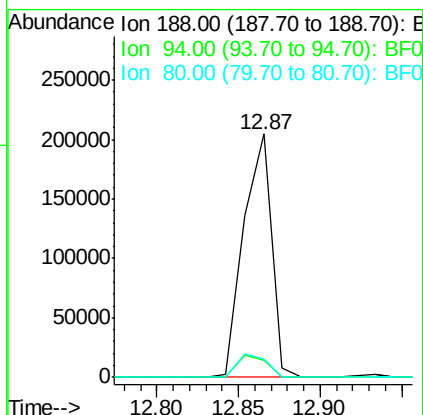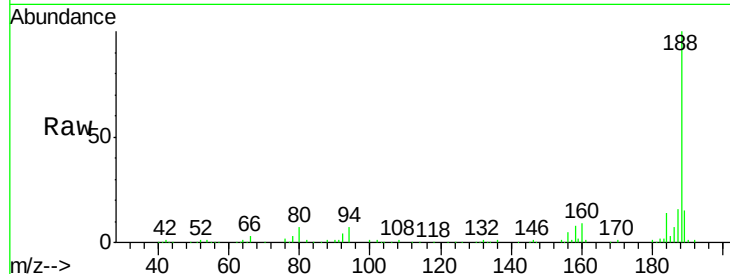

#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.17 min Scan# 1337
Delta R.T. -0.01 min
Lab File: BF077468.D
Acq: 26 Feb 2015 16:40

Tgt Ion:240 Resp: 275936
Ion Ratio Lower Upper
240 100
120 10.3 8.8 13.2
236 25.3 20.7 31.1


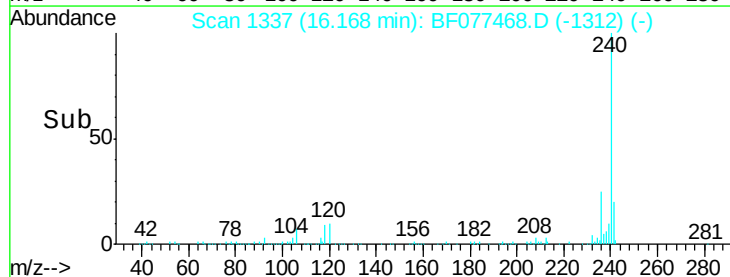
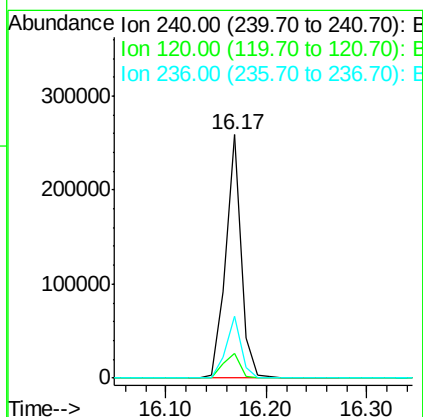
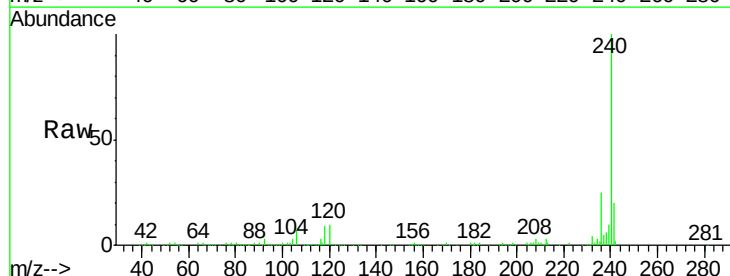


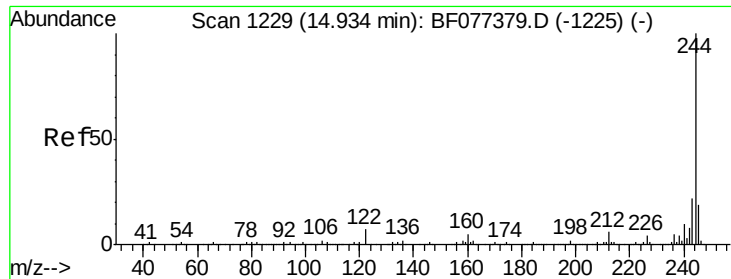

#78
 Terphenyl-d14
 Concen: 62.84 ng
 RT: 14.87 min Scan# 1223
 Delta R.T. 0.00 min
 Lab File: BF077468.D
 Acq: 26 Feb 2015 16:40

Instrument :
 BNA_G
 ClientSampleId :
 36A-EW-022515

Tgt Ion:244 Resp: 741717
 Ion Ratio Lower Upper
 244 100
 212 5.7 5.2 7.8
 122 6.2 7.8 11.8#

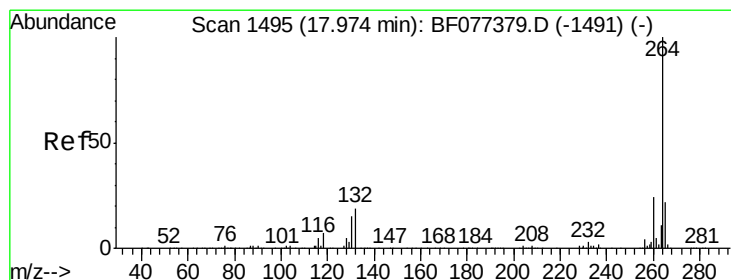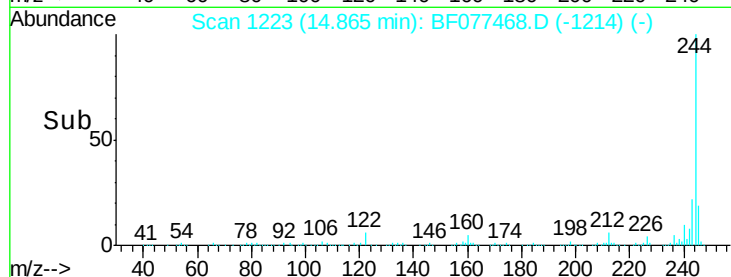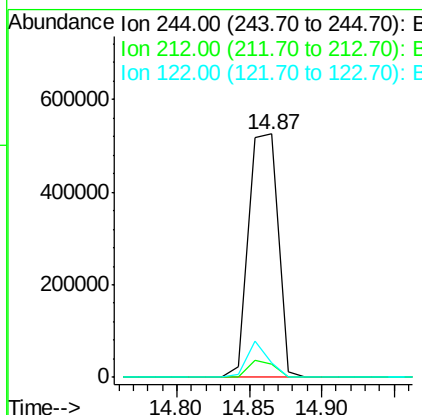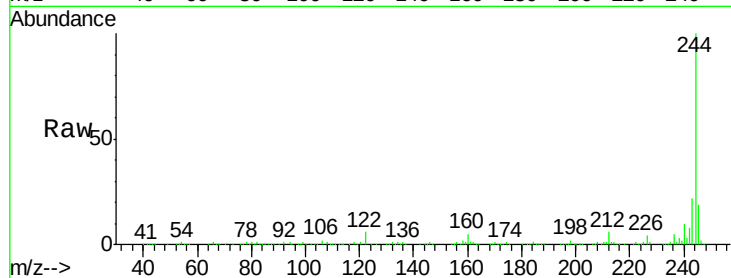

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.97 min Scan# 1495
 Delta R.T. -0.03 min
 Lab File: BF077468.D
 Acq: 26 Feb 2015 16:40

Tgt Ion:264 Resp: 275770
 Ion Ratio Lower Upper
 264 100
 260 23.5 19.3 28.9
 265 21.1 16.8 25.2

