


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022515\
 Data File : BG016034.D
 Acq On : 25 Feb 2015 10:36
 Operator : TP/IZ
 Sample : DFTPP06
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP06

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
 Title : SVOA CALIBRATION
 Last Update : Fri Feb 20 05:38:39 2015

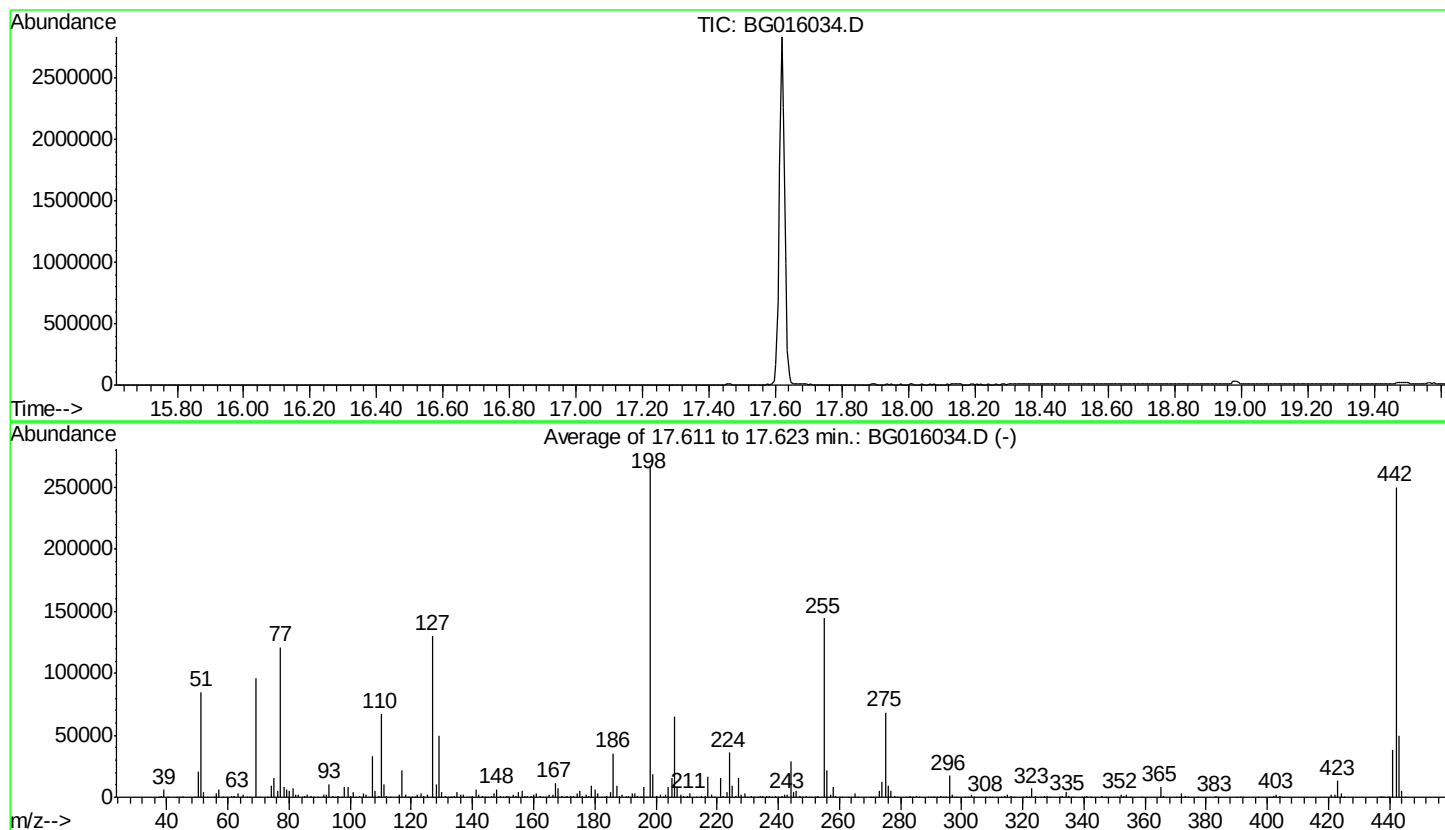

AutoFind: Scans 2540, 2541, 2542; Background Corrected with Scan 2534

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	85186	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	35.8	95865	PASS
70	69	0.00	2	0.4	361	PASS
127	198	10	80	48.7	130218	PASS
197	198	0.00	2	0.2	418	PASS
198	198	100	100	100.0	267541	PASS
199	198	5	9	7.1	18932	PASS
275	198	10	60	25.6	68610	PASS
365	198	1	100	3.2	8438	PASS
441	443	0.01	100	77.4	38749	PASS
442	198	50	100	93.6	250304	PASS
443	442	15	24	20.0	50069	PASS