
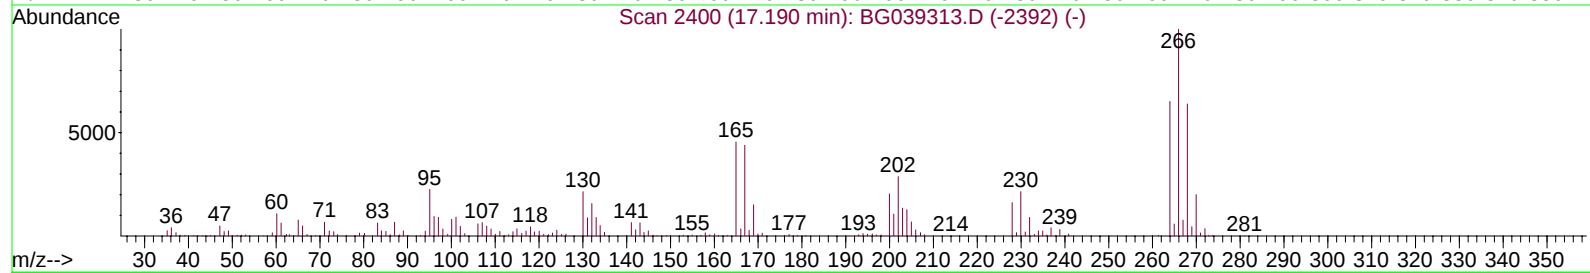
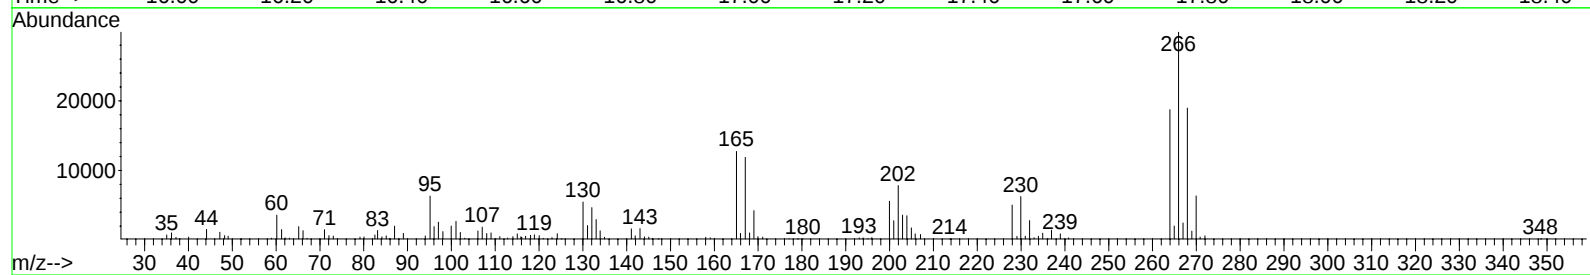


```
Data Path   : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022519\  
Data File   : BG039585.D  
Acq On      : 25 Feb 2019   13:20  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Feb 25 17:52:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

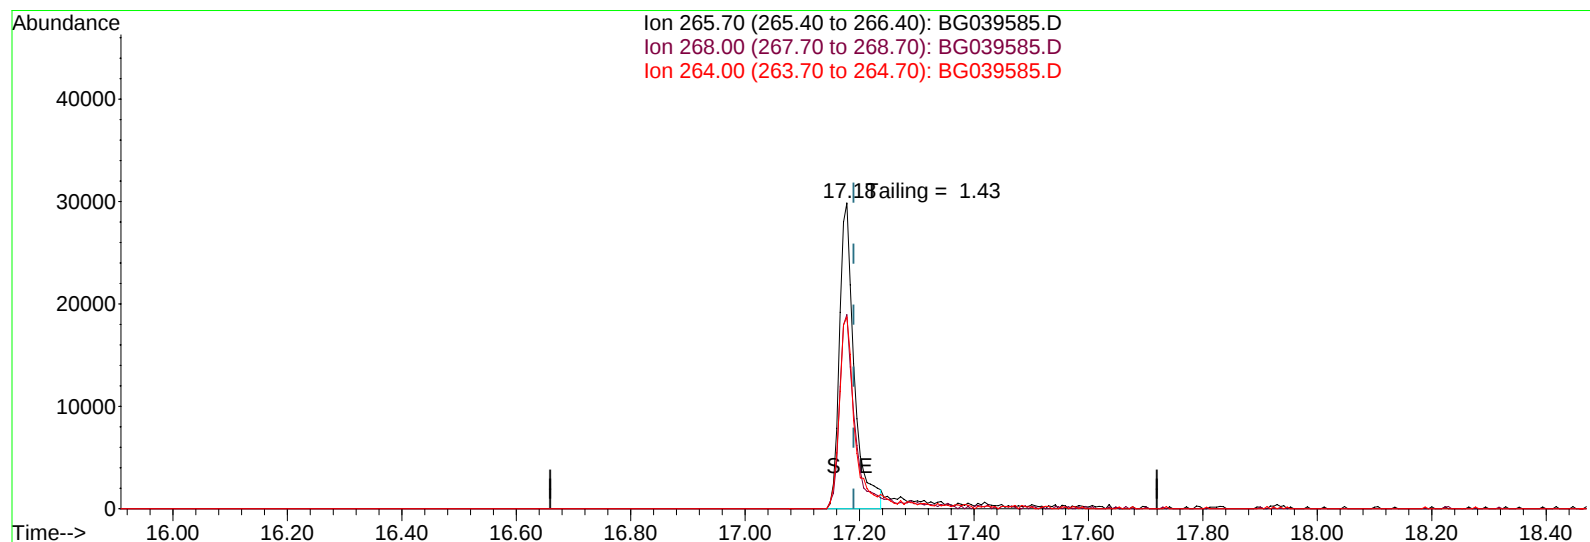

TIC: BG039585.D

(70) Pentachlorophenol (C)




17.178min (-0.012) 123798.15ng

response 55546

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.49
264.00	65.10	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG022519\
Data File : BG039585.D
Acq On : 25 Feb 2019 13:20
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 25 17:52:41 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

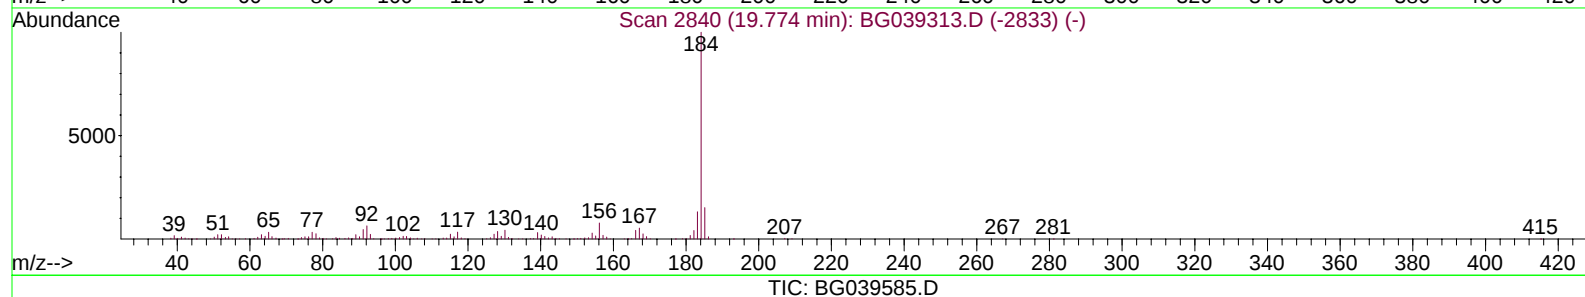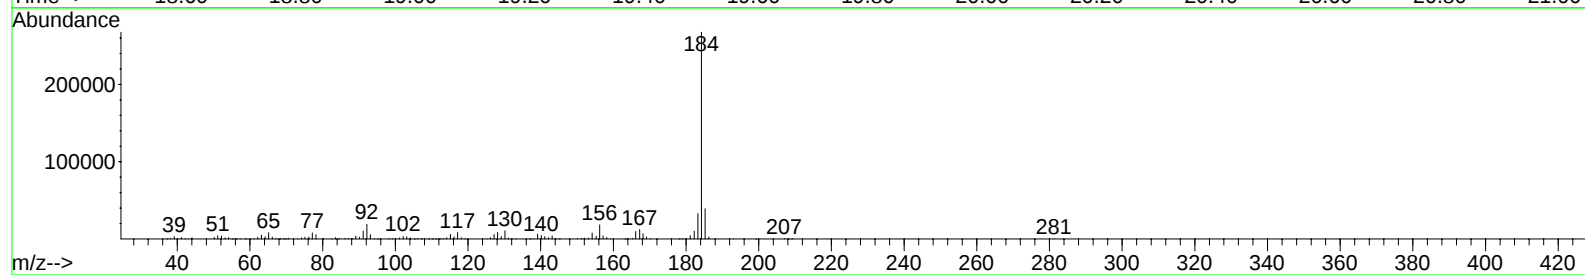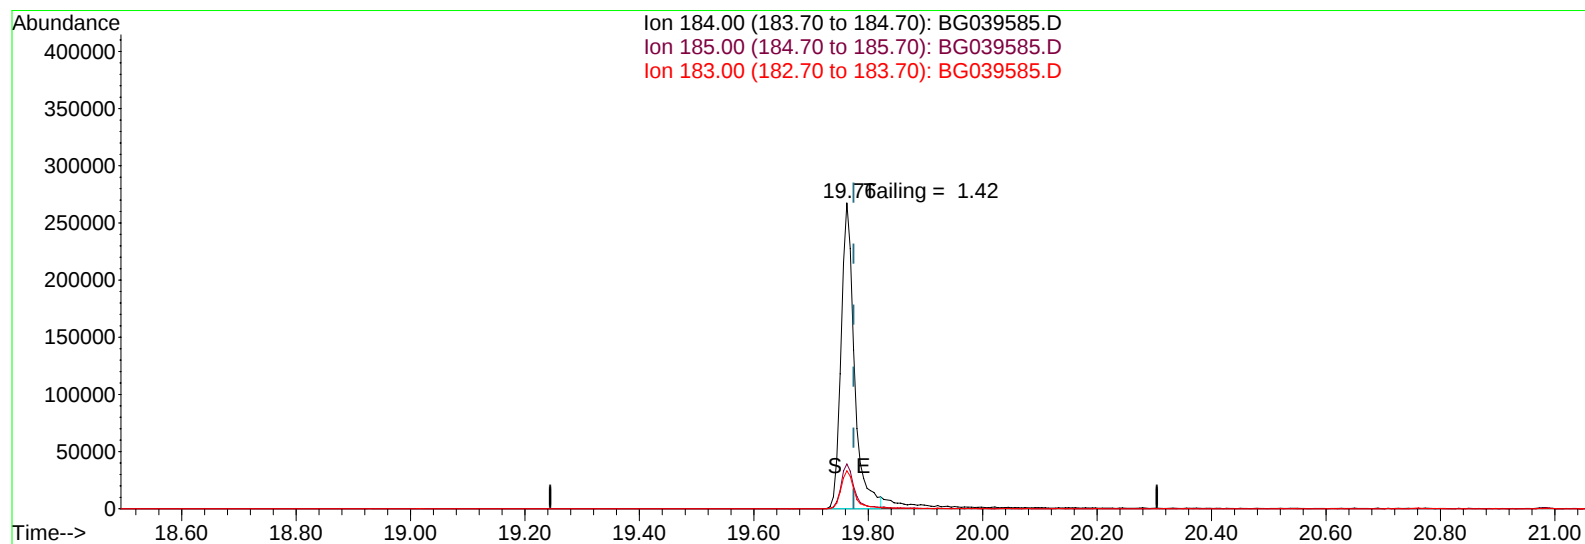

(77) Benzidine

19.763min (-0.012) 244734.71ng

response 457355

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.67
183.00	13.20	12.39
0.00	0.00	0.00