


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG022519\
 Data File : BG039585.D
 Acq On : 25 Feb 2019 13:20
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

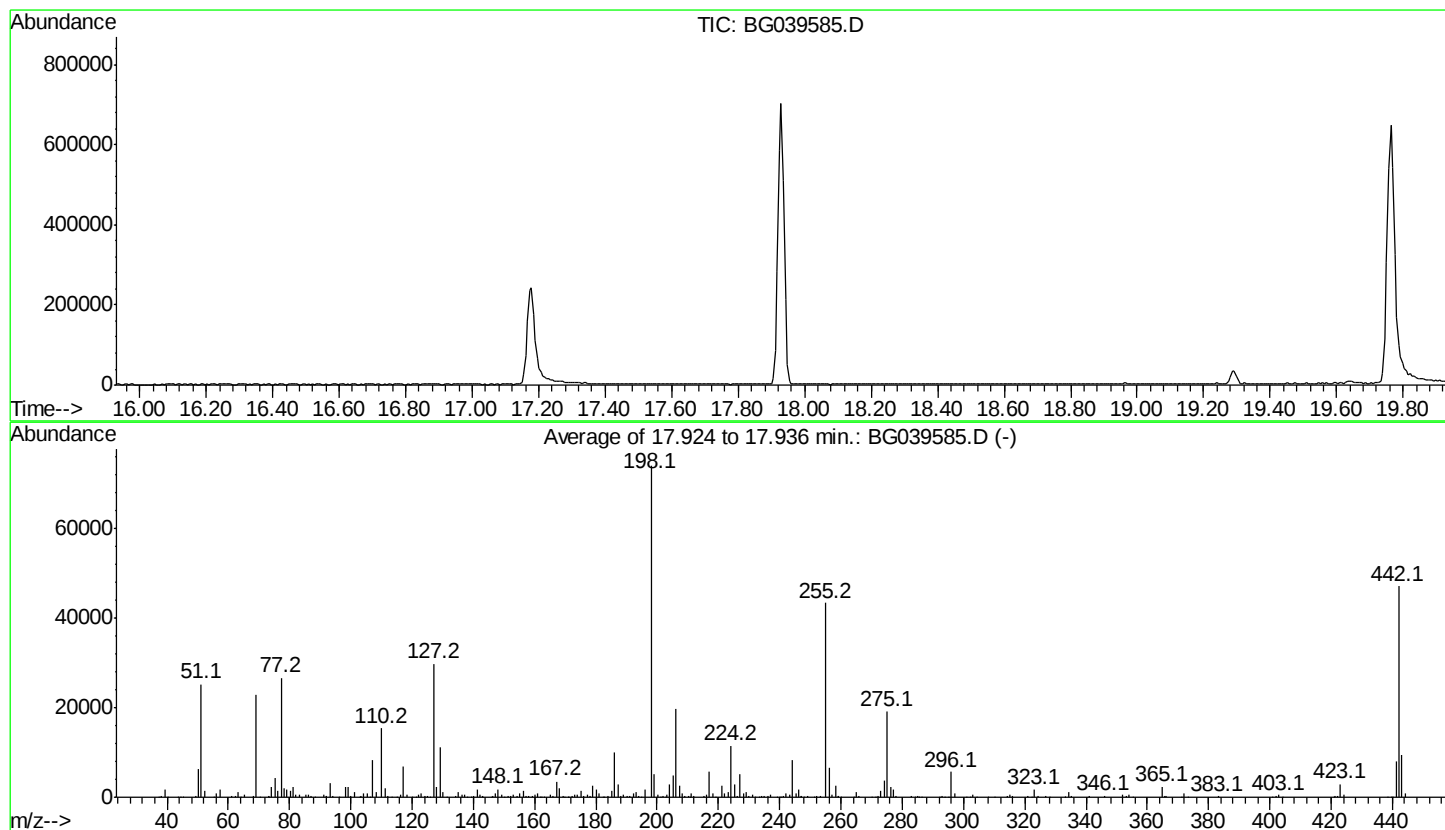

AutoFind: Scans 2525, 2526, 2527; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.1	25250	PASS
68	69	0.00	2	0.8	172	PASS
69	198	0.00	100	30.7	22786	PASS
70	69	0.00	2	0.6	142	PASS
127	198	10	80	40.3	29866	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	74128	PASS
199	198	5	9	7.1	5248	PASS
275	198	10	60	25.7	19048	PASS
365	198	1	100	3.1	2311	PASS
441	198	0.01	100	10.8	8025	PASS
442	198	50	100	63.6	47152	PASS
443	442	15	24	20.2	9518	PASS