
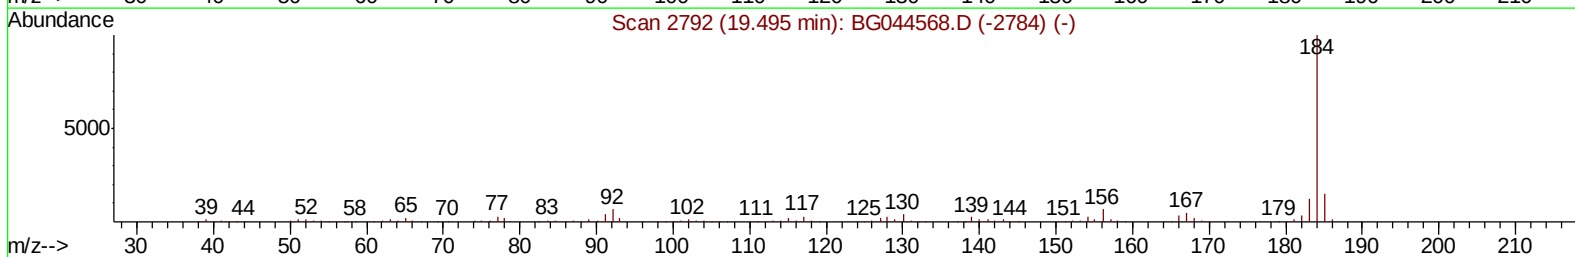
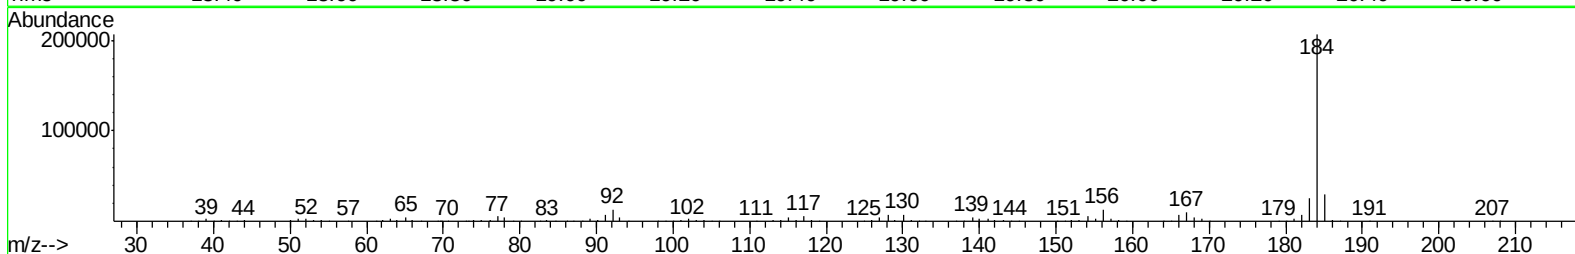


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
Data File : BG044574.D
Acq On : 25 Feb 2020 12:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 06:32:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

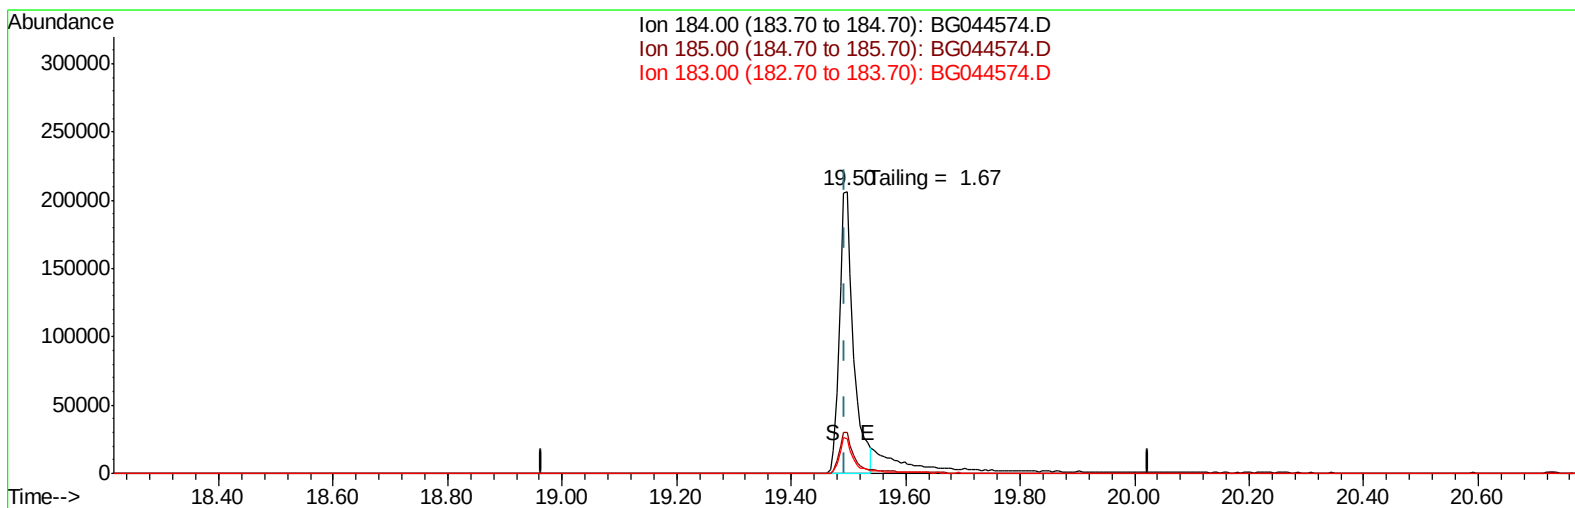

TIC: BG044574.D

(77) Benzidine




19.498min (+0.003) 0.00ng

response 422340

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.40
183.00	12.40	12.47
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
Data File : BG044574.D
Acq On : 25 Feb 2020 12:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 06:32:31 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

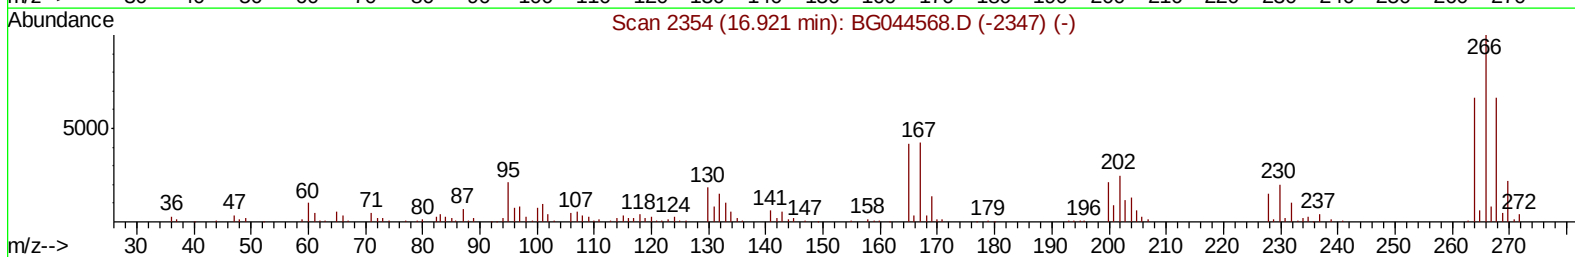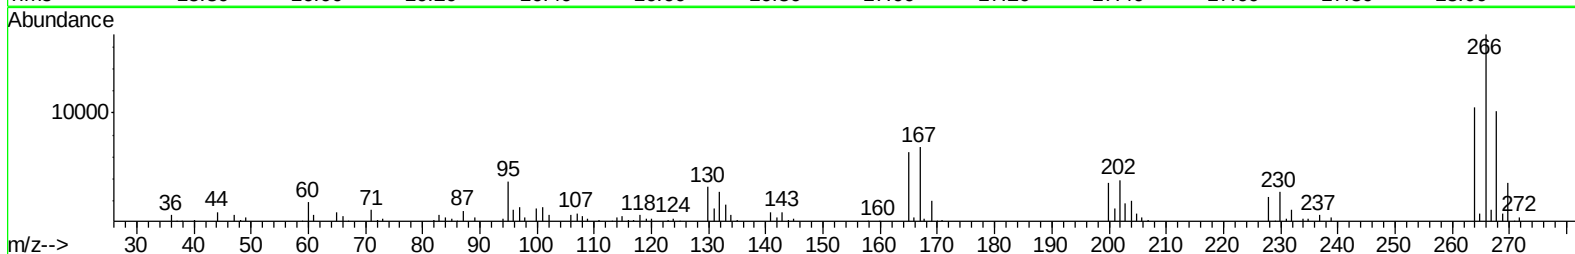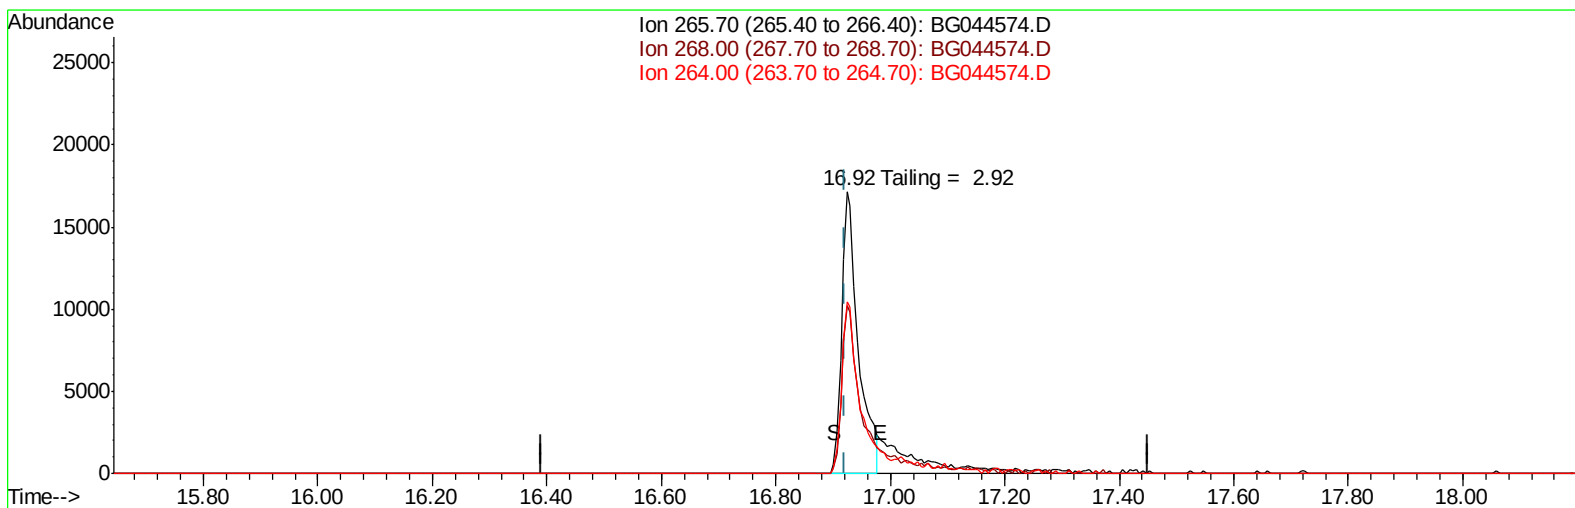

TIC: BG044574.D

(70) Pentachlorophenol (C)

16.924min (+0.003) 18852.40ng

response 41142

Ion	Exp%	Act%
265.70	100	100
268.00	66.70	59.58
264.00	66.20	61.01
0.00	0.00	0.00