
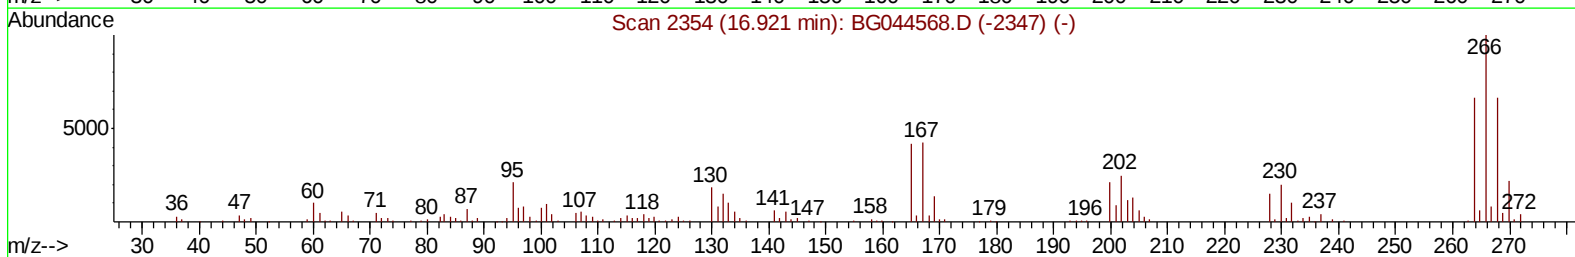
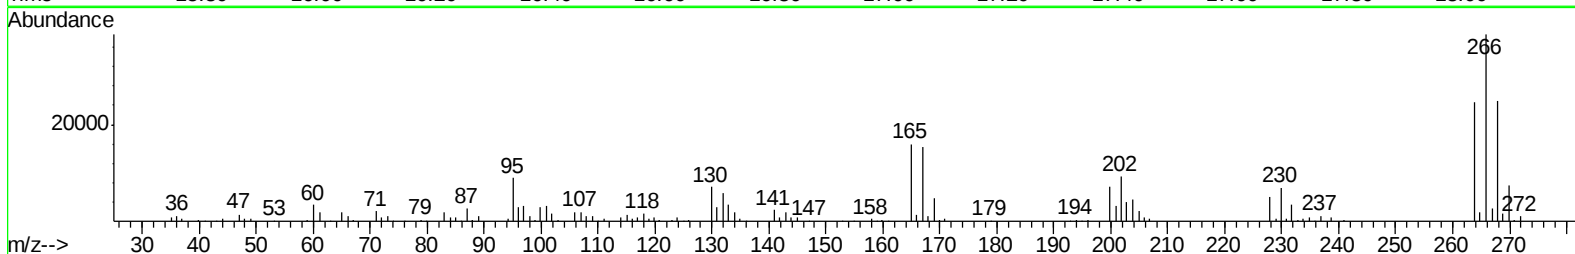


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
Data File : BG044579.D
Acq On : 25 Feb 2020 16:31
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 06:41:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 24 16:11:23 2020
Response via : Initial Calibration

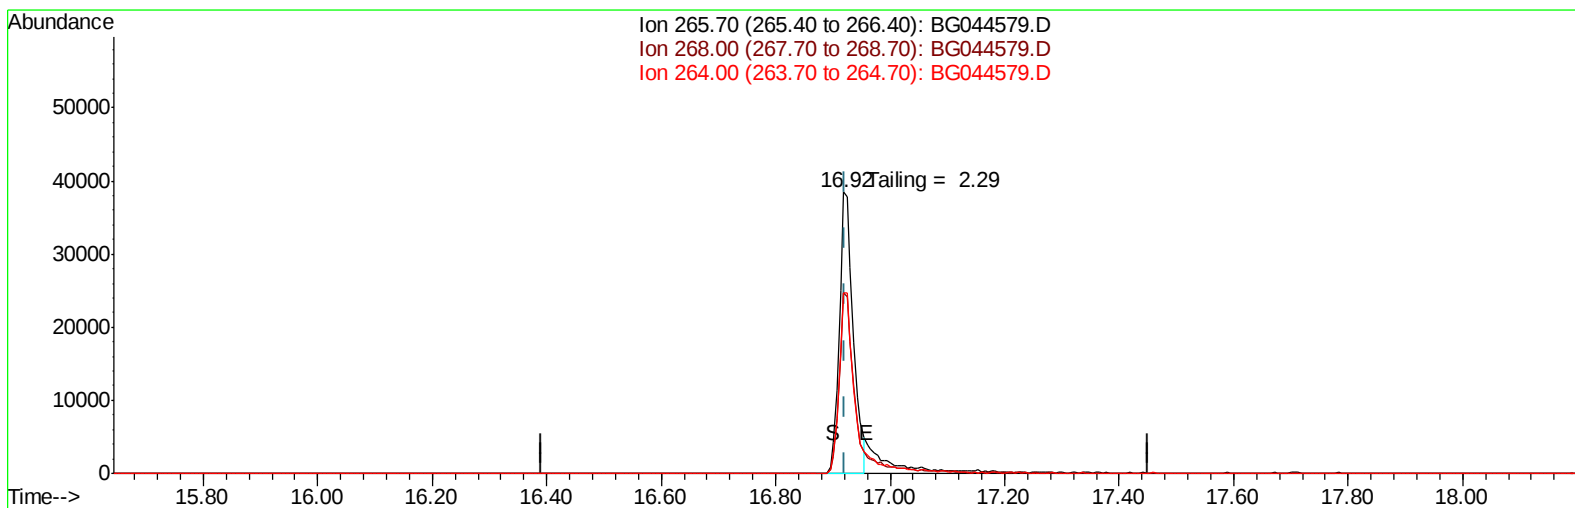

TIC: BG044579.D

(70) Pentachlorophenol (C)




16.919min (-0.002) 19739.22ng m

response 65586

Ion	Exp%	Act%
265.70	100	100
268.00	66.70	64.26
264.00	66.20	64.15
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
 Data File : BG044579.D
 Acq On : 25 Feb 2020 16:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 06:41:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 24 16:11:23 2020
 Response via : Initial Calibration

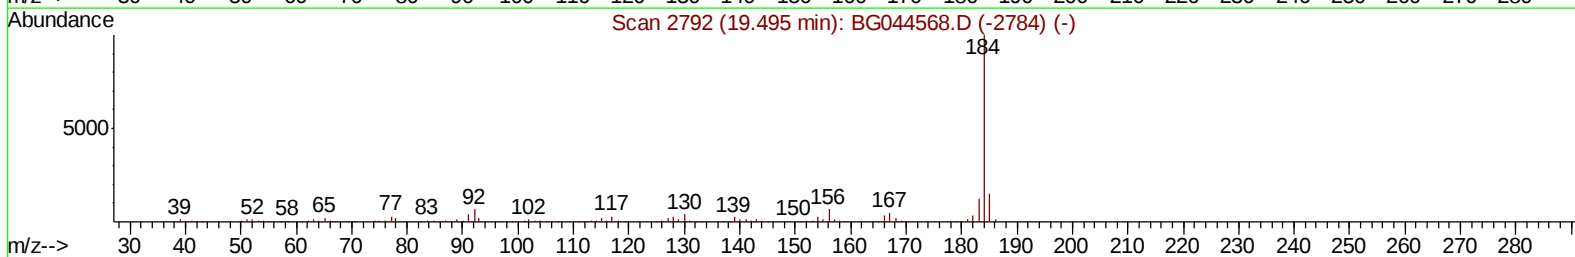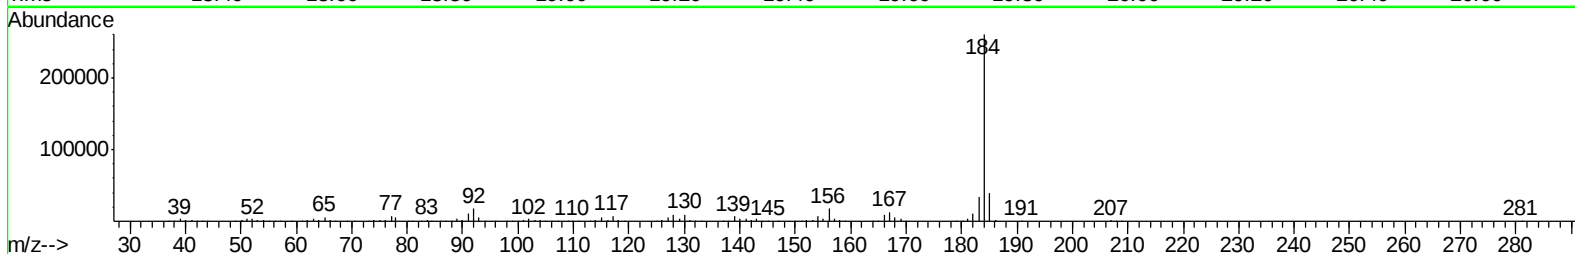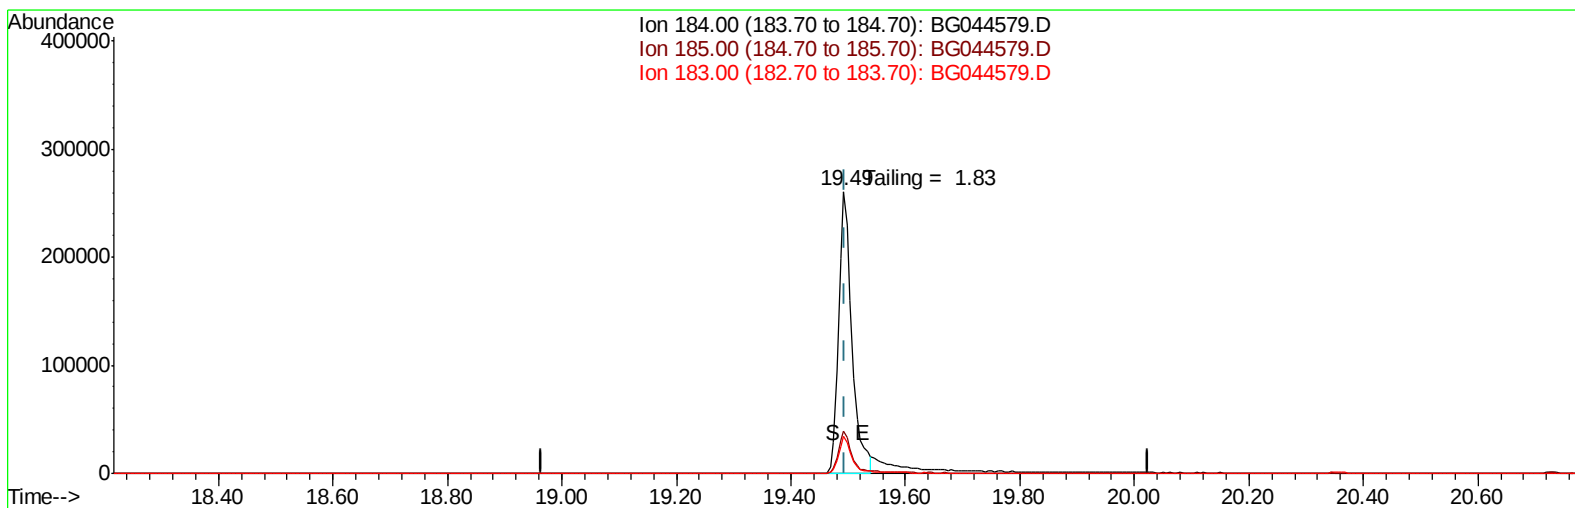

TIC: BG044579.D

(77) Benzidine

19.492min (-0.002) 0.00ng

response 471322

Ion	Exp%	Act%
184.00	100	100
185.00	15.30	14.81
183.00	12.40	12.99
0.00	0.00	0.00