

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
 Data File : BG044596.D
 Acq On : 26 Feb 2020 3:51
 Operator : CG/JU
 Sample : PB127049BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 PB127049BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.450	396	402	424	rBV	436335	736537	14.31%	3.745%
2	7.048	666	674	687	rBV	229963	431357	8.38%	2.193%
3	7.871	807	814	824	rBV	200342	342800	6.66%	1.743%
4	8.194	861	869	881	rBV	935339	1626475	31.61%	8.270%
5	9.029	1003	1011	1035	rBV	661305	1253964	24.37%	6.376%
6	10.674	1282	1291	1309	rBV	239392	467591	9.09%	2.378%
7	13.135	1703	1710	1730	rBV	1886497	3075004	59.76%	15.636%
8	14.516	1938	1945	1962	rBV	418441	683834	13.29%	3.477%
9	16.009	2191	2199	2224	rBV	1509457	2473706	48.07%	12.579%
10	17.260	2405	2412	2426	rBV	553173	893348	17.36%	4.543%
11	19.881	2851	2858	2877	rBV	3764586	5145644	100.00%	26.165%
12	21.502	3127	3134	3151	rBV	606109	1033952	20.09%	5.258%
13	22.284	3262	3267	3273	rBV	42190	66353	1.29%	0.337%
14	22.942	3374	3379	3389	rVB	54262	101678	1.98%	0.517%
15	23.711	3503	3510	3518	rVB2	51175	108234	2.10%	0.550%
16	24.563	3644	3655	3673	rBV2	367641	1159421	22.53%	5.896%
17	25.668	3837	3843	3854	rVB6	22525	66121	1.28%	0.336%


Sum of corrected areas: 19666019

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
Data File : BG044596.D
Acq On : 26 Feb 2020 3:51
Operator : CG/JU
Sample : PB127049BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
PB127049BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG022420.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

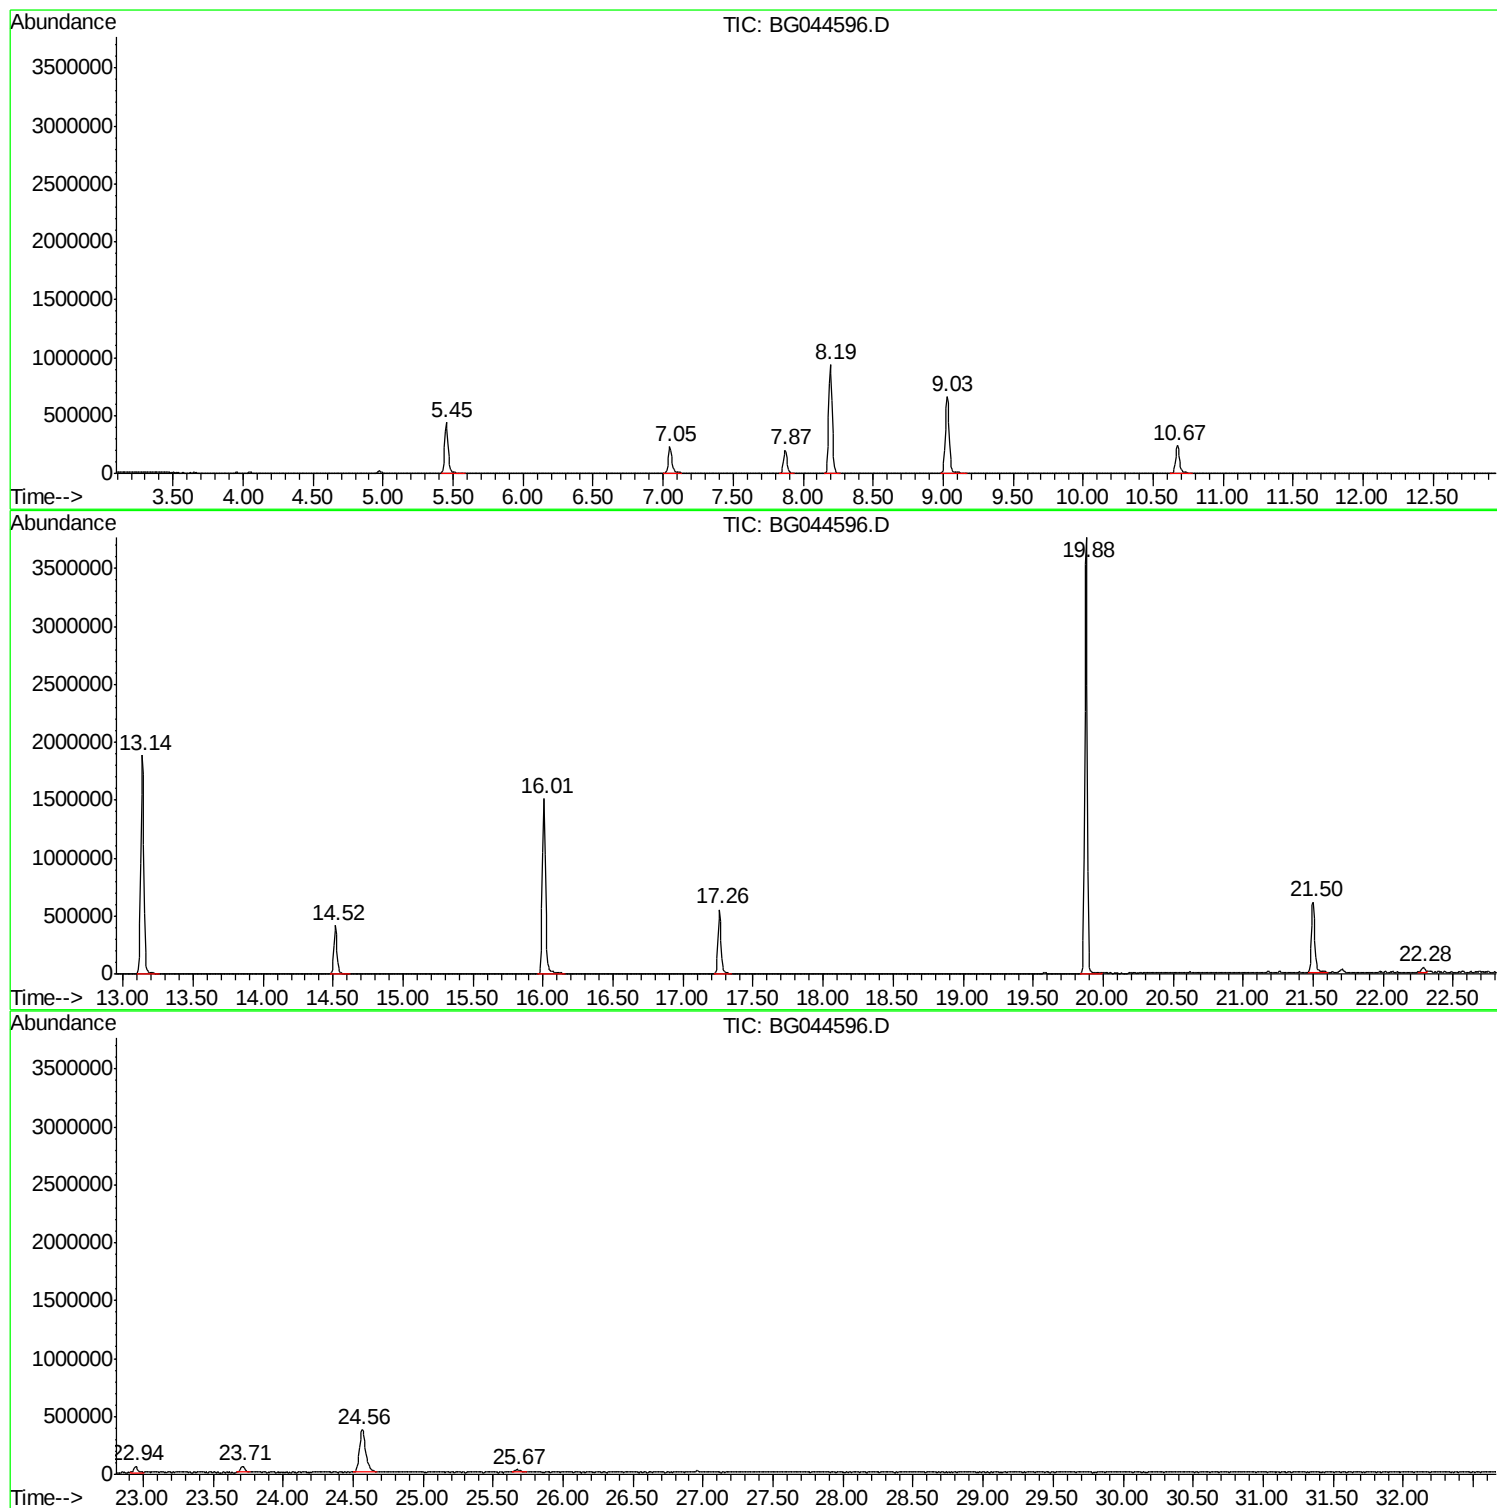

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022520\
Data_File : BG044596.D
Acq_On : 26_Feb_2020 3:511
Operator : CG/JUU
Sample : PB127049BLL
Misc :
ALS_Vial : 18 Sample_Multiplier: 11

Instrument :
BNA_G
ClientSampleId :
PB127049BL

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATIONN

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
