


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
 Data File : BG044574.D
 Acq On : 25 Feb 2020 12:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 24 16:11:23 2020

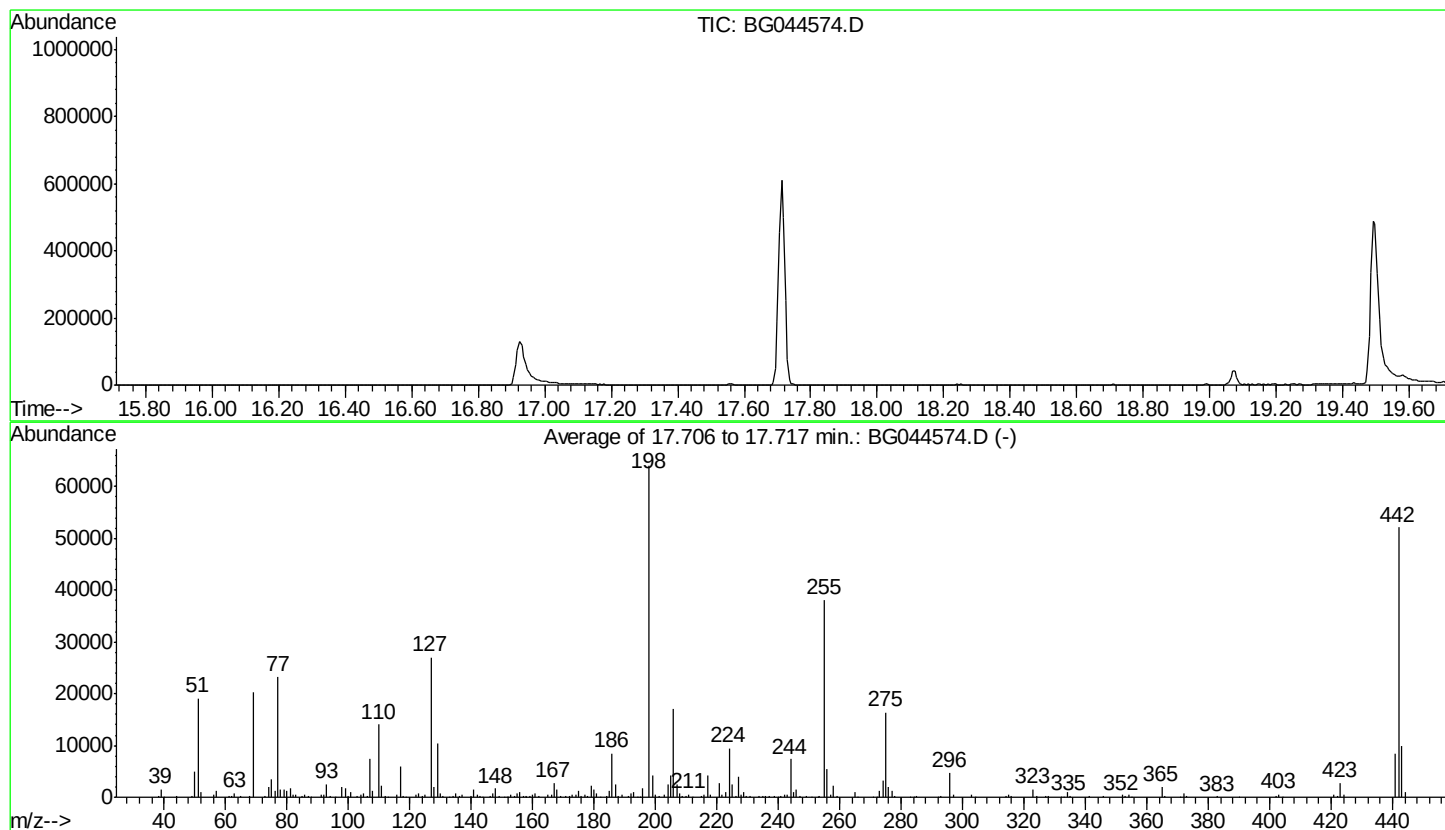

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	19115	PASS
68	69	0.00	2	1.4	281	PASS
69	198	0.00	100	31.7	20282	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.2	27058	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64053	PASS
199	198	5	9	6.6	4202	PASS
275	198	10	60	25.6	16414	PASS
365	198	1	100	3.3	2111	PASS
441	198	0.01	100	13.0	8298	PASS
442	198	50	100	81.4	52136	PASS
443	442	15	24	19.2	10003	PASS