


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022520\
 Data File : BG044579.D
 Acq On : 25 Feb 2020 16:31
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG022420.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 24 16:11:23 2020

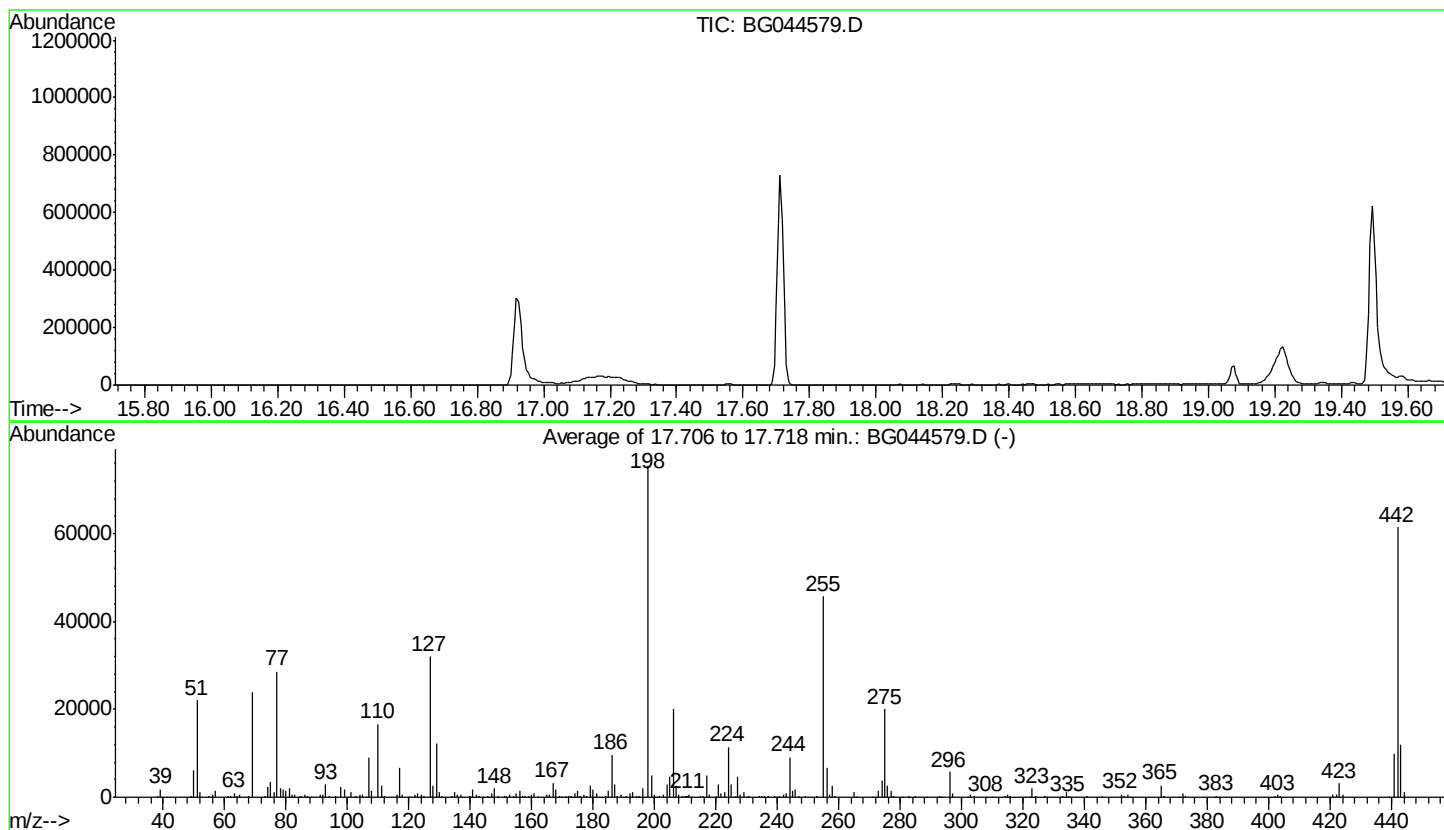

AutoFind: Scans 2488, 2489, 2490; Background Corrected with Scan 2481

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	22085	PASS
68	69	0.00	2	0.7	178	PASS
69	198	0.00	100	31.7	23928	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	42.4	31986	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	75432	PASS
199	198	5	9	6.7	5024	PASS
275	198	10	60	26.6	20053	PASS
365	198	1	100	3.5	2674	PASS
441	198	0.01	100	13.3	10039	PASS
442	198	50	100	81.3	61322	PASS
443	442	15	24	19.7	12069	PASS