


Data Path : Z:\HPCHEM1\BNA_G\Data\BG022615\
Data File : BG016045.D
Acq On : 26 Feb 2015 12:08
Operator : TP/IZ
Sample : DFTPP07
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP07

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM01.2-EPA-MA-BG021915.M
Title : SVOA CALIBRATION
Last Update : Fri Feb 20 05:38:39 2015

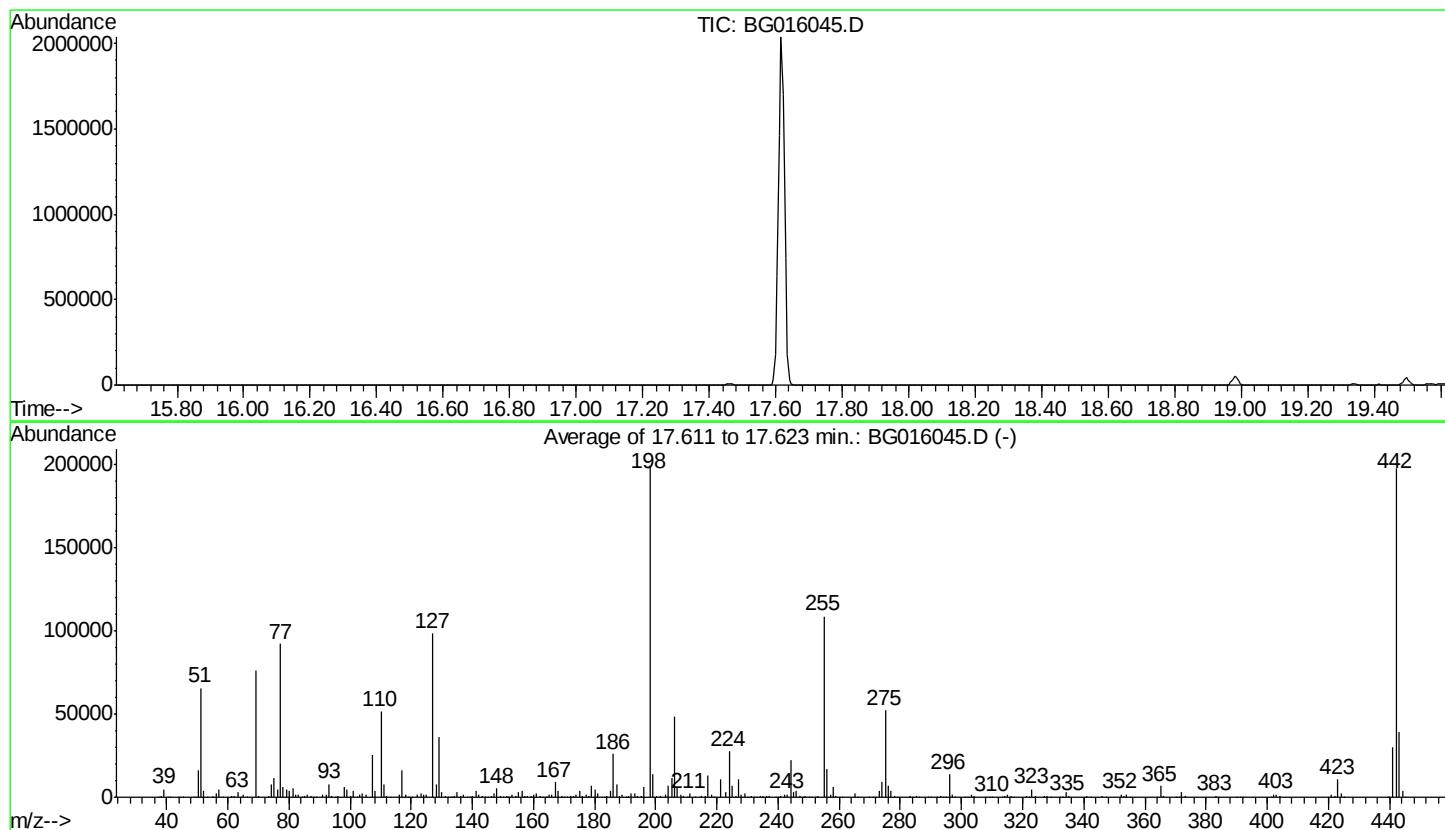

AutoFind: Scans 2540, 2541, 2542; Background Corrected with Scan 2534

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	65517	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	75858	PASS
70	69	0.00	2	0.6	476	PASS
127	198	10	80	49.3	98114	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	198890	PASS
199	198	5	9	7.0	13851	PASS
275	198	10	60	26.1	51877	PASS
365	198	1	100	3.4	6829	PASS
441	443	0.01	100	76.7	29824	PASS
442	198	50	100	99.4	197677	PASS
443	442	15	24	19.7	38893	PASS