

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
 Data File : BM004448.D
 Acq On : 27 Feb 2016 04:28
 Operator : SJ/UM
 Sample : H1564-22
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Feb 27 05:45:39 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 27 00:43:30 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.62	152	26730	20.00	ng/ul	0.00
18) Naphthalene-d8	10.40	136	110280	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	58356	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	122283	20.00	ng/ul	0.00
78) Chrysene-d12	21.24	240	135639	20.00	ng/ul	0.00
86) Perylene-d12	23.46	264	136010	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.07	96	3376	6.66	ng/uL	0.00
5) Phenol-d5	6.80	99	69776	31.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.95	67	37024	32.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.15	132	64737	33.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	58895	29.41	ng/ul	0.00
19) Nitrobenzene-d5	8.77	128	30678	36.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.49	143	34235	35.80	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	57019	32.98	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	80550	37.38	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	171669	34.30	ng/ul	0.00
47) Acenaphthylene-d8	13.97	160	217784	37.17	ng/ul	0.00
52) 4-Nitrophenol-d4	14.53	143	21872	27.19	ng/ul	0.00
58) Fluorene-d10	15.27	176	147739	34.71	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.43	200	15338	20.42	ng/ul	0.00
71) Anthracene-d10	17.13	188	222647	37.16	ng/ul	0.00
79) Pyrene-d10	19.44	212	245685	37.45	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.33	264	268745	37.65	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	13.73	163	58580	11.22	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM022616\
Data File : BM004448.D
Acq On : 27 Feb 2016 04:28
Operator : SJ/UM
Sample : H1564-22
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Feb 27 05:45:39 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM022216.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 27 00:43:30 2016
Response via : Initial Calibration

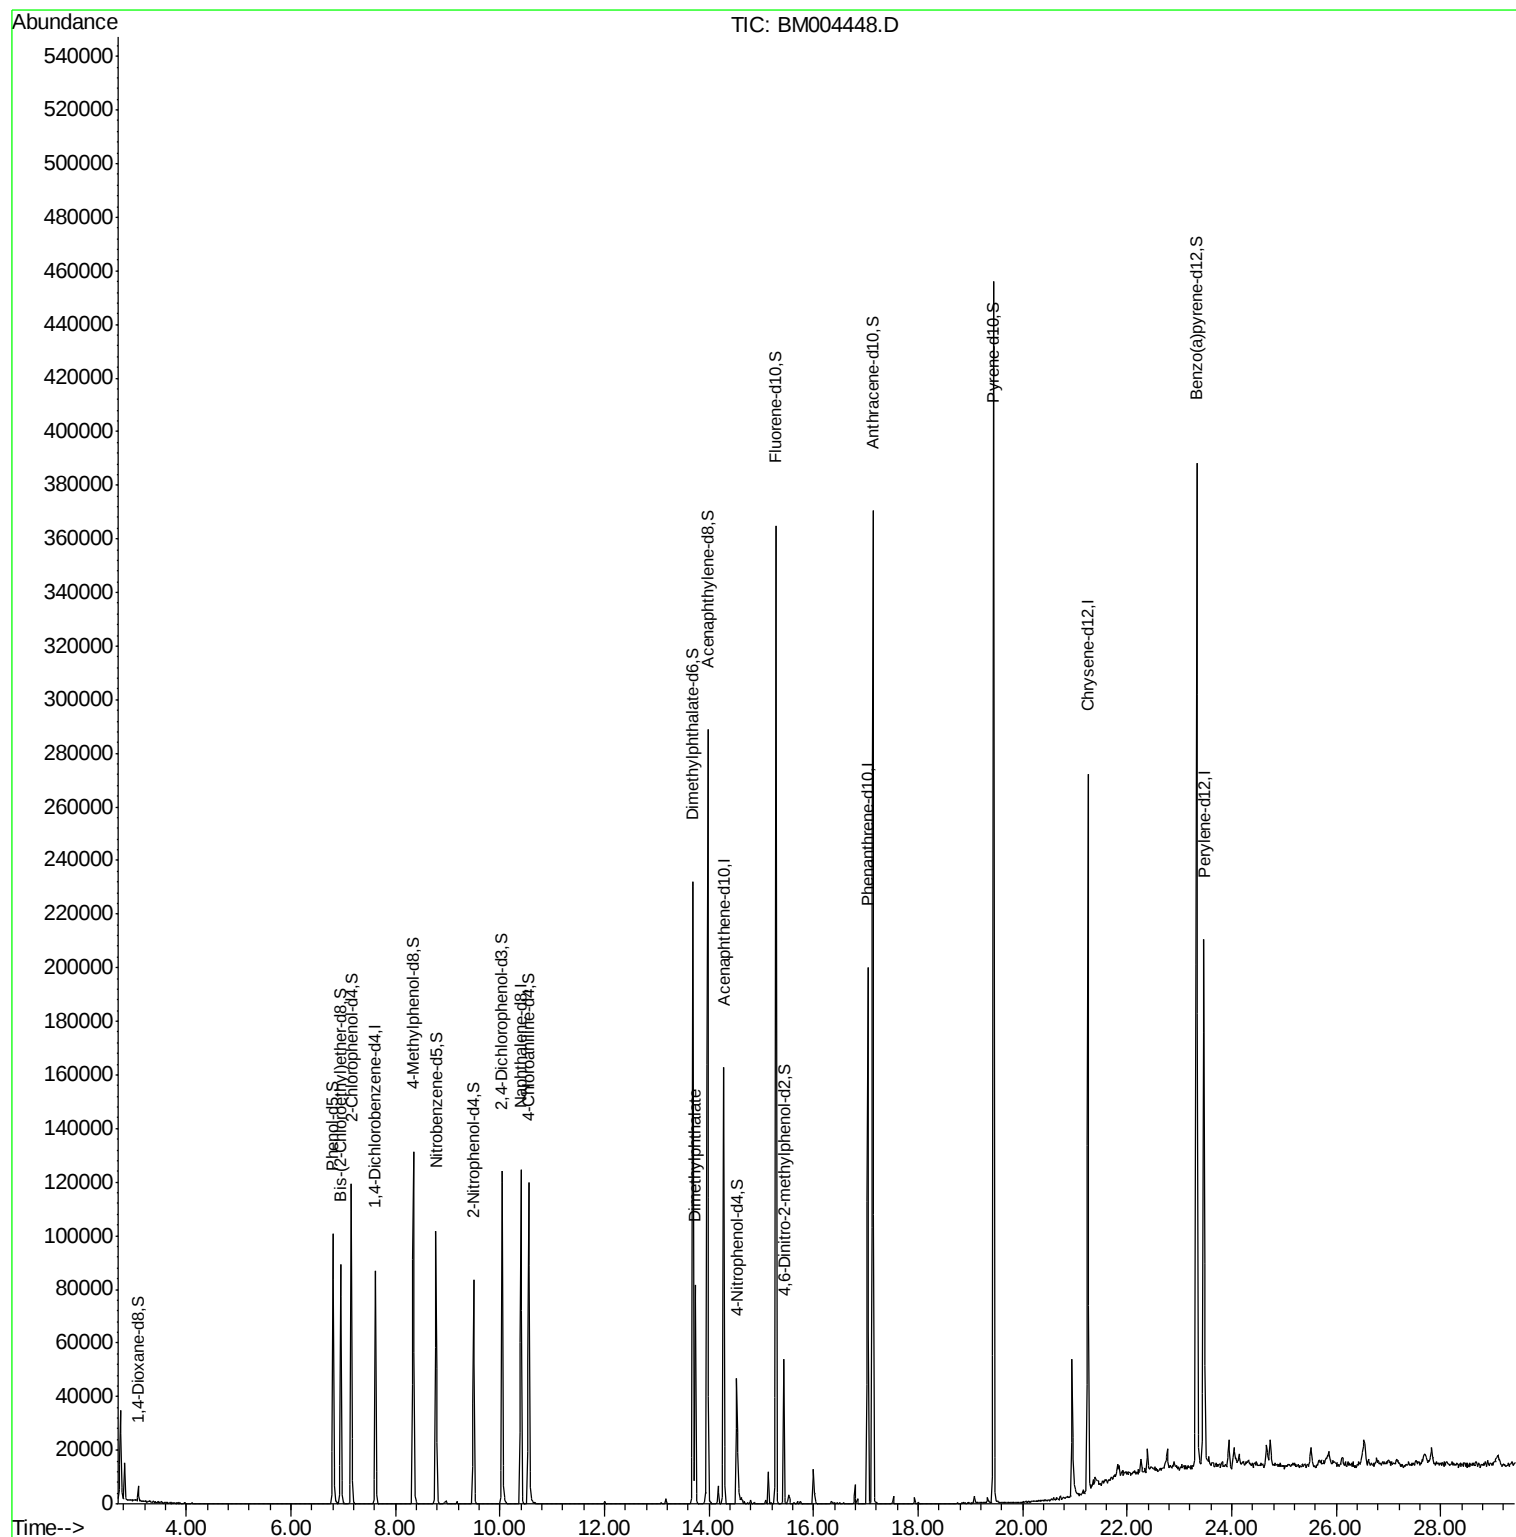

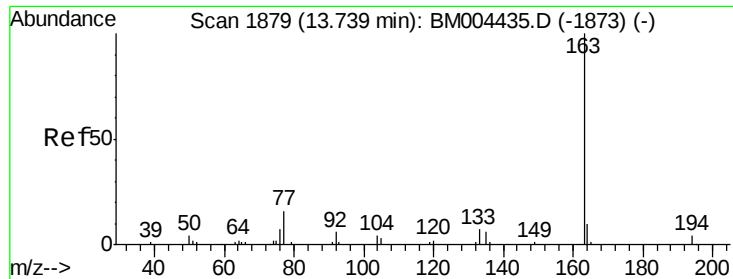

#45

Dimethylphthalate

Concen: 11.22 ng/ul

RT: 13.73 min Scan# 1878

Delta R.T. -0.01 min

Lab File: BM004448.D

Acq: 27 Feb 2016 04:28

Instrument :

BNA_G

ClientSampleId :

DFTPP


Tgt Ion:163 Resp: 58580

Ion Ratio Lower Upper

163 100

194 3.9 3.2 4.8

164 10.0 7.8 11.8

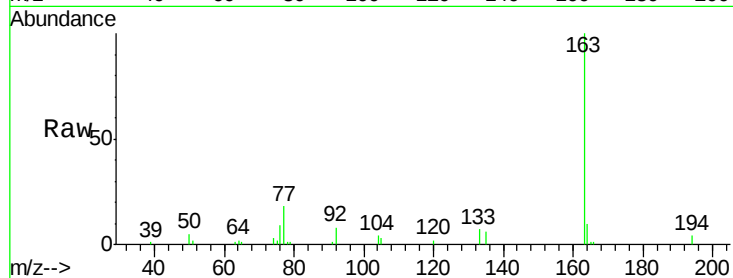

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

