
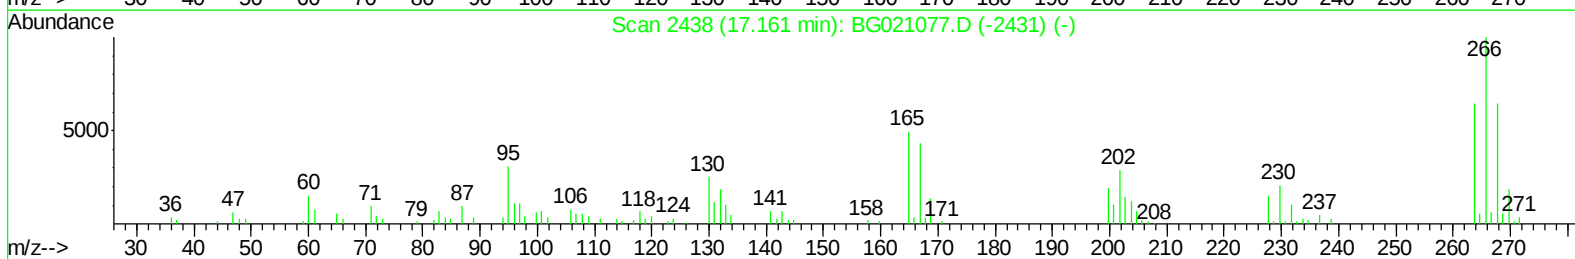
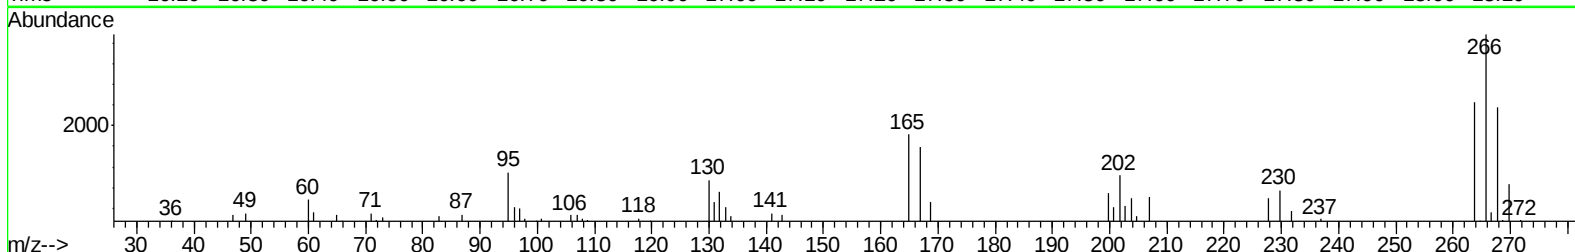


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022616\
Data File : BG021073.D
Acq On : 26 Feb 2016 10:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 17:42:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 16:39:44 2016
Response via : Initial Calibration

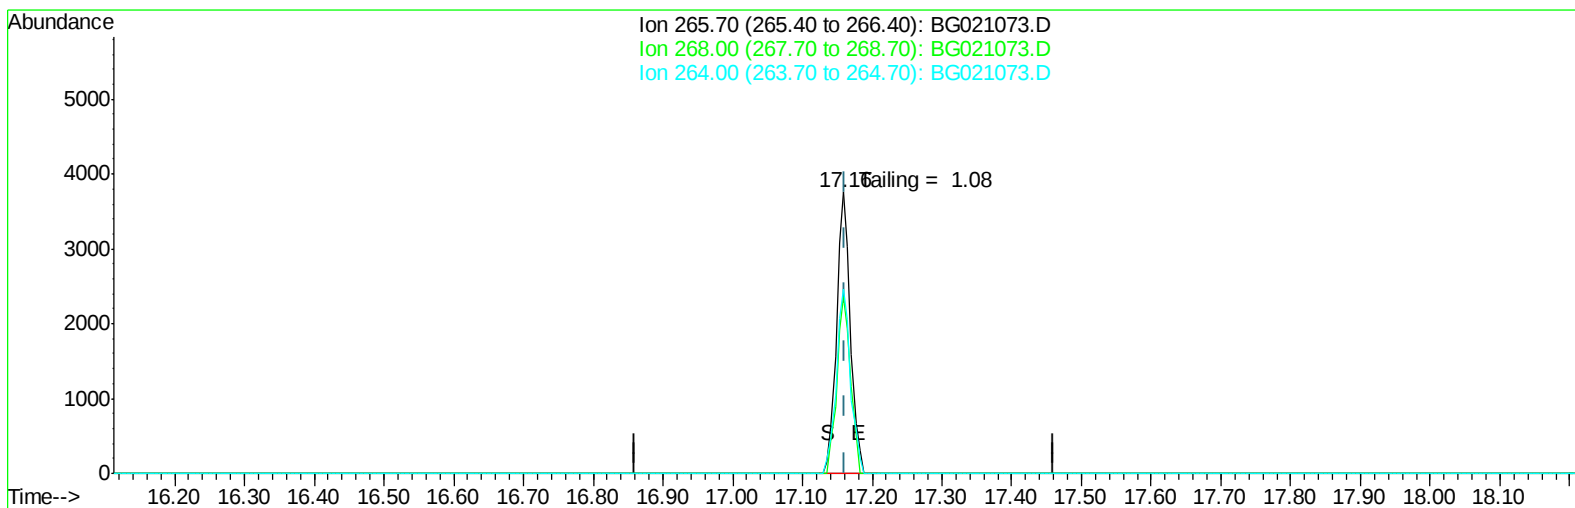

TIC: BG021073.D

(69) Pentachlorophenol (C)




17.159min (-0.003) 0.00ng

response 5200

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	67.63
264.00	59.80	69.39
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022616\
Data File : BG021073.D
Acq On : 26 Feb 2016 10:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 26 17:42:18 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 16:39:44 2016
Response via : Initial Calibration

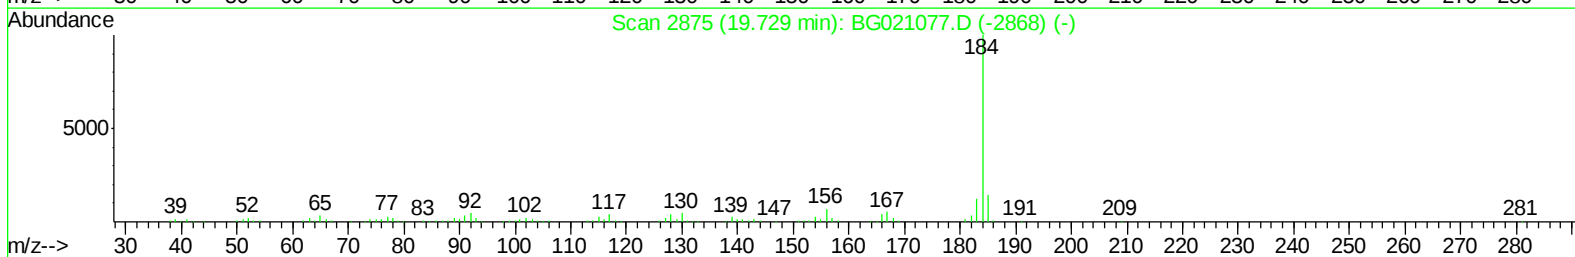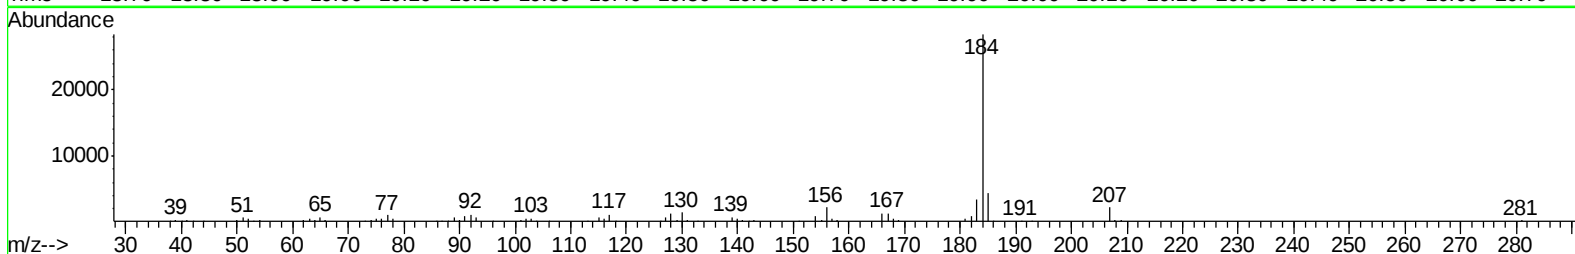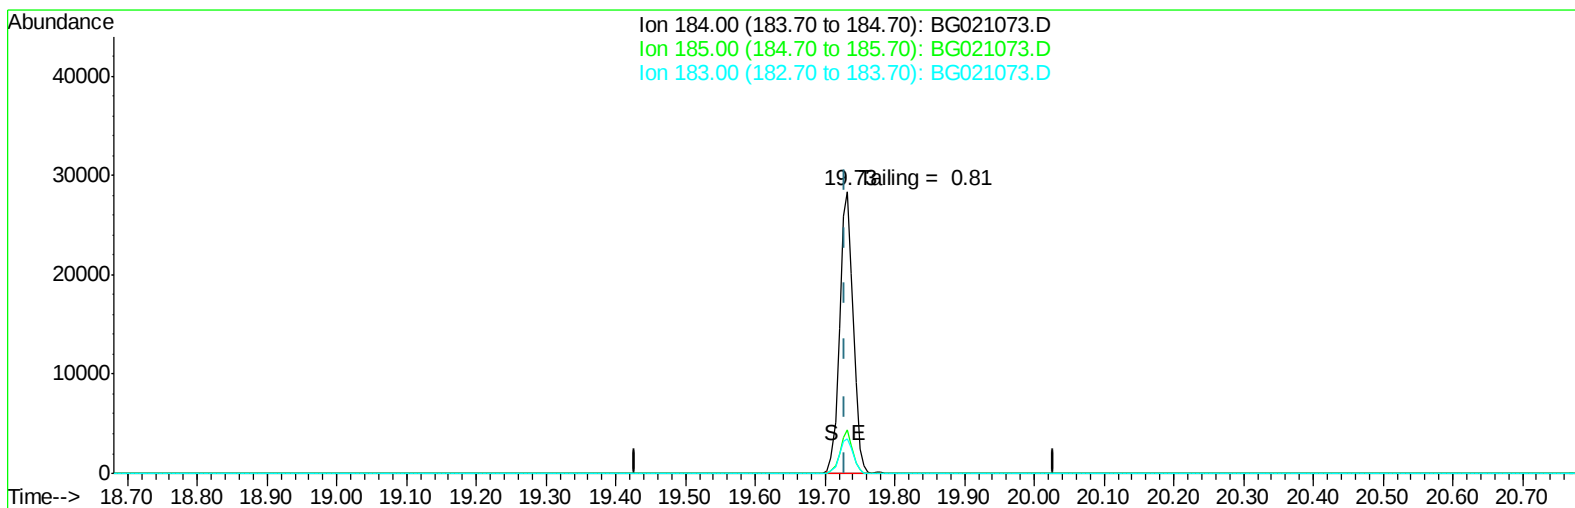

TIC: BG021073.D

(76) Benzidine

19.732min (+0.003) 0.00ng

response 38187

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	15.65
183.00	12.60	12.18
0.00	0.00	0.00