


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG022616\
Data File : BG021073.D
Acq On : 26 Feb 2016 10:47
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022616.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 26 16:39:44 2016

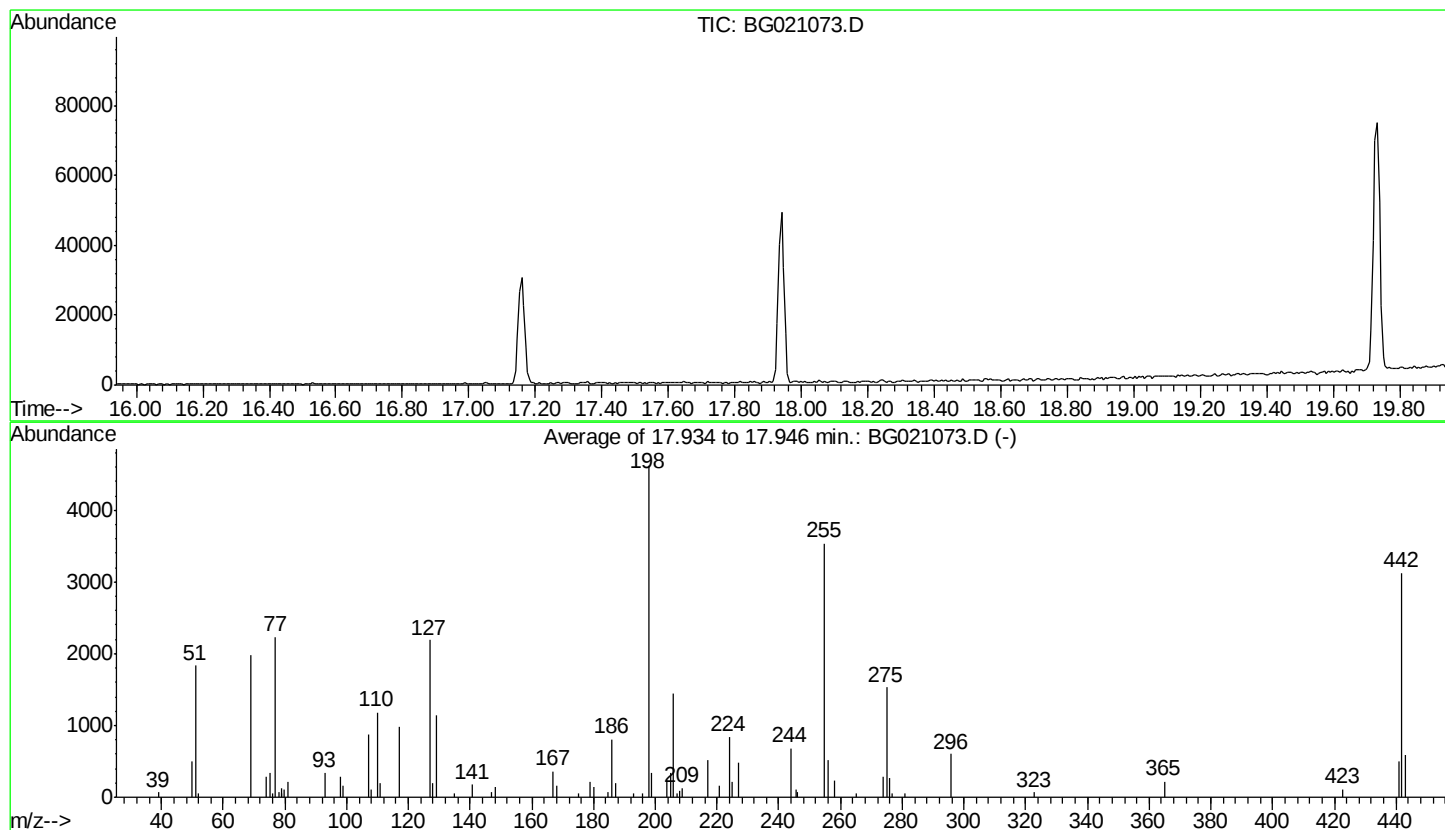

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	1835	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	42.9	1983	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.3	2186	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	4621	PASS
199	198	5	9	7.3	339	PASS
275	198	10	60	33.2	1533	PASS
365	198	1	100	4.8	220	PASS
441	442	0.01	24	16.0	500	PASS
442	198	50	100	67.6	3122	PASS
443	442	15	24	18.7	583	PASS