


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022616\  
 Data File : BG021082.D  
 Acq On : 26 Feb 2016 17:10  
 Operator : UM/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_G\METHODS\8270-BG022616.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Feb 26 16:39:44 2016

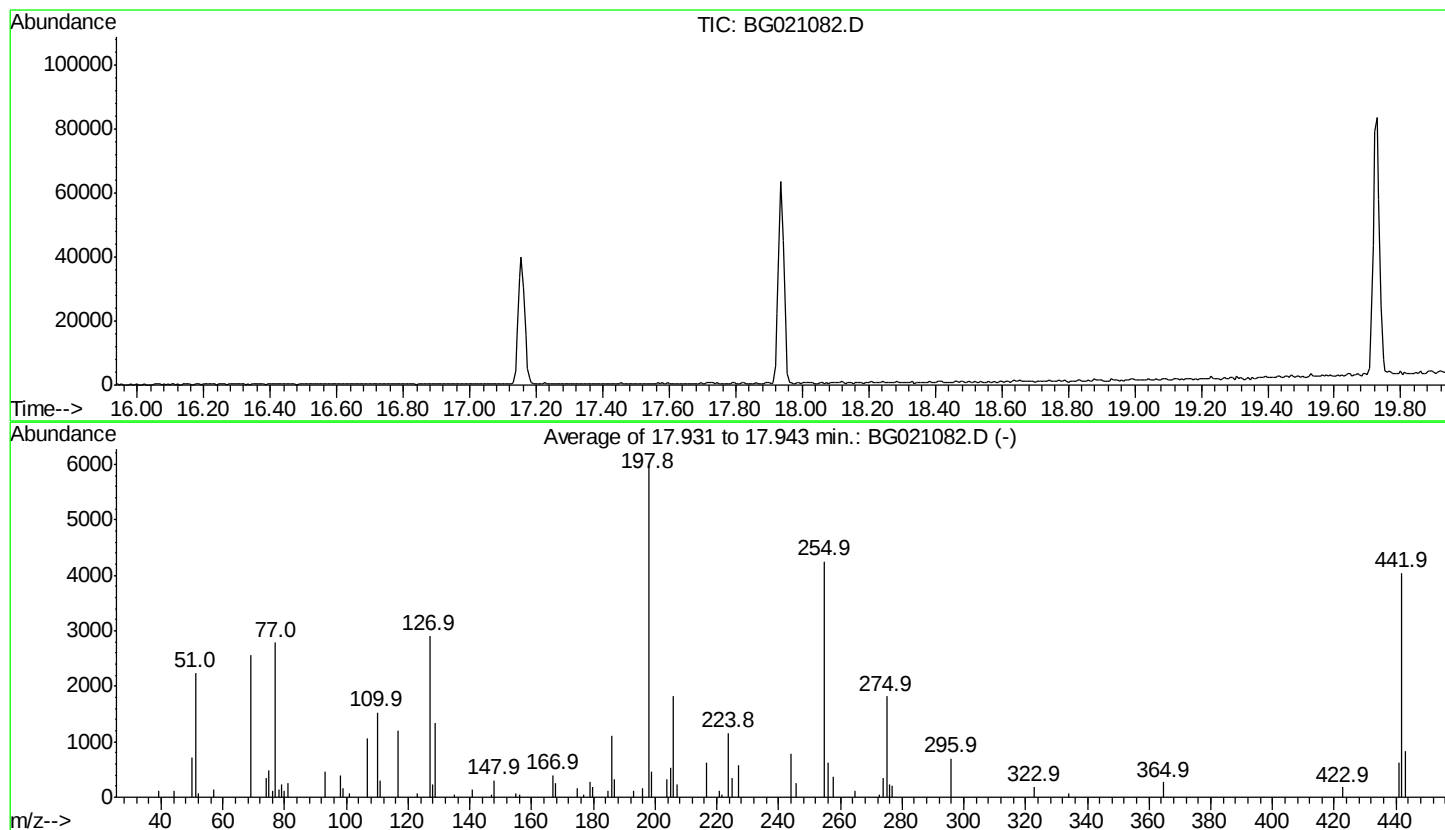

AutoFind: Scans 2569, 2570, 2571; Background Corrected with Scan 2563

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 37.5         | 2238       | PASS                |
| 68             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 69             | 198             | 0.00            | 100             | 42.7         | 2551       | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 48.7         | 2908       | PASS                |
| 197            | 198             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 5973       | PASS                |
| 199            | 198             | 5               | 9               | 7.6          | 451        | PASS                |
| 275            | 198             | 10              | 60              | 30.5         | 1820       | PASS                |
| 365            | 198             | 1               | 100             | 4.6          | 275        | PASS                |
| 441            | 442             | 0.01            | 24              | 15.7         | 634        | PASS                |
| 442            | 198             | 50              | 100             | 67.6         | 4037       | PASS                |
| 443            | 442             | 15              | 24              | 20.5         | 829        | PASS                |