

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022618\
 Data File : BG032817.D
 Acq On : 26 Feb 2018 11:35
 Operator : SJ/JU
 Sample : J1642-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Feb 26 17:35:00 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 26 17:33:40 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.92	152	82823	20.00	ng	0.00
21) Naphthalene-d8	11.81	136	353652	20.00	ng	0.00
38) Acenaphthene-d10	15.54	164	197110	20.00	ng	0.00
63) Phenanthrene-d10	18.26	188	440647	20.00	ng	0.00
75) Chrysene-d12	22.62	240	450317	20.00	ng	0.00
86) Perylene-d12	26.44	264	490127	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	6.33	112	301868	58.31	ng	0.00
7) Phenol-d6	8.01	99	233515	32.36	ng	0.00
23) Nitrobenzene-d5	10.12	82	582626	110.91	ng	0.00
41) 2,4,6-Tribromophenol	17.01	330	337883	163.03	ng	0.00
44) 2-Fluorobiphenyl	14.17	172	1286924	94.16	ng	0.00
78) Terphenyl-d14	20.79	244	1837320	91.67	ng	0.00
Target Compounds						
19) n-Nitroso-di-n-propylamine	10.12	70	76090	14.936	ng	# 81
24) Nitrobenzene	10.12	77	1686	6.640	ng	# 38
47) 2-Nitroaniline	14.18	65	2252	10.388	ng	# 1
50) 2,6-Dinitrotoluene	15.54	165	25654	16.442	ng	# 21
56) 2,4-Dinitrotoluene	15.54	165	25654	14.640	ng	# 19
64) 4,6-Dinitro-2-methylphenol	17.00	198	1126	6.032	ng	# 1
66) 4-Bromophenyl-phenylether	17.01	248	24570	5.273	ng	# 1
76) Benzidine	20.79	184	32009	2.085	ng	# 95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG022618\
Data File : BG032817.D
Acq On : 26 Feb 2018 11:35
Operator : SJ/JU
Sample : J1642-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Feb 26 17:35:00 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:33:40 2018
Response via : Initial Calibration

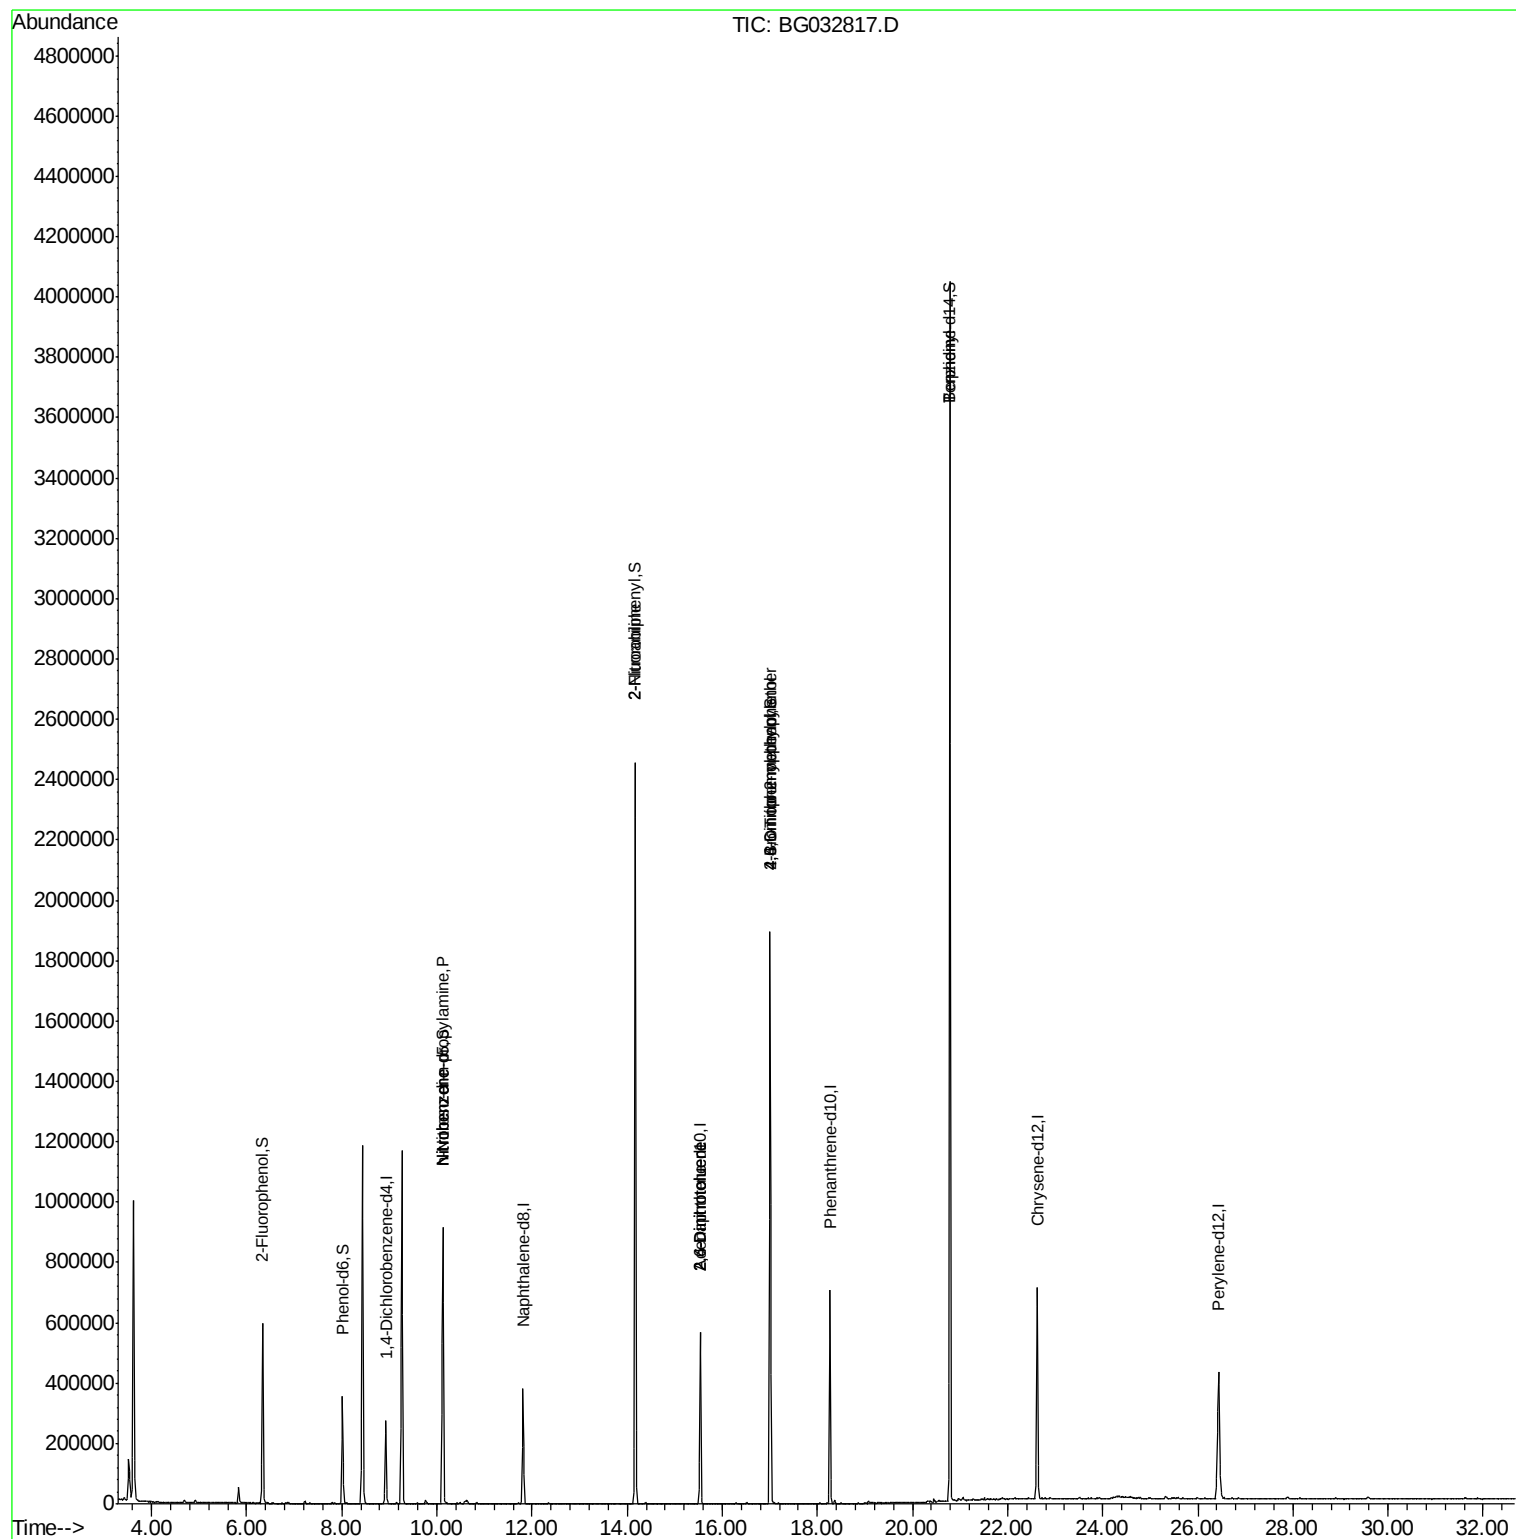




#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.92 min Scan# 959
Delta R.T. -0.00 min
Lab File: BG032817.D
Acq: 26 Feb 2018 11:35

Instrument :
BNA_G
ClientSampled :

Tot Ion:152 Resp: 82823
Ion Ratio Lower Upper
152 100
150 157.1 126.6 189.8
115 57.6 53.0 79.4

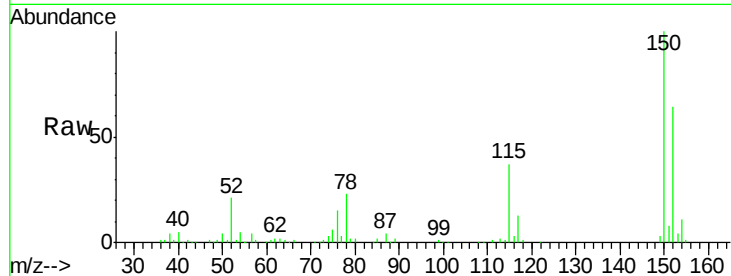


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

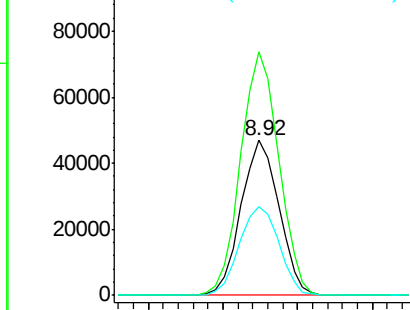



#5

2-Fluorophenol
Concen: 58.310 ng
RT: 6.33 min Scan# 518
Delta R.T. -0.00 min
Lab File: BG032817.D
Acq: 26 Feb 2018 11:35

Tgt Ion:112 Resp: 301868
Ion Ratio Lower Upper
112 100
64 61.1 56.3 84.5
63 30.7 30.1 45.1



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BGO
Ion 63.00 (62.70 to 63.70): BGO

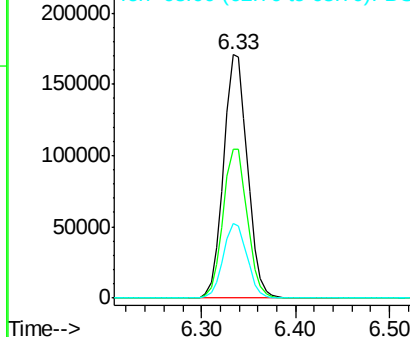



#7

Phenol-d6

Concen: 32.361 ng

RT: 8.01 min Scan# 804

Delta R.T. -0.00 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35

Instrument :

BNA_G

ClientSampleId :


Tot Ion: 99 Resp: 233515

Ion Ratio Lower Upper




99 100

42 18.5 14.1 21.1

71 29.9 26.1 39.1



Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

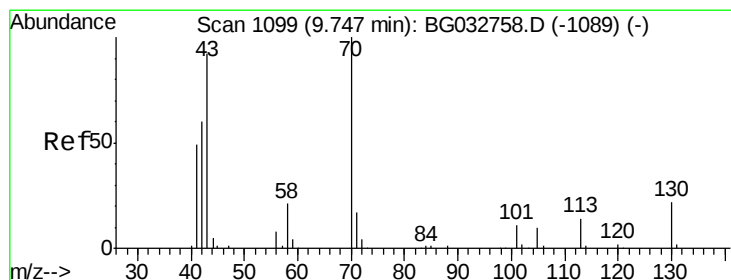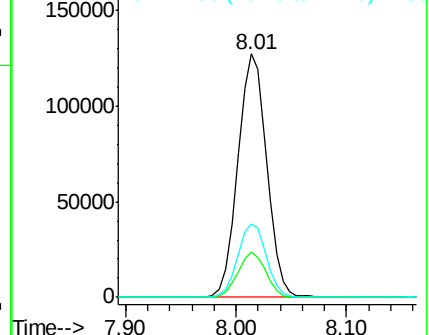

#19

n-Nitroso-di-n-propylamine

Concen: 14.936 ng

RT: 10.12 min Scan# 1163

Delta R.T. 0.39 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35

Tgt Ion: 70 Resp: 76090


Ion Ratio Lower Upper

70 100



42 51.3 49.1 73.7

101 0.0 8.5 12.7#

130 2.0 13.4 20.0#

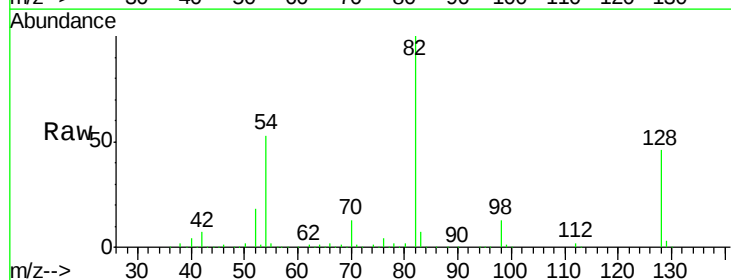

Abundance Ion 70.00 (69.70 to 70.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 101.00 (100.70 to 101.70): BGC
Ion 130.00 (129.70 to 130.70): BGC

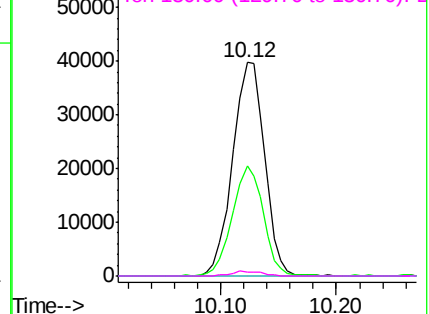







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 11.81 min Scan# 1451
Delta R.T. 0.00 min
Lab File: BG032817.D
Acq: 26 Feb 2018 11:35

Instrument :
BNA_G
ClientSampleId :

Tot Ion:136	Resp:	353652
Ion Ratio	Lower	Upper
136	100	
137	10.9	9.2 13.8
54	9.1	10.3 15.5#
68	6.5	4.5 6.7

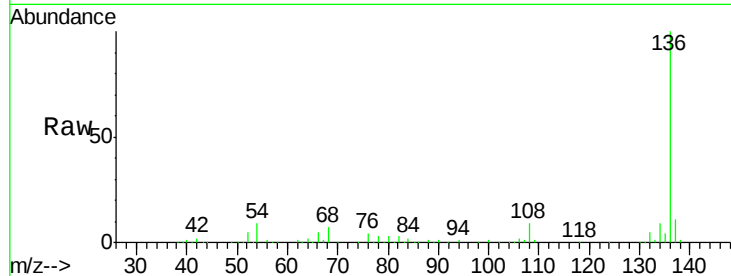


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC

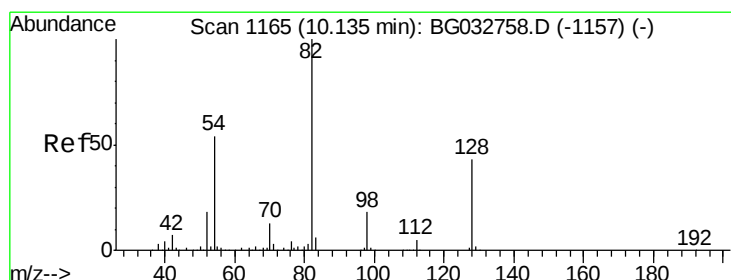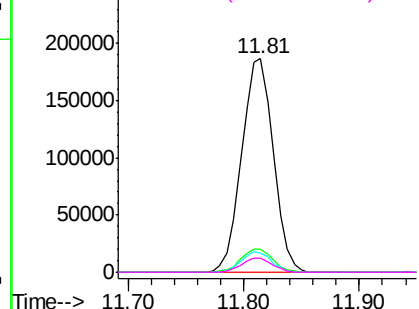



#23
Nitrobenzene-d5
Concen: 110.906 ng
RT: 10.12 min Scan# 1163
Delta R.T. -0.00 min
Lab File: BG032817.D
Acq: 26 Feb 2018 11:35

Tgt Ion: 82	Resp:	582626
Ion Ratio	Lower	Upper
82	100	
128	45.8	29.7 44.5#
54	53.3	43.1 64.7



Abundance Ion 82.00 (81.70 to 82.70): BGC
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BGC

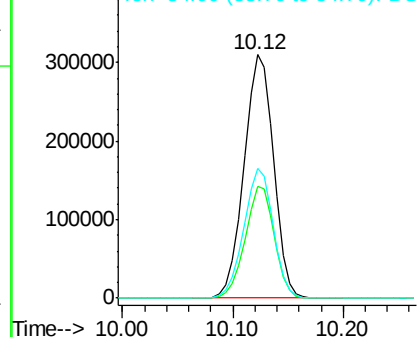



#24

Nitrobenzene

Concen: 6.640 ng

RT: 10.12 min Scan# 1163

Delta R.T. -0.04 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35

Instrument :

BNA_G

ClientSampled :


Tot Ion: 77 Resp: 1686

Ion Ratio Lower Upper




77 100

123 0.0 33.0 49.6#

65 38.2 13.0 19.6#

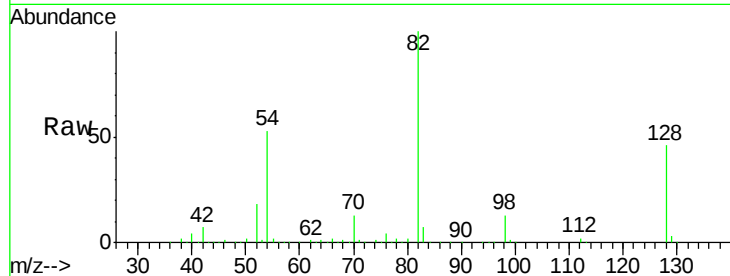

Abundance Ion 77.00 (76.70 to 77.70): BGC
Ion 123.00 (122.70 to 123.70): BGC
Ion 65.00 (64.70 to 65.70): BGC

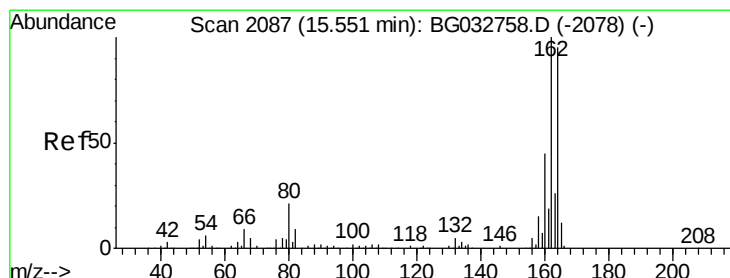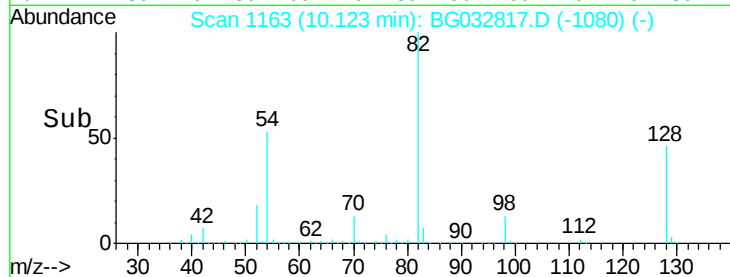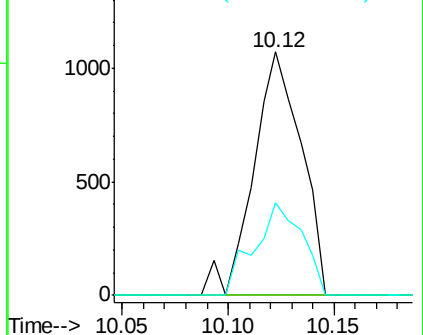

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 15.54 min Scan# 2085

Delta R.T. -0.00 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35


Tgt Ion:164 Resp: 197110

Ion Ratio Lower Upper



164 100


162 105.3 78.8 118.2

160 46.5 35.4 53.0

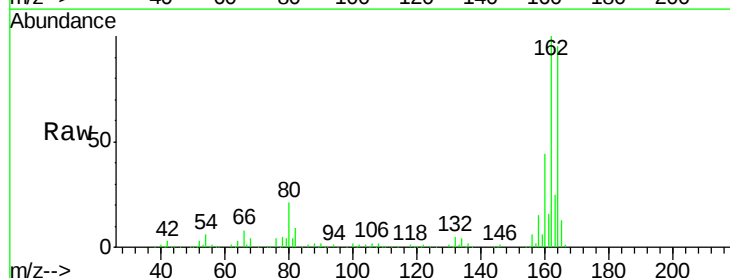

Abundance Ion 164.00 (163.70 to 164.70): BGC
Ion 162.00 (161.70 to 162.70): BGC
Ion 160.00 (159.70 to 160.70): BGC

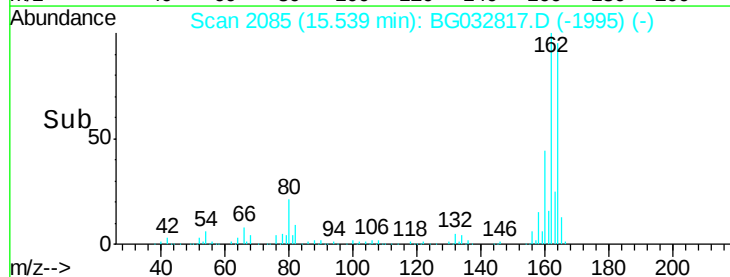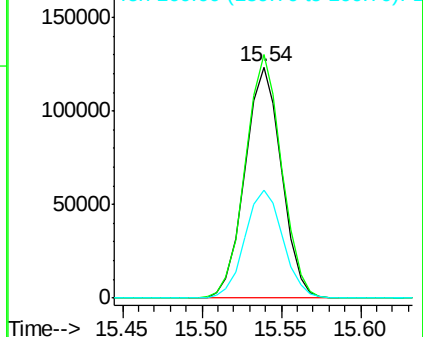


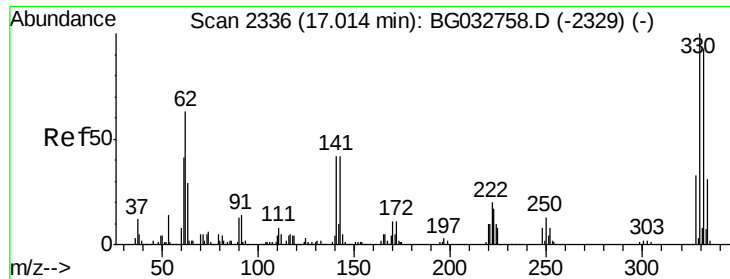



#41
 2,4,6-Tribromophenol
 Concen: 163.028 ng
 RT: 17.01 min Scan# 2335
 Delta R.T. -0.00 min
 Lab File: BG032817.D
 Acq: 26 Feb 2018 11:35

Instrument :
 BNA_G
 ClientSampled :

Tot Ion:330 Resp: 337883
 Ion Ratio Lower Upper
 330 100
 332 94.9 77.0 115.6
 141 42.0 25.2 37.8#

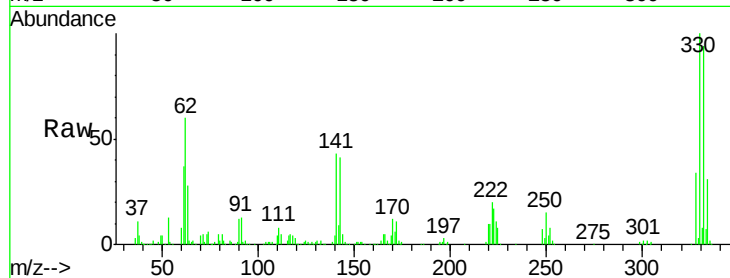


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

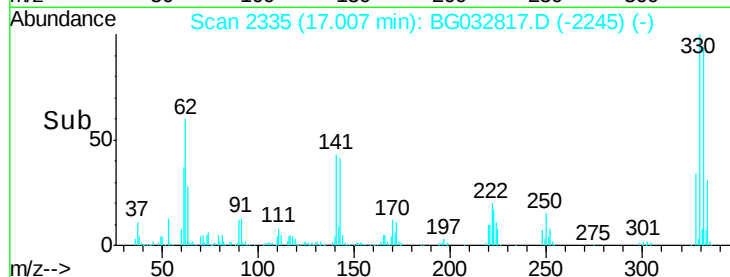
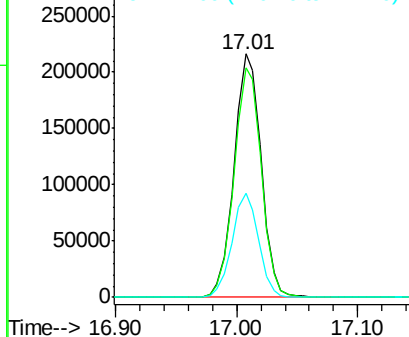



#44
 2-Fluorobiphenyl
 Concen: 94.164 ng
 RT: 14.17 min Scan# 1852
 Delta R.T. -0.00 min
 Lab File: BG032817.D
 Acq: 26 Feb 2018 11:35

Tgt Ion:172 Resp: 1286924
 Ion Ratio Lower Upper
 172 100
 171 39.0 30.0 45.0
 170 25.4 19.5 29.3

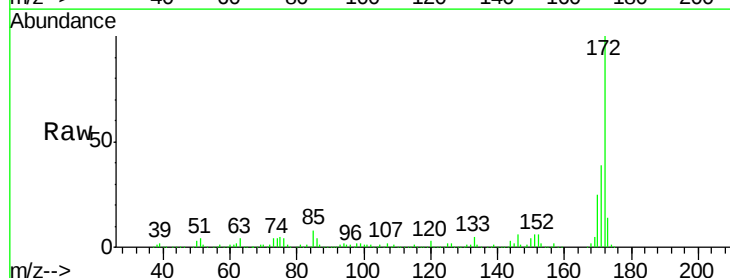

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



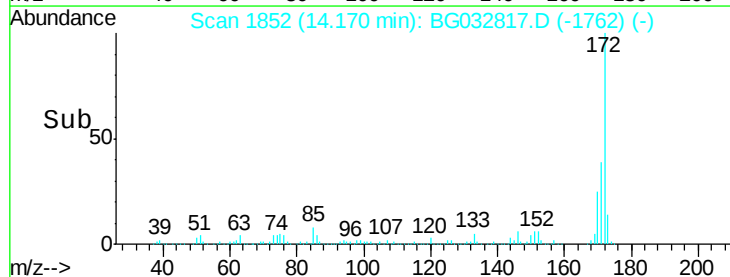
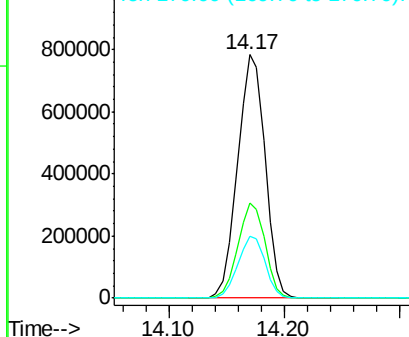




#47
2-Nitroaniline
Concen: 10.388 ng
RT: 14.18 min Scan# 1853
Delta R.T. -0.44 min
Lab File: BG032817.D
Acq: 26 Feb 2018 11:35




Instrument :
BNA_G
ClientSampled :


Tot Ion: 65 Resp: 2252
Ion Ratio Lower Upper
65 100
92 205.0 54.6 82.0#
138 39.0 72.9 109.3#

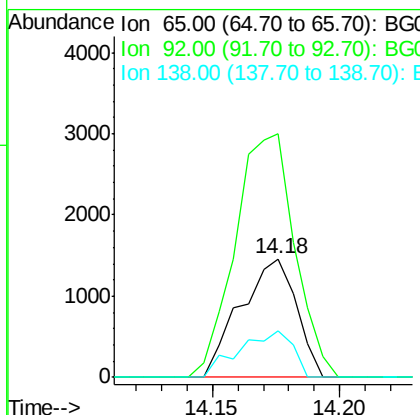

#50
2,6-Dinitrotoluene
Concen: 16.442 ng
RT: 15.54 min Scan# 2085
Delta R.T. 0.44 min
Lab File: BG032817.D
Acq: 26 Feb 2018 11:35

Tgt Ion:165 Resp: 25654
Ion Ratio Lower Upper
165 100
63 1.7 52.7 79.1#
89 2.2 49.2 73.8#



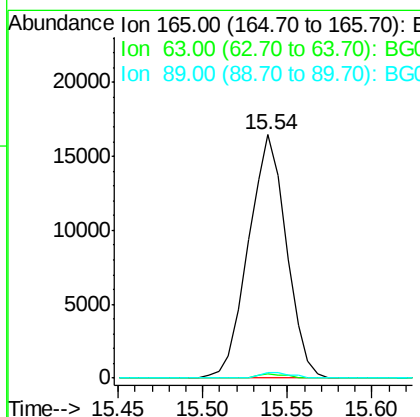



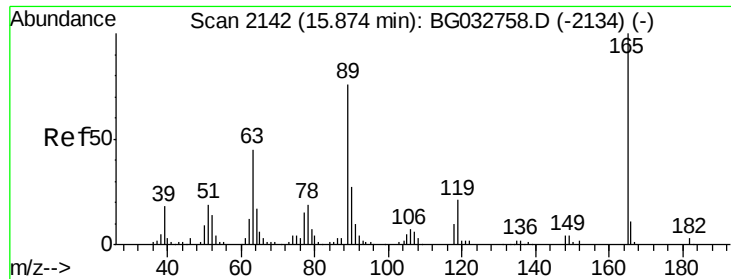

#56
 2,4-Dinitrotoluene
 Concen: 14.640 ng
 RT: 15.54 min Scan# 2085
 Delta R.T. -0.33 min
 Lab File: BG032817.D
 Acq: 26 Feb 2018 11:35




Instrument :
 BNA_G
 ClientSampled :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.7	42.0	63.0#
89	2.2	66.9	100.3#
182	0.0	2.6	3.8#

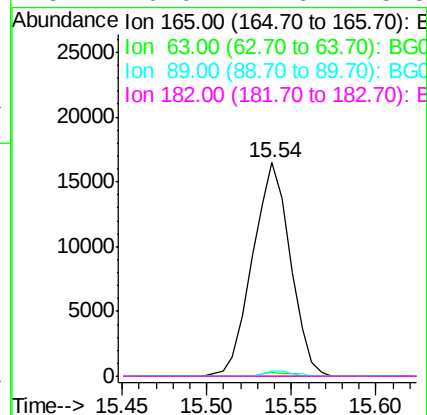

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 18.26 min Scan# 2549
 Delta R.T. -0.00 min
 Lab File: BG032817.D
 Acq: 26 Feb 2018 11:35

Tgt Ion	Ratio	Lower	Upper
188	100		
94	10.9	6.9	10.3#
80	11.7	7.7	11.5#

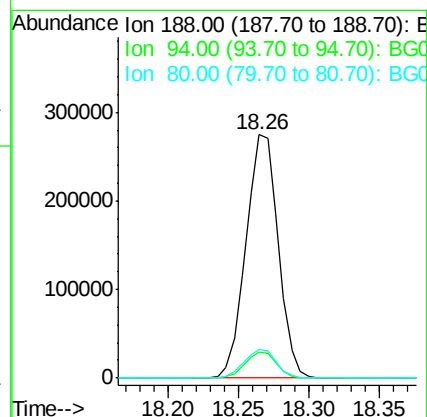


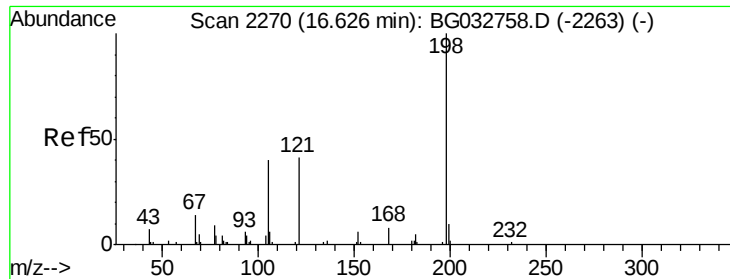




#64
 4,6-Dinitro-2-methylphenol
 Concen: 6.032 ng
 RT: 17.00 min Scan# 2334
 Delta R.T. 0.38 min
 Lab File: BG032817.D
 Acq: 26 Feb 2018 11:35

Instrument :
 BNA_G
 ClientSampleId :

Tot Ion:198 Resp: 1126
 Ion Ratio Lower Upper
 198 100
 51 124.2 30.6 70.6#
 105 159.9 23.8 63.8#

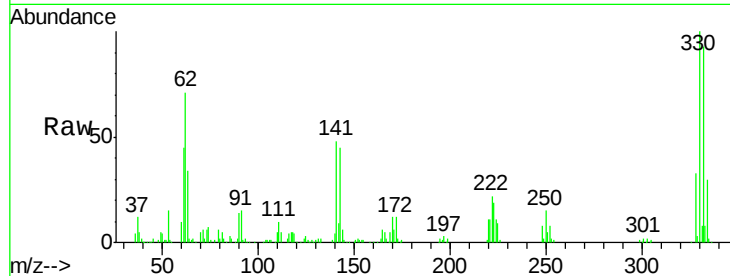


Abundance Ion 198.00 (197.70 to 198.70): E
 Ion 51.00 (50.70 to 51.70): BGO
 Ion 105.00 (104.70 to 105.70): E

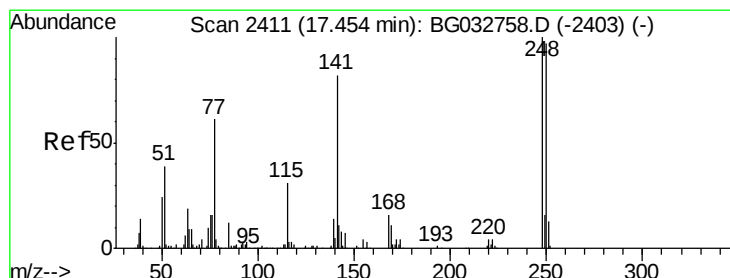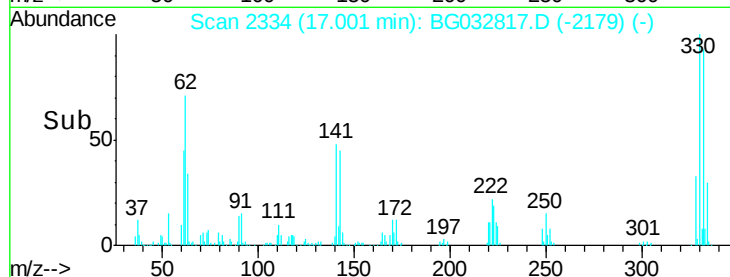
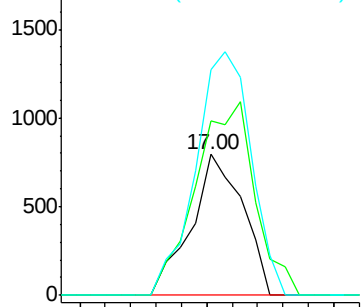



#66
 4-Bromophenyl-phenylether
 Concen: 5.273 ng
 RT: 17.01 min Scan# 2335
 Delta R.T. -0.44 min
 Lab File: BG032817.D
 Acq: 26 Feb 2018 11:35

Tgt Ion:248 Resp: 24570
 Ion Ratio Lower Upper
 248 100
 250 196.4 77.1 115.7#
 141 577.8 50.8 76.2#

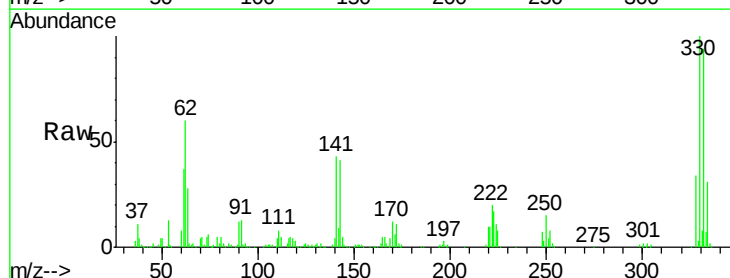

Abundance Ion 248.00 (247.70 to 248.70): E
 Ion 250.00 (249.70 to 250.70): E
 Ion 141.00 (140.70 to 141.70): E

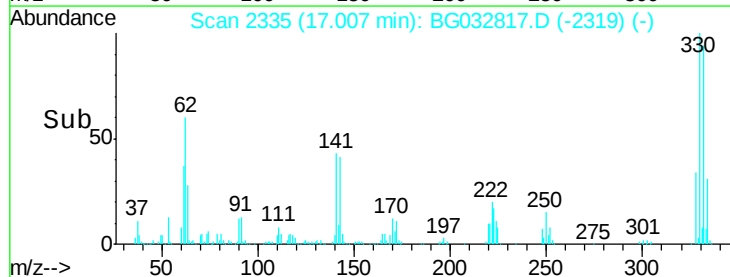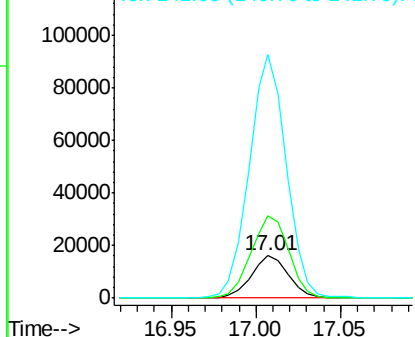



#75

Chrysene-d12

Concen: 20.000 ng

RT: 22.62 min Scan# 3291

Delta R.T. -0.01 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35

Instrument :

BNA_G

ClientSampleId :


Tot Ion:240 Resp: 450317

Ion Ratio Lower Upper

240 100

120 12.7 6.8 10.2#




236 26.1 20.9 31.3



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

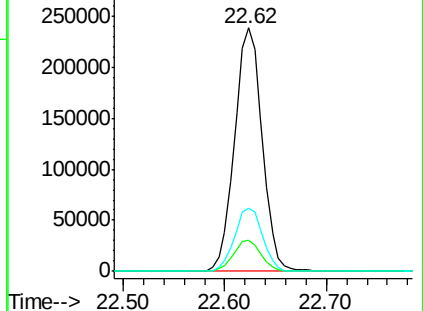

#76

Benzidine

Concen: 2.085 ng

RT: 20.79 min Scan# 2979

Delta R.T. 0.00 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35


Tgt Ion:184 Resp: 32009

Ion Ratio Lower Upper

184 100

185 15.5 11.1 16.7



183 10.6 10.6 16.0#




Abundance Ion 184.00 (183.70 to 184.70): E

Ion 185.00 (184.70 to 185.70): E

Ion 183.00 (182.70 to 183.70): E

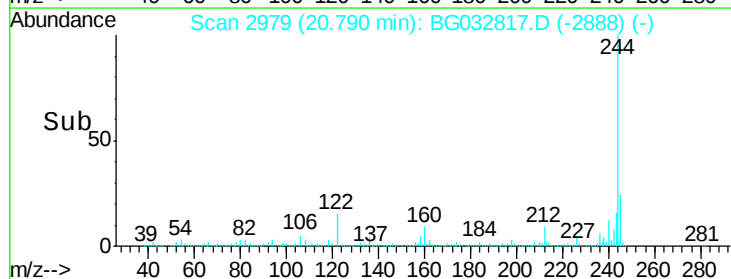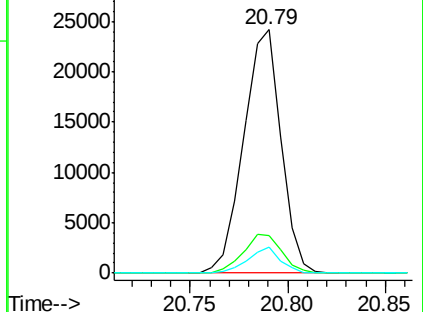

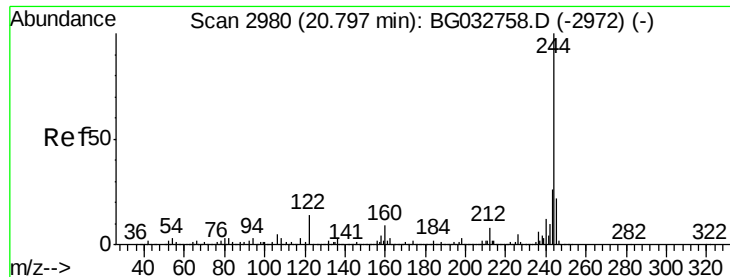

#78

Terphenyl-d14

Concen: 91.668 ng

RT: 20.79 min Scan# 2979

Delta R.T. 0.00 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35

Instrument :

BNA_G

ClientSampleId :


Tot Ion:244 Resp: 1837320

Ion Ratio Lower Upper

244 100

212 8.8 5.8 8.8#




122 14.7 7.0 10.4#

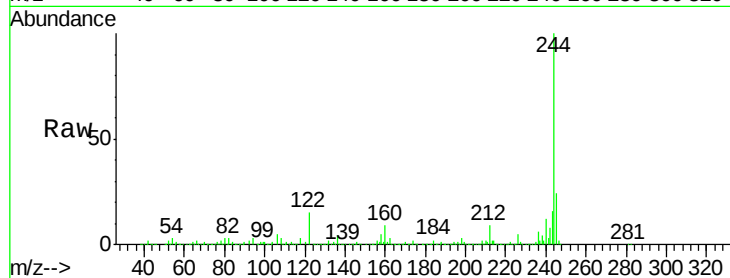

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

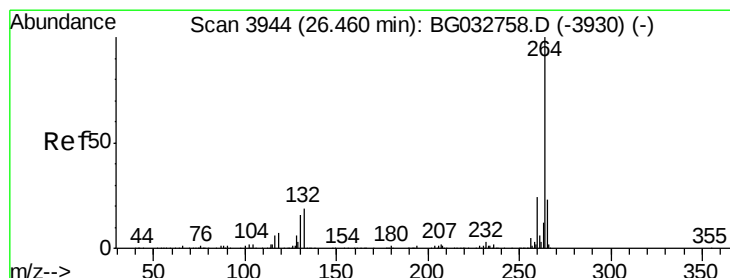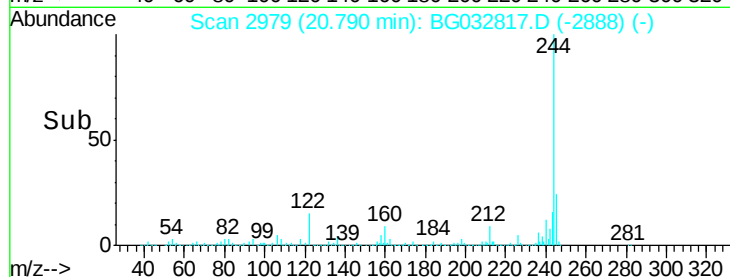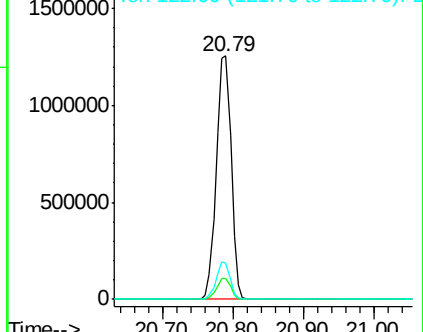

#86

Perylene-d12

Concen: 20.000 ng

RT: 26.44 min Scan# 3940

Delta R.T. -0.00 min

Lab File: BG032817.D

Acq: 26 Feb 2018 11:35


Tgt Ion:264 Resp: 490127

Ion Ratio Lower Upper

264 100

260 23.9 17.4 26.0

265 21.3 17.7 26.5

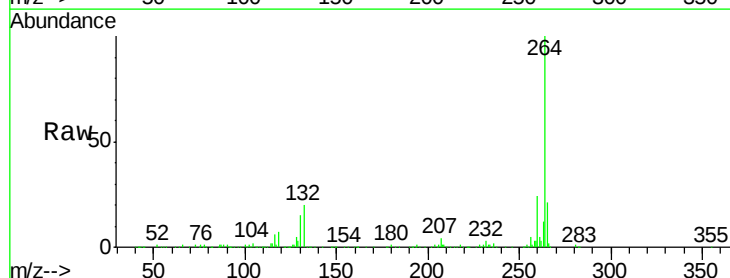

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

