
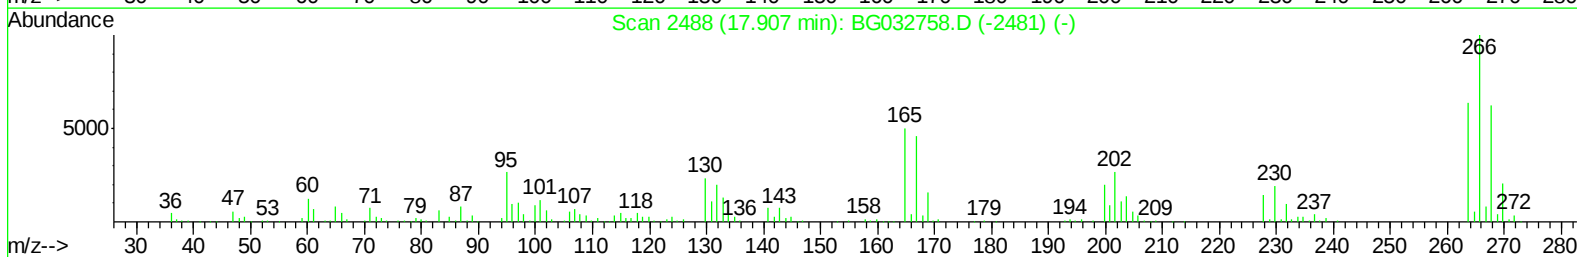
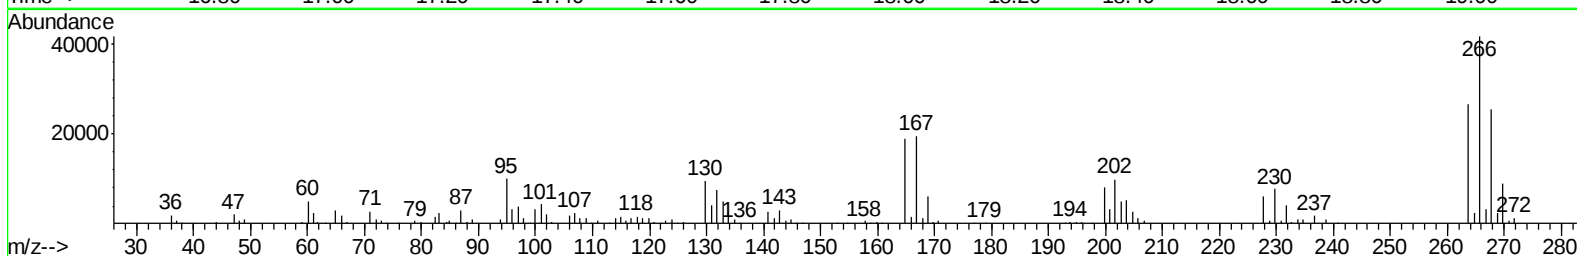


Data Path : Z:\HPCHEM1\BNA G\DATA\BG022618\
Data File : BG032831.D
Acq On : 26 Feb 2018 21:32
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 04:02:23 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 26 17:50:45 2018
Response via : Initial Calibration

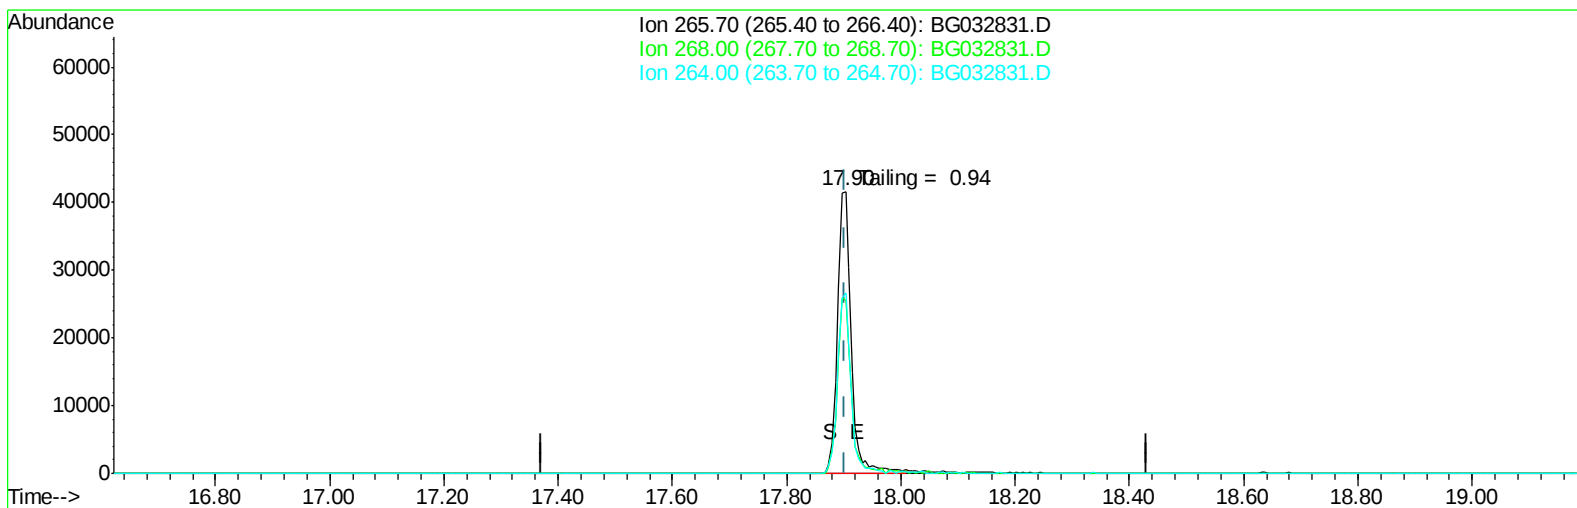

TIC: BG032831.D

(69) Pentachlorophenol (C)




17.903min (+0.000) 27838.22ng

response 70529

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.46
264.00	62.00	63.98
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG022618\
 Data File : BG032831.D
 Acq On : 26 Feb 2018 21:32
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 04:02:23 2018
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 26 17:50:45 2018
 Response via : Initial Calibration

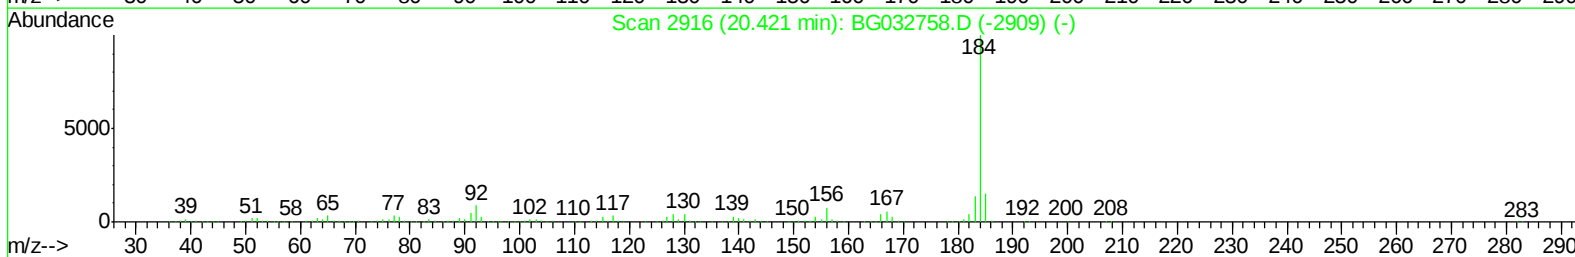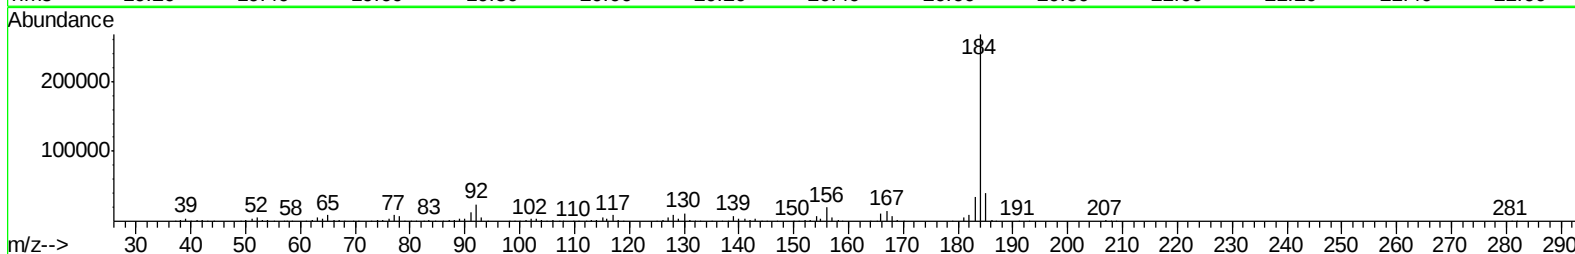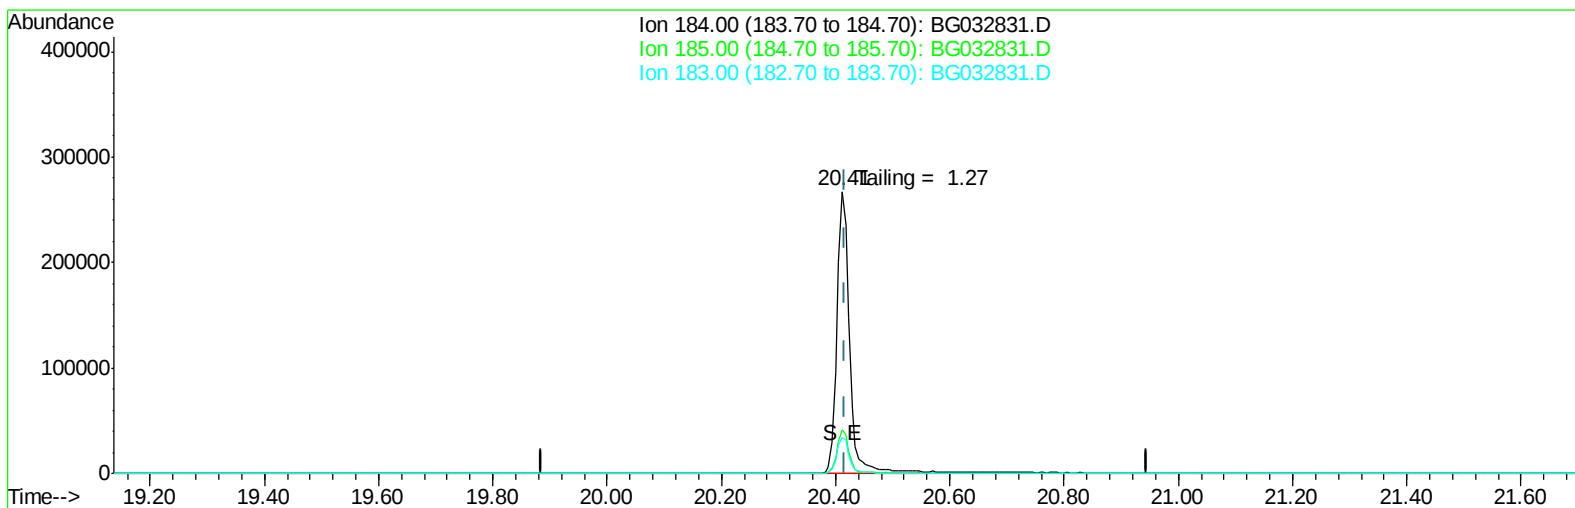

TIC: BG032831.D

(76) Benzidine

20.411min (-0.006) 0.00ng

response 407890

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.28
183.00	13.30	12.81
0.00	0.00	0.00