


Data Path : Z:\HPCHEM1\BNA G\Data\BG022618\
 Data File : BG032814.D
 Acq On : 26 Feb 2018 9:02
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 26 17:50:45 2018

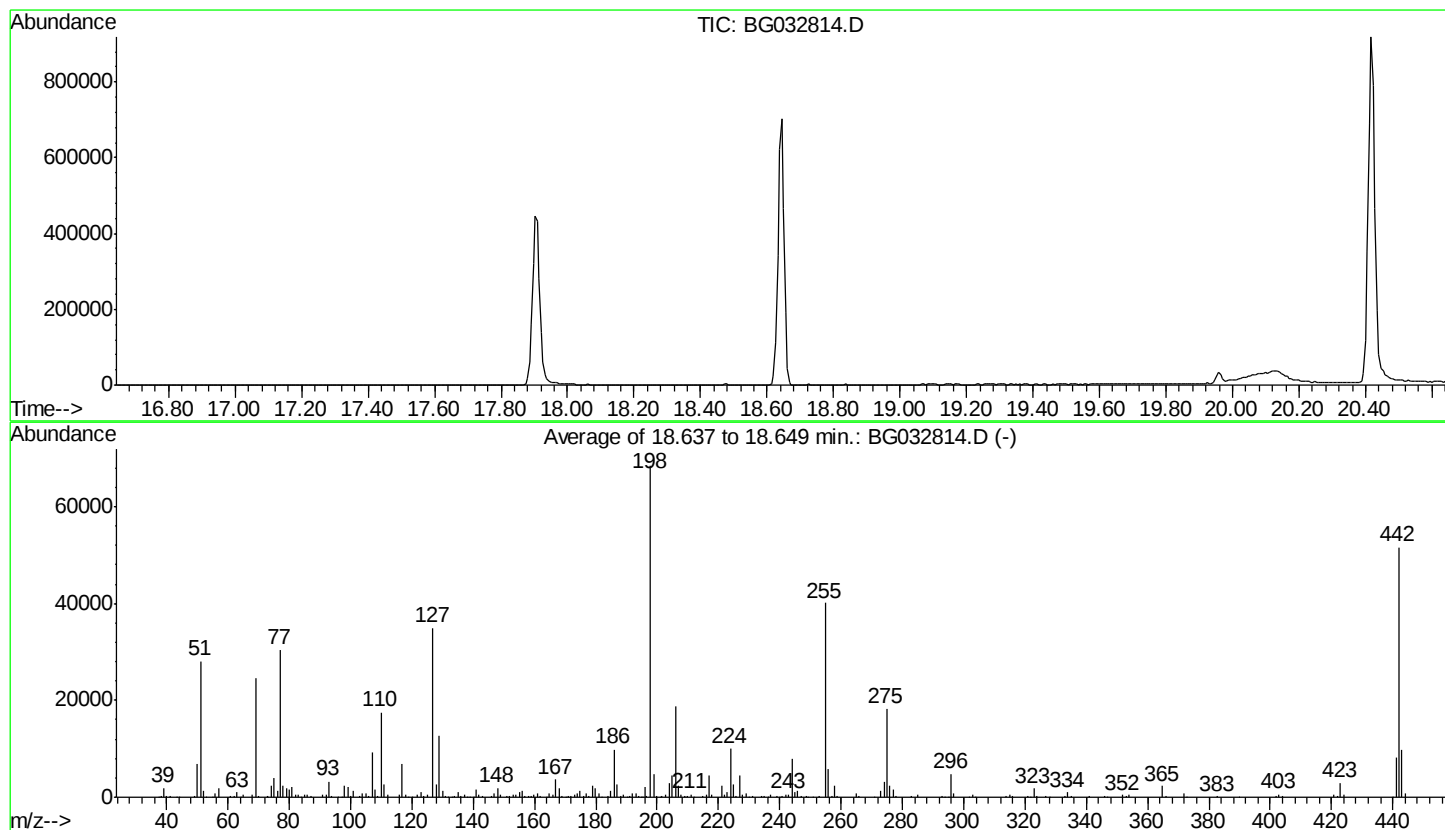

AutoFind: Scans 2613, 2614, 2615; Background Corrected with Scan 2606

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.9	28029	PASS
68	69	0.00	2	1.8	429	PASS
69	198	0.00	100	35.7	24464	PASS
70	69	0.00	2	0.6	144	PASS
127	198	10	80	51.1	35000	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	68469	PASS
199	198	5	9	7.0	4769	PASS
275	198	10	60	26.7	18265	PASS
365	198	1	100	3.4	2352	PASS
441	442	0.01	24	15.7	8110	PASS
442	198	50	100	75.4	51658	PASS
443	442	15	24	18.9	9775	PASS