
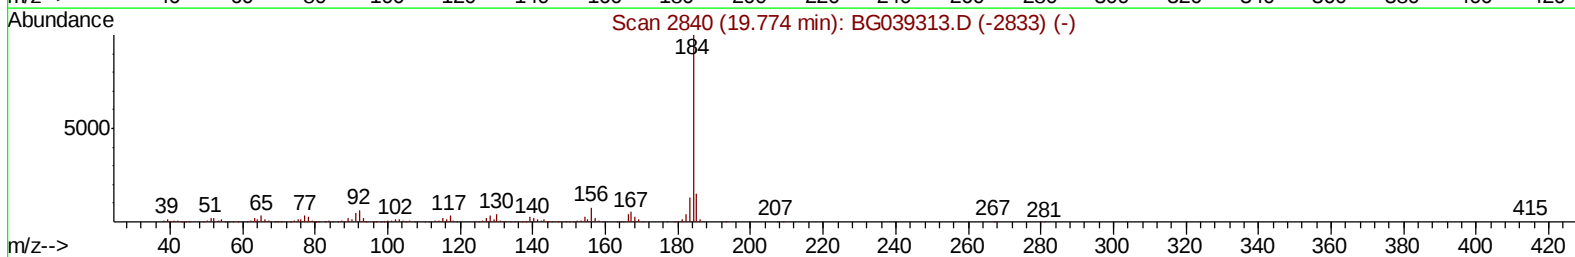
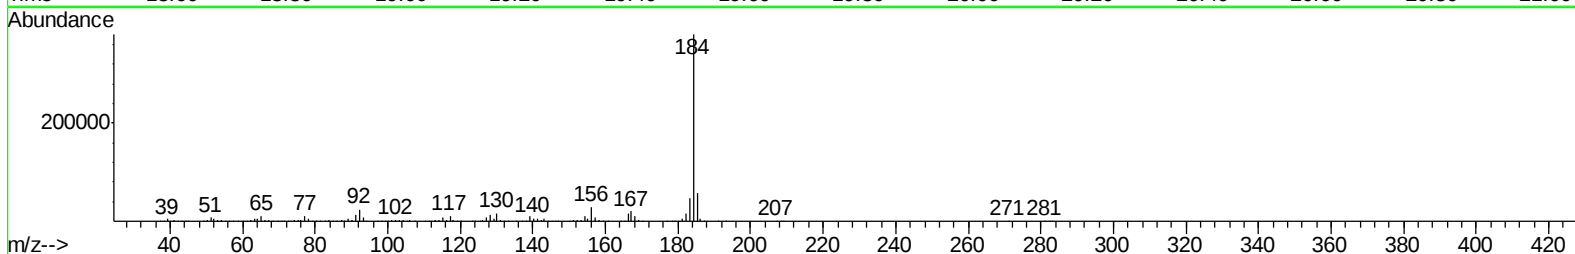


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022619\
Data File : BG039596.D
Acq On : 26 Feb 2019 12:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 08:22:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

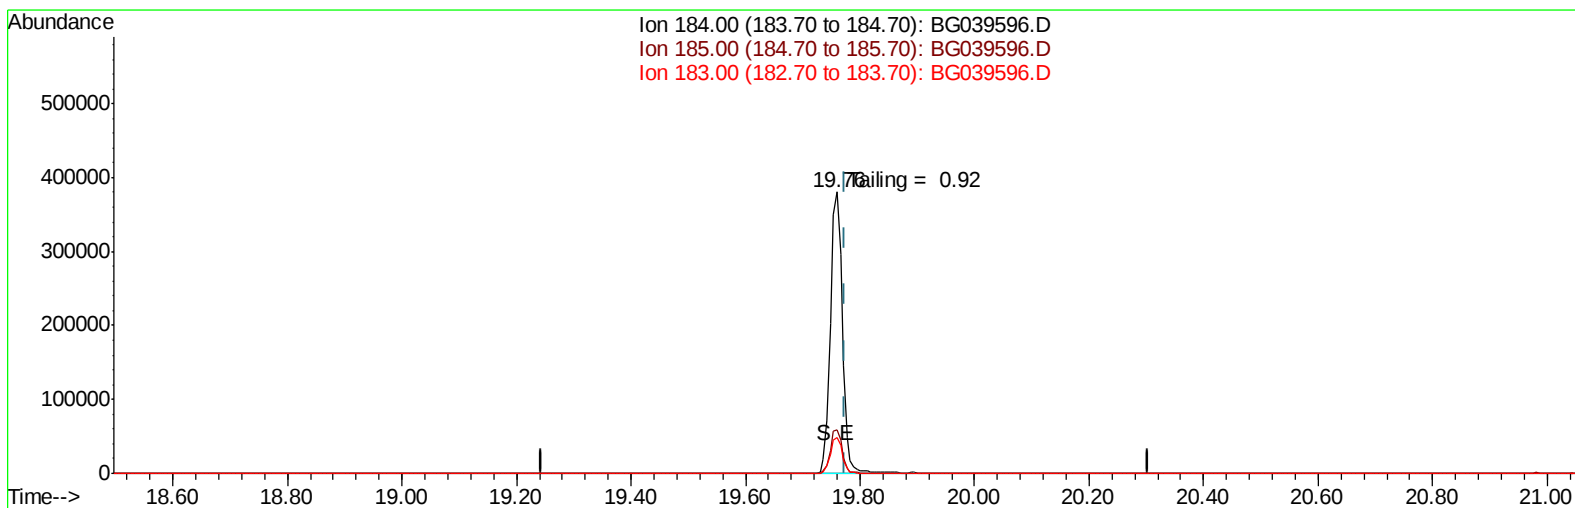

TIC: BG039596.D

(77) Benzidine




19.760min (-0.015) 313198.80ng

response 554494

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	15.45
183.00	13.20	12.59
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG022619\
Data File : BG039596.D
Acq On : 26 Feb 2019 12:05
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 27 08:22:18 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

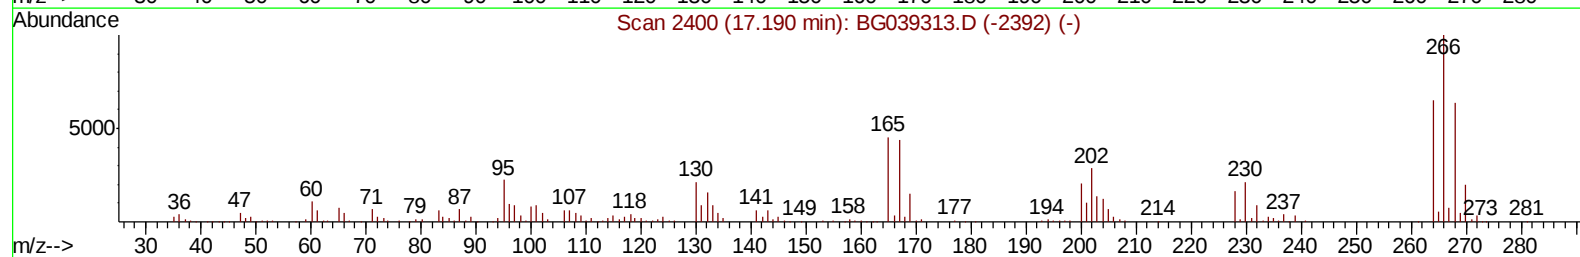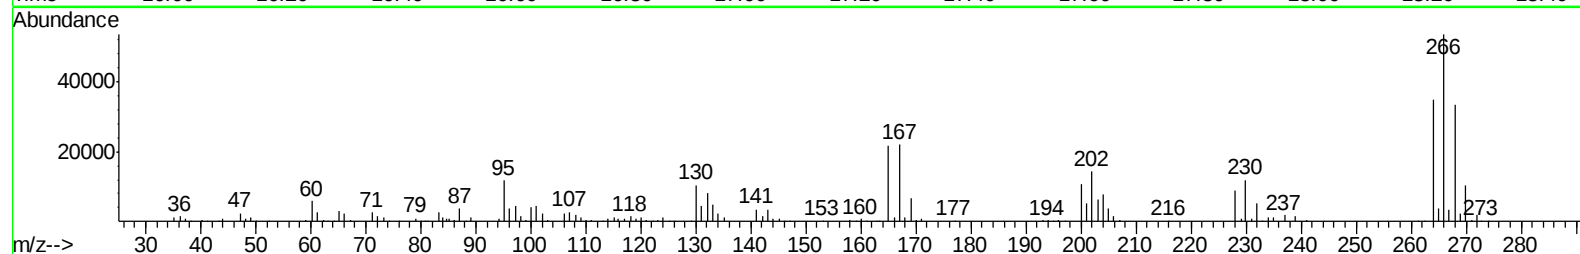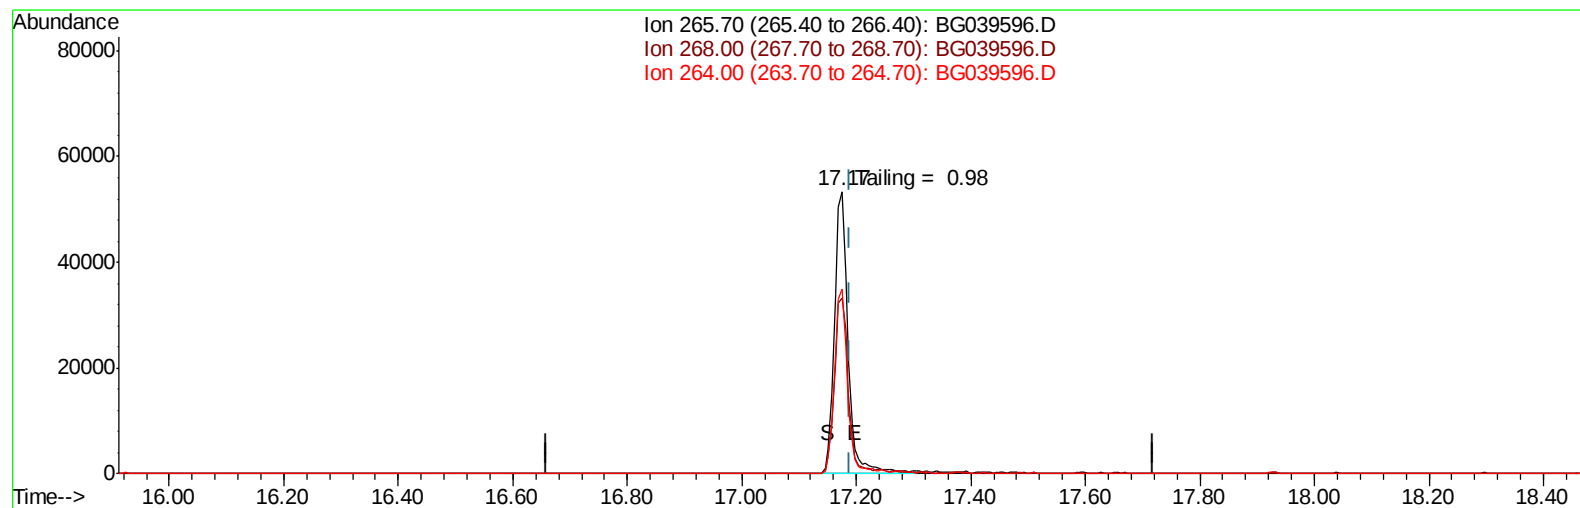

TIC: BG039596.D

(70) Pentachlorophenol (C)

17.175min (-0.015) 28268.76ng

response 87255

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.12
264.00	65.10	65.48
0.00	0.00	0.00