

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022619\
 Data File : BG039620.D
 Acq On : 27 Feb 2019 4:38
 Operator : JU/SJ
 Sample : K1597-04
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-26

Quant Time: Feb 27 06:50:50 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 29 15:41:51 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.17	152	57599	20.00	ng	-0.01
21) Naphthalene-d8	10.99	136	244712	20.00	ng	-0.02
39) Acenaphthene-d10	14.79	164	159755	20.00	ng	-0.02
64) Phenanthrene-d10	17.54	188	379923	20.00	ng	-0.02
76) Chrysene-d12	21.82	240	419384	20.00	ng	-0.03
87) Perylene-d12	25.20	264	412854	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.72	112	450764	133.94	ng	0.00
7) Phenol-d6	7.31	99	574884	116.05	ng	0.00
23) Nitrobenzene-d5	9.35	82	432077	110.30	ng	-0.02
42) 2,4,6-Tribromophenol	16.28	330	259440	150.81	ng	-0.01
45) 2-Fluorobiphenyl	13.41	172	999547	89.76	ng	-0.02
79) Terphenyl-d14	20.13	244	1618833	81.70	ng	-0.02


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022619\
Data File : BG039620.D
Acq On : 27 Feb 2019 4:38
Operator : JU/SJ
Sample : K1597-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-26

Quant Time: Feb 27 06:50:50 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG012919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 29 15:41:51 2019
Response via : Initial Calibration

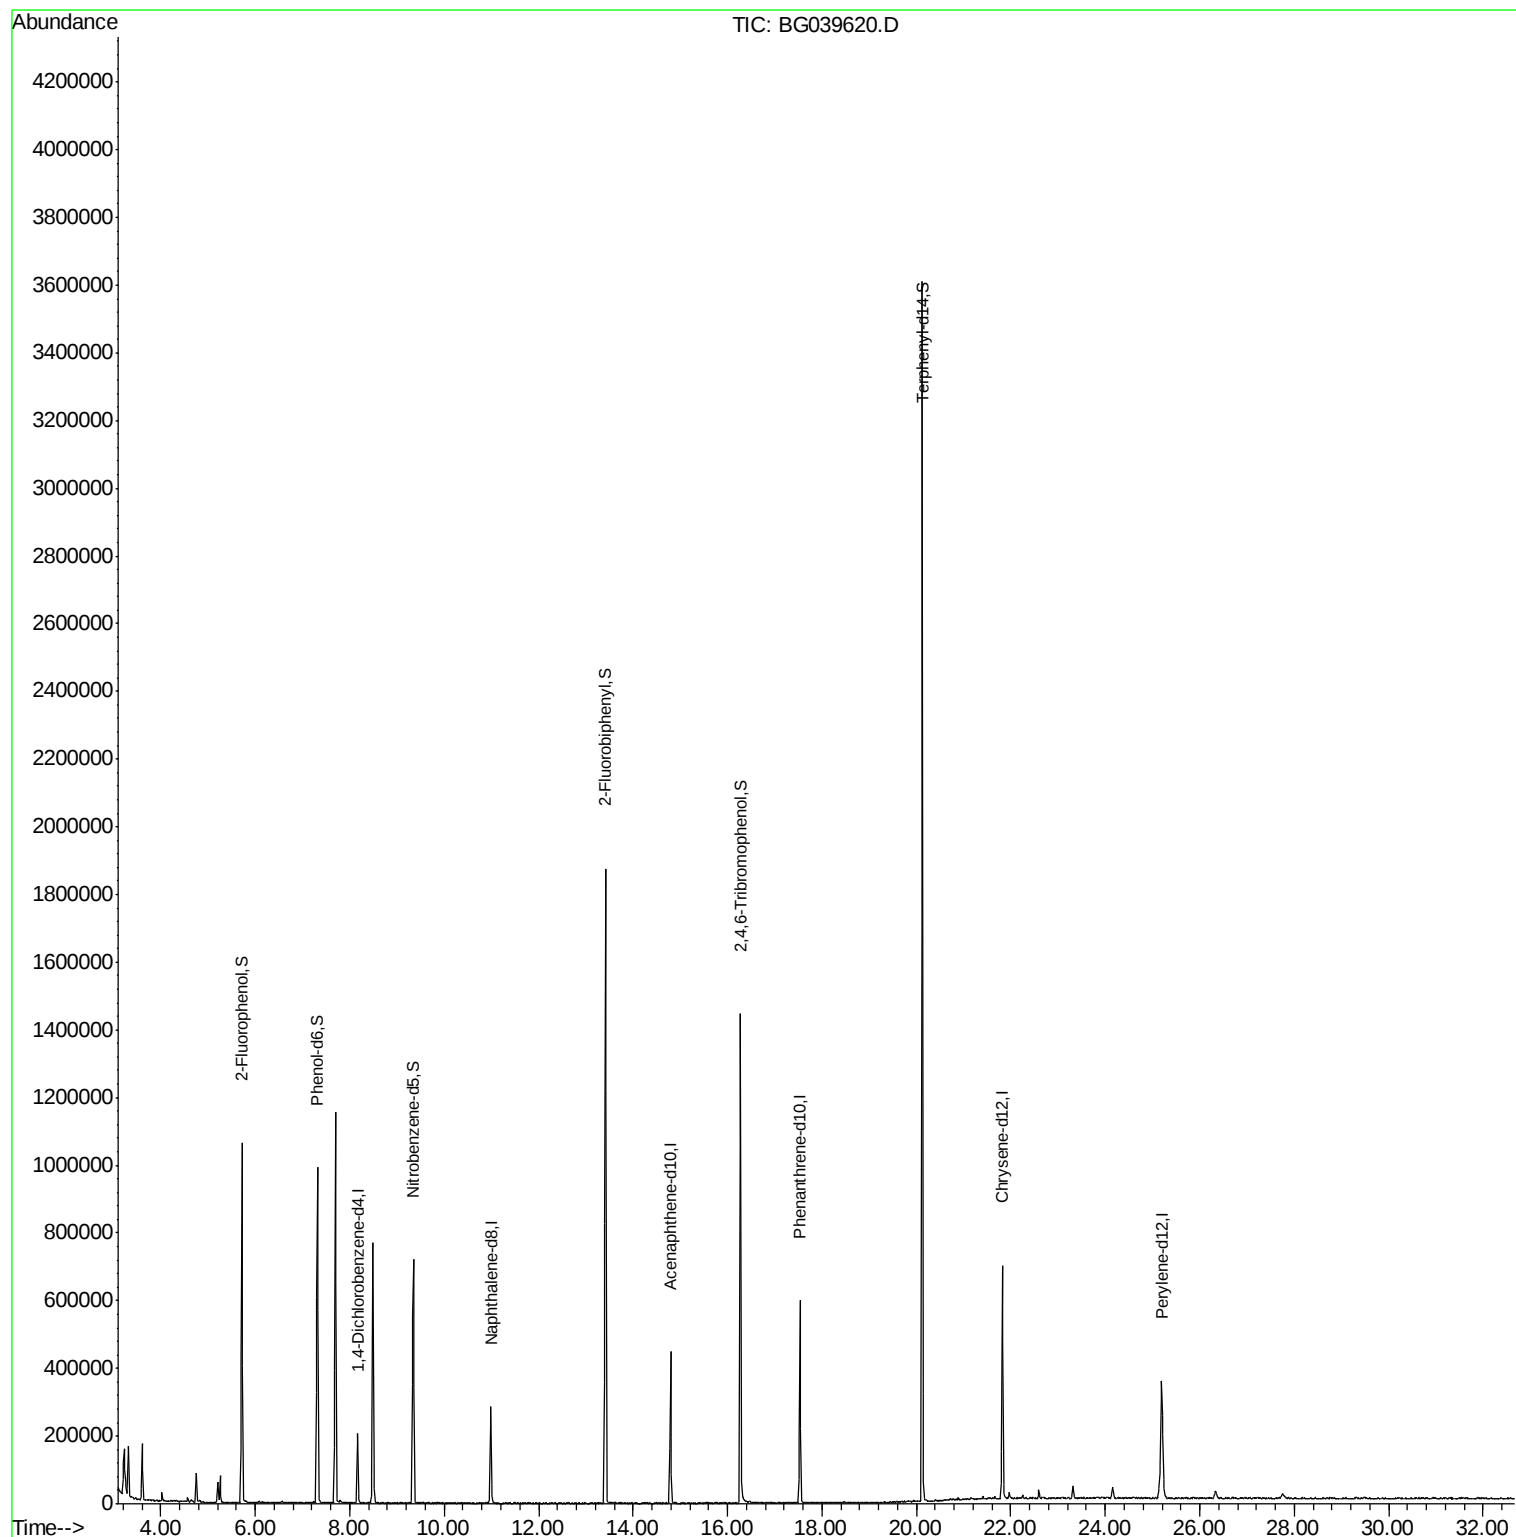




#1

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.17 min Scan# 865
Delta R.T. -0.01 min
Lab File: BG039620.D
Acq: 27 Feb 2019 4:38

Instrument :
BNA_G
ClientSampleId :
TP-26

Tot Ion	Ratio	Lower	Upper
152	100		
150	141.1	123.7	185.5
115	57.2	45.9	68.9


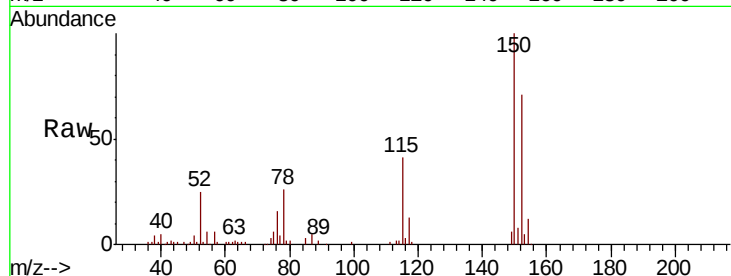


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E


Ion 115.00 (114.70 to 115.70): E

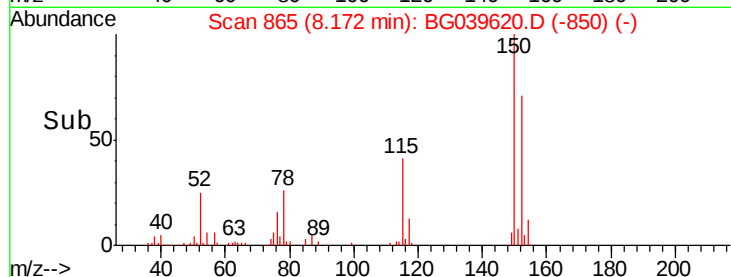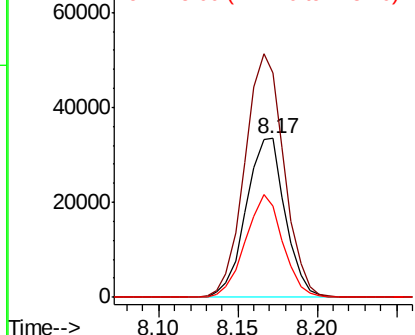

#5

2-Fluorophenol
Concen: 133.941 ng
RT: 5.72 min Scan# 447
Delta R.T. -0.00 min
Lab File: BG039620.D
Acq: 27 Feb 2019 4:38

Tgt Ion	Ratio	Lower	Upper
112	100		
64	66.7	57.8	86.8
63	37.0	29.8	44.6


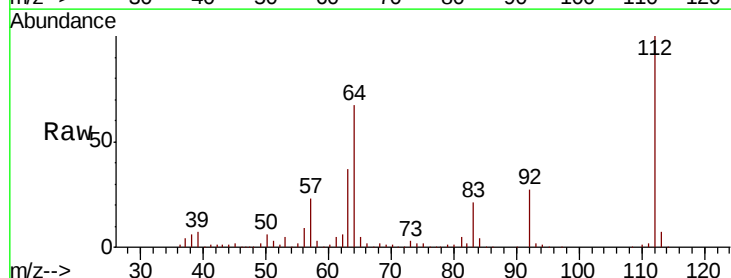


Abundance

Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BG

Ion 63.00 (62.70 to 63.70): BG

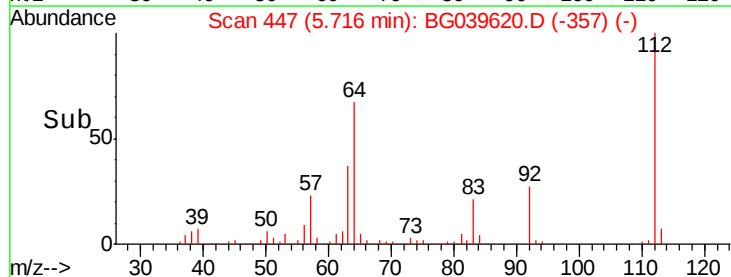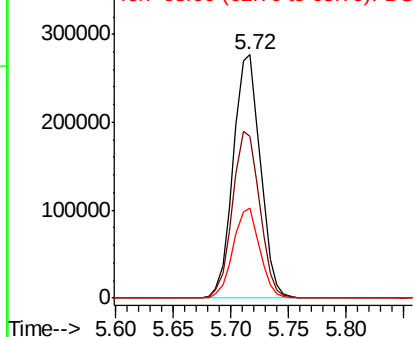



#7

Phenol-d6

Concen: 116.050 ng

RT: 7.31 min Scan# 719

Delta R.T. -0.01 min

Lab File: BG039620.D

Acq: 27 Feb 2019 4:38

Instrument :

BNA_G

ClientSampleId :

TP-26


Tot Ion: 99 Resp: 574884

Ion Ratio Lower Upper




99 100

42 20.1 18.2 27.2

71 35.5 28.0 42.0

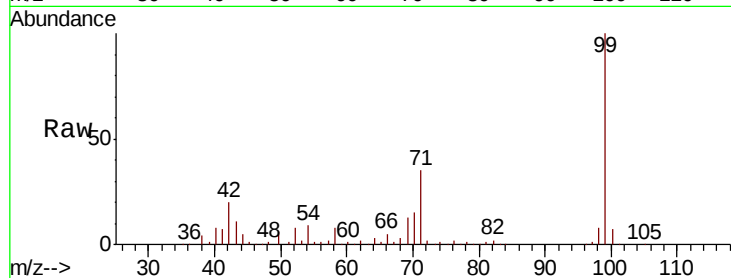

Abundance Ion 99.00 (98.70 to 99.70): BGC
Ion 42.00 (41.70 to 42.70): BGC
Ion 71.00 (70.70 to 71.70): BGC

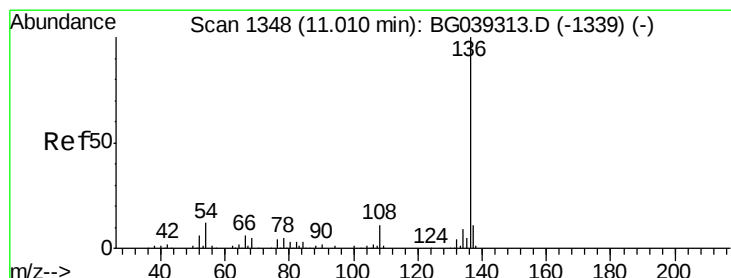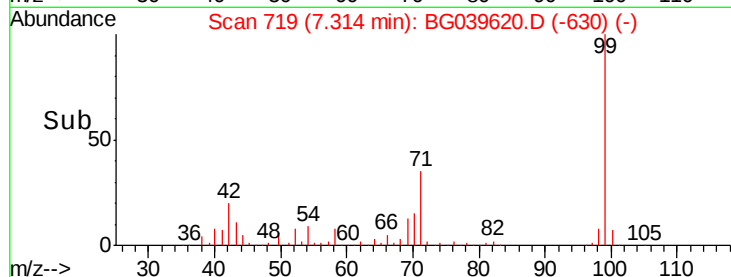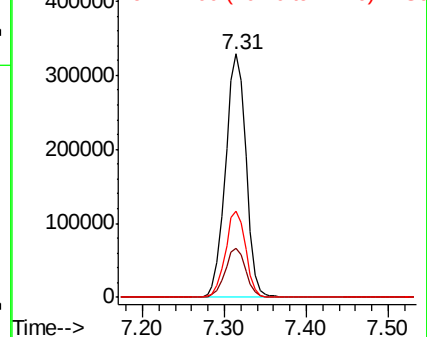

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 10.99 min Scan# 1344

Delta R.T. -0.02 min

Lab File: BG039620.D

Acq: 27 Feb 2019 4:38

Tgt Ion: 136 Resp: 244712


Ion Ratio Lower Upper

136 100



137 10.6 9.1 13.7


54 10.3 9.4 14.2

68 6.0 4.2 6.4

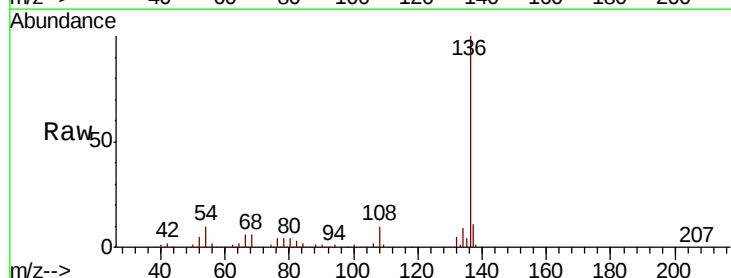

Abundance Ion 136.00 (135.70 to 136.70): BGC
Ion 137.00 (136.70 to 137.70): BGC
Ion 54.00 (53.70 to 54.70): BGC
Ion 68.00 (67.70 to 68.70): BGC



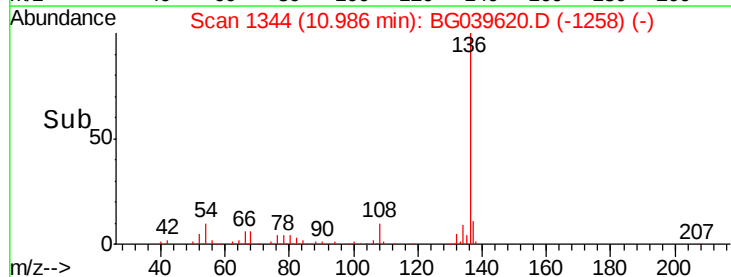
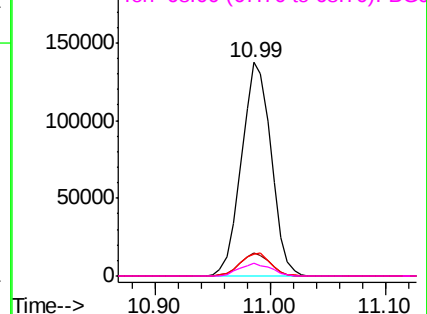


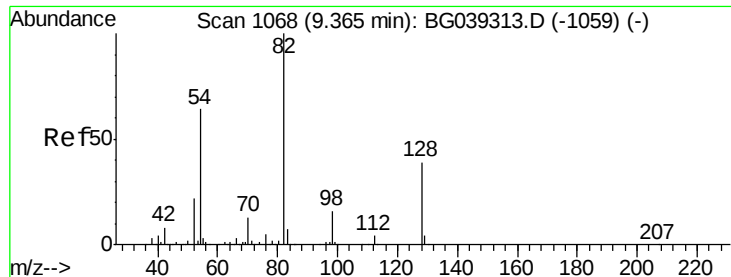

#23
 Nitrobenzene-d5
 Concen: 110.303 ng
 RT: 9.35 min Scan# 1065
 Delta R.T. -0.02 min
 Lab File: BG039620.D
 Acq: 27 Feb 2019 4:38




Instrument :
 BNA_G
 ClientSampleId :
 TP-26


Tot Ion	82.00	Resp	432077
Ion Ratio	Lower	Upper	
82	100		
128	44.4	31.3	46.9
54	59.6	50.9	76.3

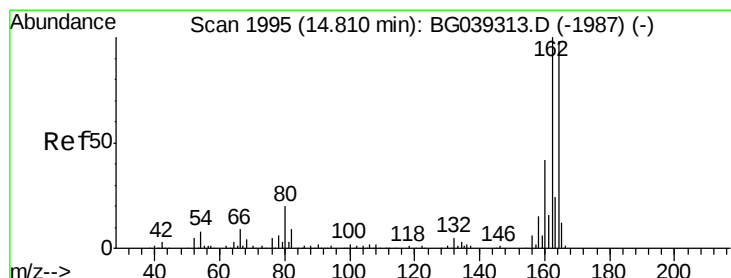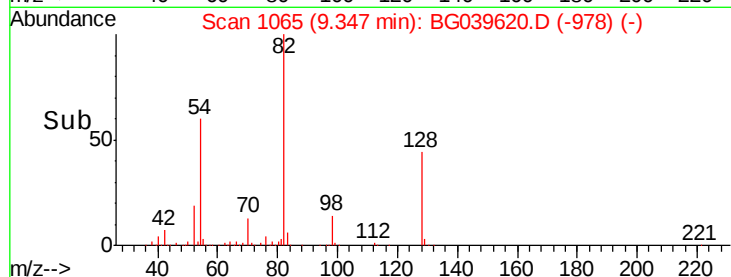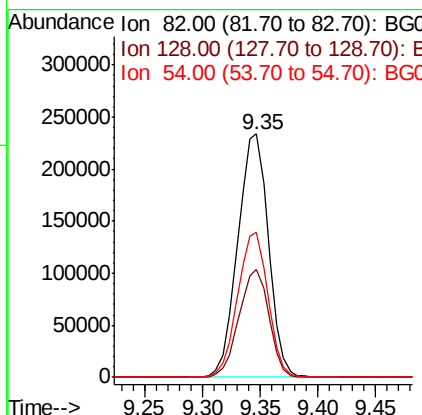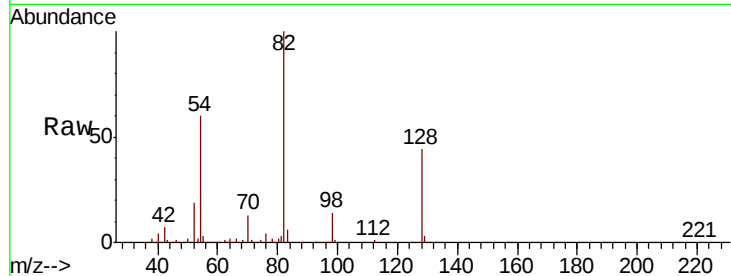

#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 14.79 min Scan# 1992
 Delta R.T. -0.02 min
 Lab File: BG039620.D
 Acq: 27 Feb 2019 4:38

Tgt Ion	164	Resp	159755
Ion Ratio	Lower	Upper	
164	100		
162	101.7	81.6	122.4
160	44.2	34.2	51.2

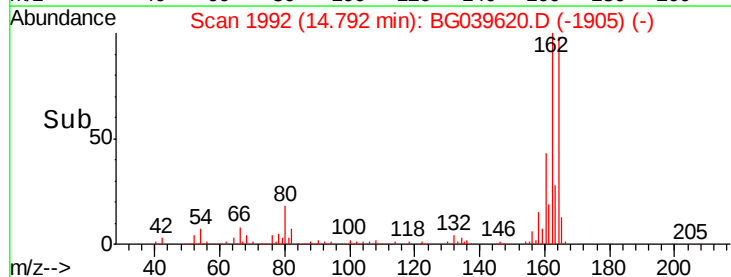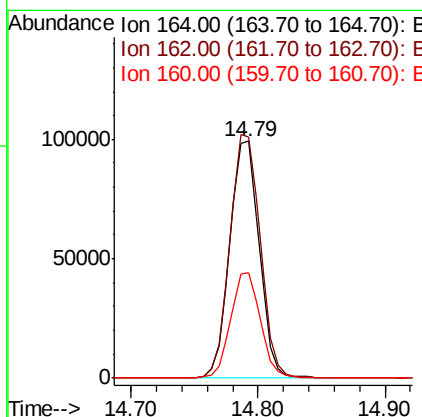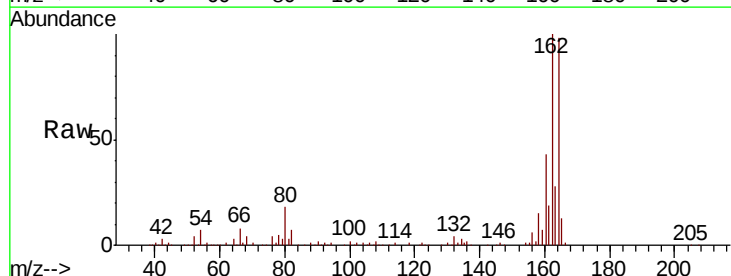


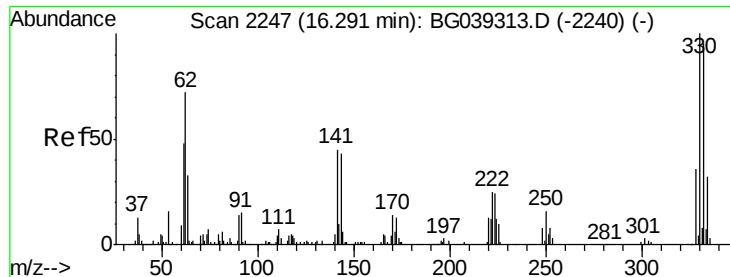



#42
 2,4,6-Tribromophenol
 Concen: 150.812 ng
 RT: 16.28 min Scan# 2245
 Delta R.T. -0.01 min
 Lab File: BG039620.D
 Acq: 27 Feb 2019 4:38

Instrument :
 BNA_G
 ClientSampleId :
 TP-26

Tot Ion:330 Resp: 259440
 Ion Ratio Lower Upper
 330 100
 332 95.4 75.7 113.5
 141 41.4 35.6 53.4

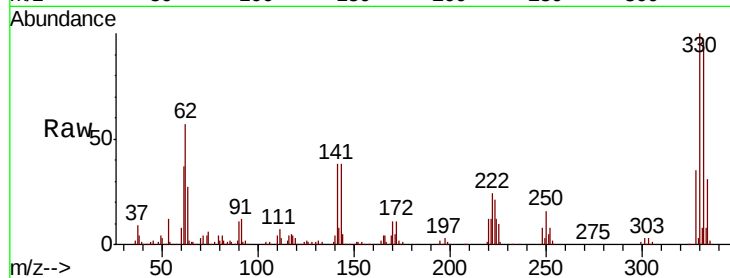


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

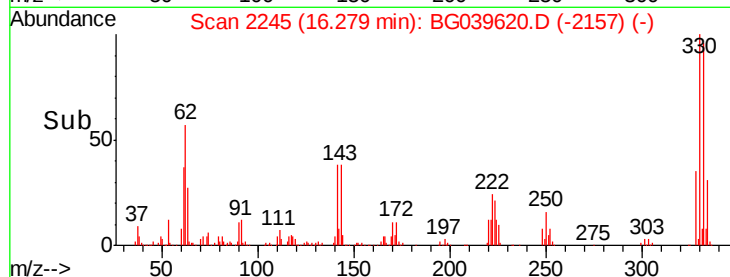
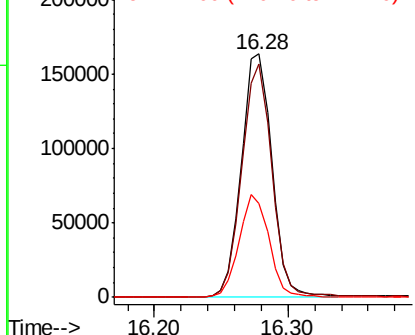


#45
 2-Fluorobiphenyl
 Concen: 89.756 ng
 RT: 13.41 min Scan# 1757
 Delta R.T. -0.02 min
 Lab File: BG039620.D
 Acq: 27 Feb 2019 4:38

Tgt Ion:172 Resp: 999547
 Ion Ratio Lower Upper
 172 100
 171 37.1 30.8 46.2
 170 25.9 20.2 30.4

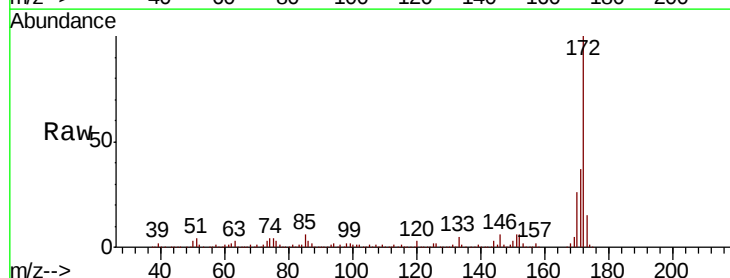

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

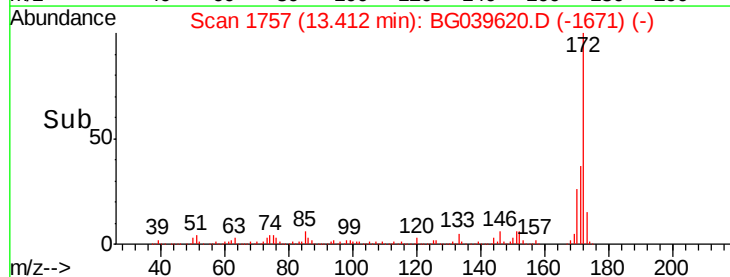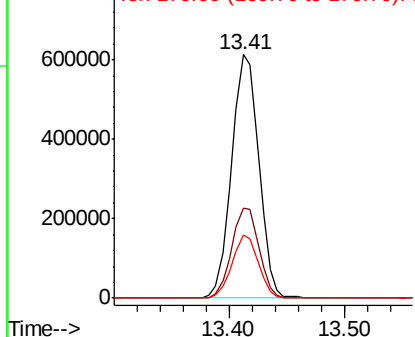



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 17.54 min Scan# 2459

Delta R.T. -0.02 min

Lab File: BG039620.D

Acq: 27 Feb 2019 4:38

Instrument :

BNA_G

ClientSampleId :

TP-26


Tot Ion:188 Resp: 379923

Ion Ratio Lower Upper

188 100

94 7.8 6.9 10.3

80 8.9 8.1 12.1

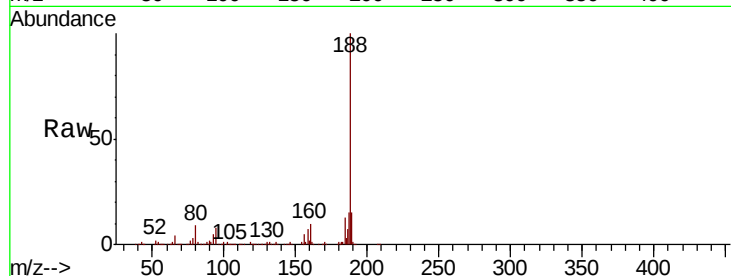

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BG

Ion 80.00 (79.70 to 80.70): BG

300000

200000

100000



0

17.54

17.50

17.60

Time-->

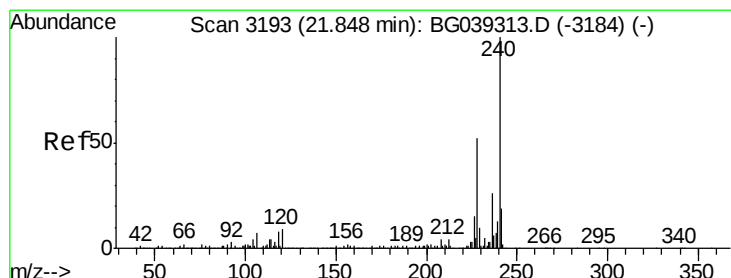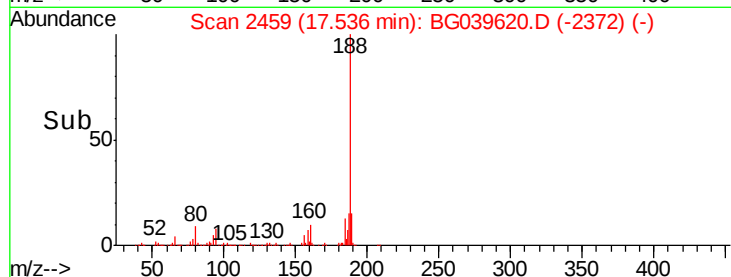

#76

Chrysene-d12

Concen: 20.000 ng

RT: 21.82 min Scan# 3188

Delta R.T. -0.03 min

Lab File: BG039620.D

Acq: 27 Feb 2019 4:38


Tgt Ion:240 Resp: 419384

Ion Ratio Lower Upper

240 100

120 8.9 7.0 10.6

236 26.4 21.0 31.4

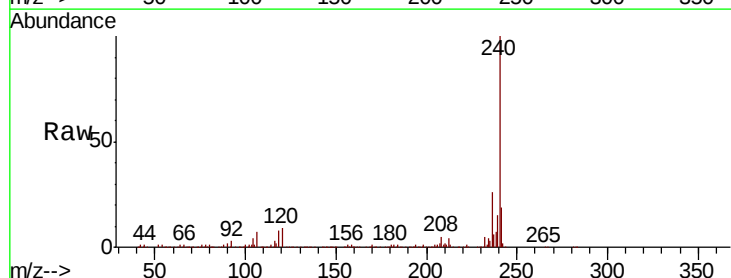

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

300000

200000

100000


0


21.82

21.70

21.90

Time-->

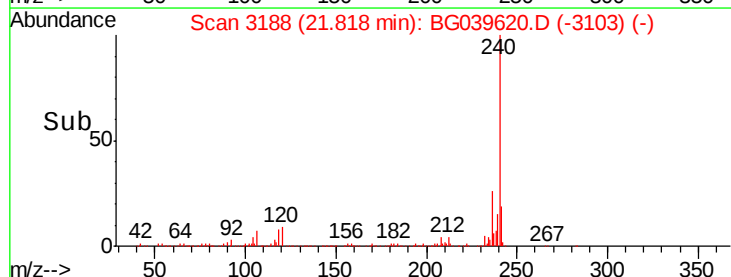

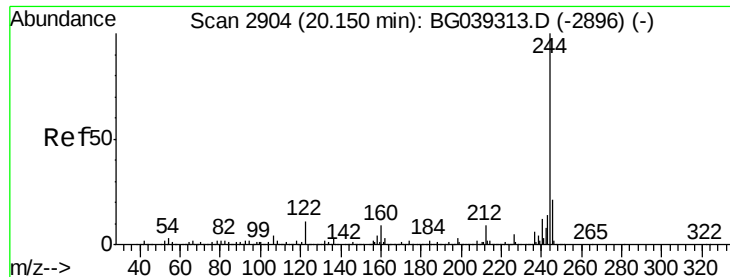

#79

Terphenyl-d14

Concen: 81.705 ng

RT: 20.13 min Scan# 2900

Delta R.T. -0.02 min

Lab File: BG039620.D

Acq: 27 Feb 2019 4:38

Instrument :

BNA_G

ClientSampleId :

TP-26


Tot Ion:244 Resp: 1618833

Ion Ratio Lower Upper

244 100

212 9.9 7.3 10.9



122 9.9 8.4 12.6

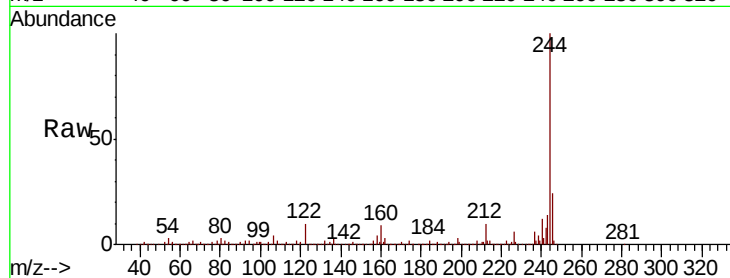

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

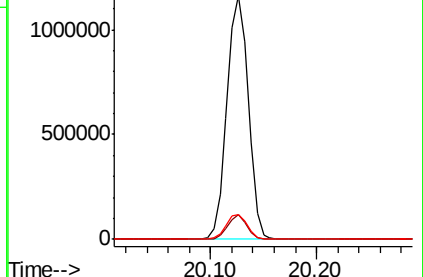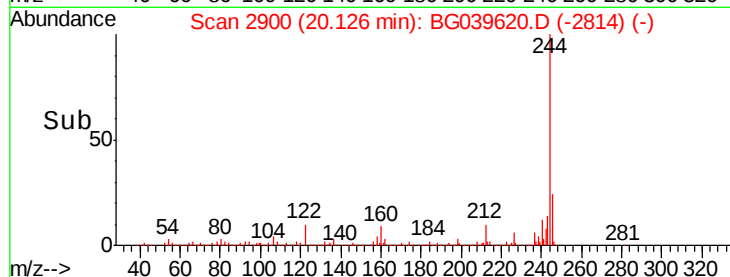

#87

Perylene-d12

Concen: 20.000 ng

RT: 25.20 min Scan# 3763

Delta R.T. -0.05 min

Lab File: BG039620.D

Acq: 27 Feb 2019 4:38


Tgt Ion:264 Resp: 412854

Ion Ratio Lower Upper

264 100

260 24.0 18.2 27.4

265 21.8 18.5 27.7

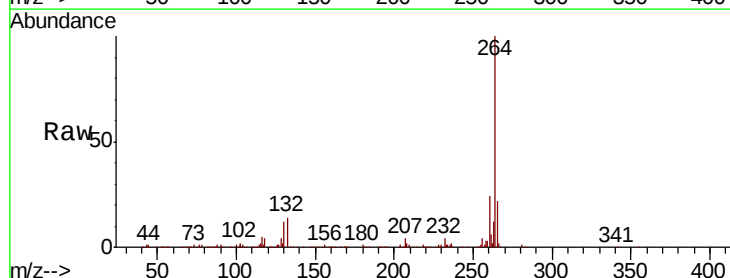

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

