


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG022619\
 Data File : BG039615.D
 Acq On : 27 Feb 2019 1:17
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG012919.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 29 15:41:51 2019

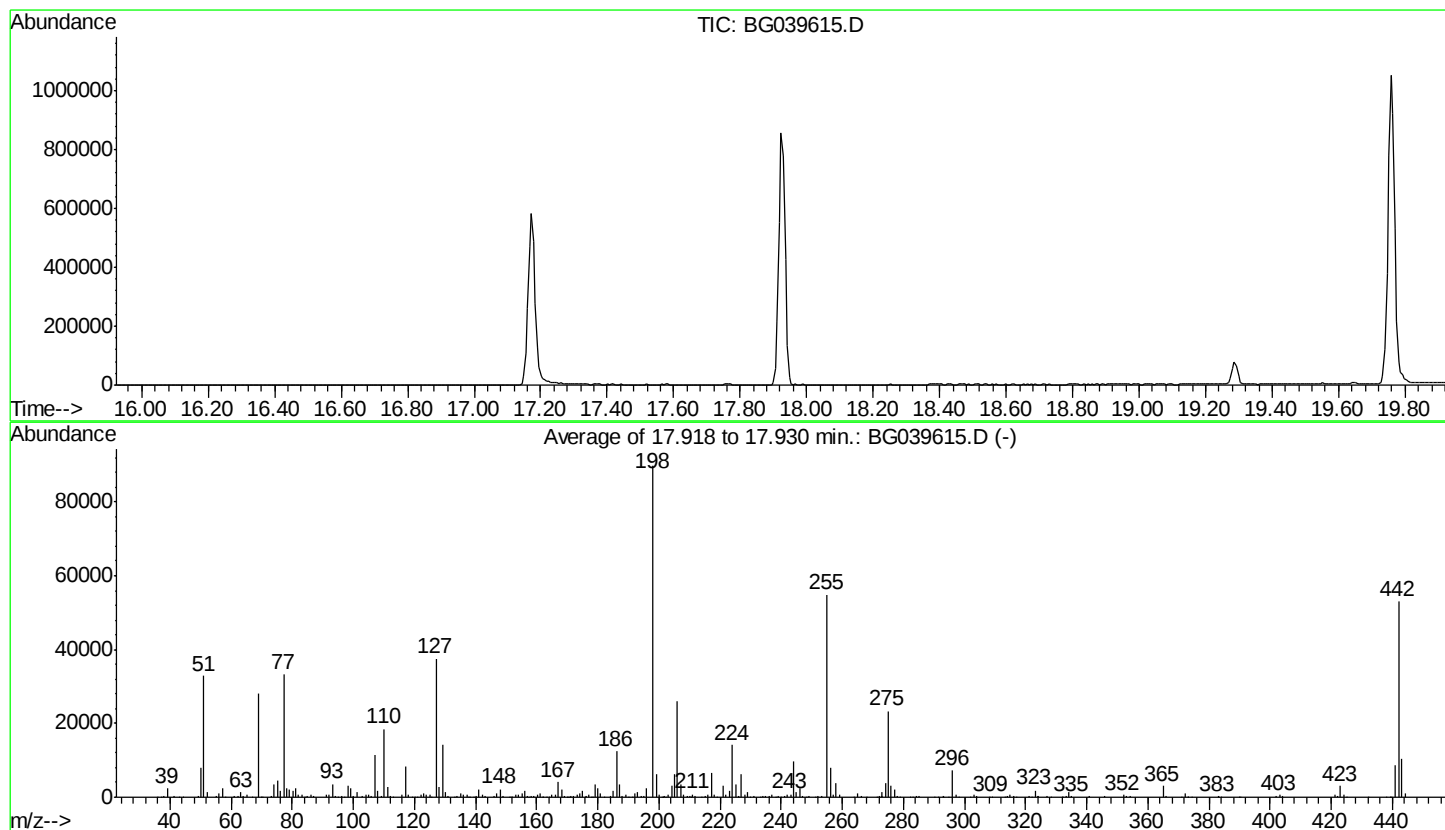

AutoFind: Scans 2524, 2525, 2526; Background Corrected with Scan 2518

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	32853	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	31.4	28186	PASS
70	69	0.00	2	0.4	107	PASS
127	198	10	80	41.8	37578	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	89818	PASS
199	198	5	9	7.0	6307	PASS
275	198	10	60	25.9	23293	PASS
365	198	1	100	3.4	3033	PASS
441	198	0.01	100	9.6	8615	PASS
442	198	50	100	58.9	52898	PASS
443	442	15	24	19.8	10470	PASS